

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061423\
 Data File : VW026182.D
 Acq On : 14 Jun 2023 16:51
 Operator : SY/MD
 Sample : 03234-02
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBTX0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/15/2023
 Supervised By :Mahesh Dadoda 06/15/2023

Quant Time: Jun 14 23:26:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 14 23:24:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	777016	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	685299	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	279561	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	187322	17.137	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	68.560%		
7) Chloroethane-d5	2.893	69	170065	20.783	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.120%		
11) 1,1-Dichloroethene-d2	4.027	65	95430	17.705	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	70.840%		
21) 2-Butanone-d5	7.075	46	199941	62.827	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	125.660%		
24) Chloroform-d	7.648	84	456957	20.083	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.320%		
26) 1,2-Dichloroethane-d4	8.307	65	287310m	23.092	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.360%		
32) Benzene-d6	8.276	84	909262	19.718	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	78.880%		
36) 1,2-Dichloropropane-d6	9.270	67	310435	21.250	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.000%		
41) Toluene-d8	10.325	98	750446	18.351	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.400%		
43) trans-1,3-Dichloroprop...	10.575	79	113566	19.617	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.480%		
47) 2-Hexanone-d5	10.922	63	126043	54.717	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.440%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	275512	25.916	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.680%		
66) 1,2-Dichlorobenzene-d4	13.848	152	225520	21.076	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.320%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.769	75	6197	0.990	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061423\
Data File : VW026182.D
Acq On : 14 Jun 2023 16:51
Operator : SY/MD
Sample : 03234-02
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
YBTX0

Quant Time: Jun 14 23:26:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 14 23:24:58 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/15/2023
Supervised By :Mahesh Dadoda 06/15/2023

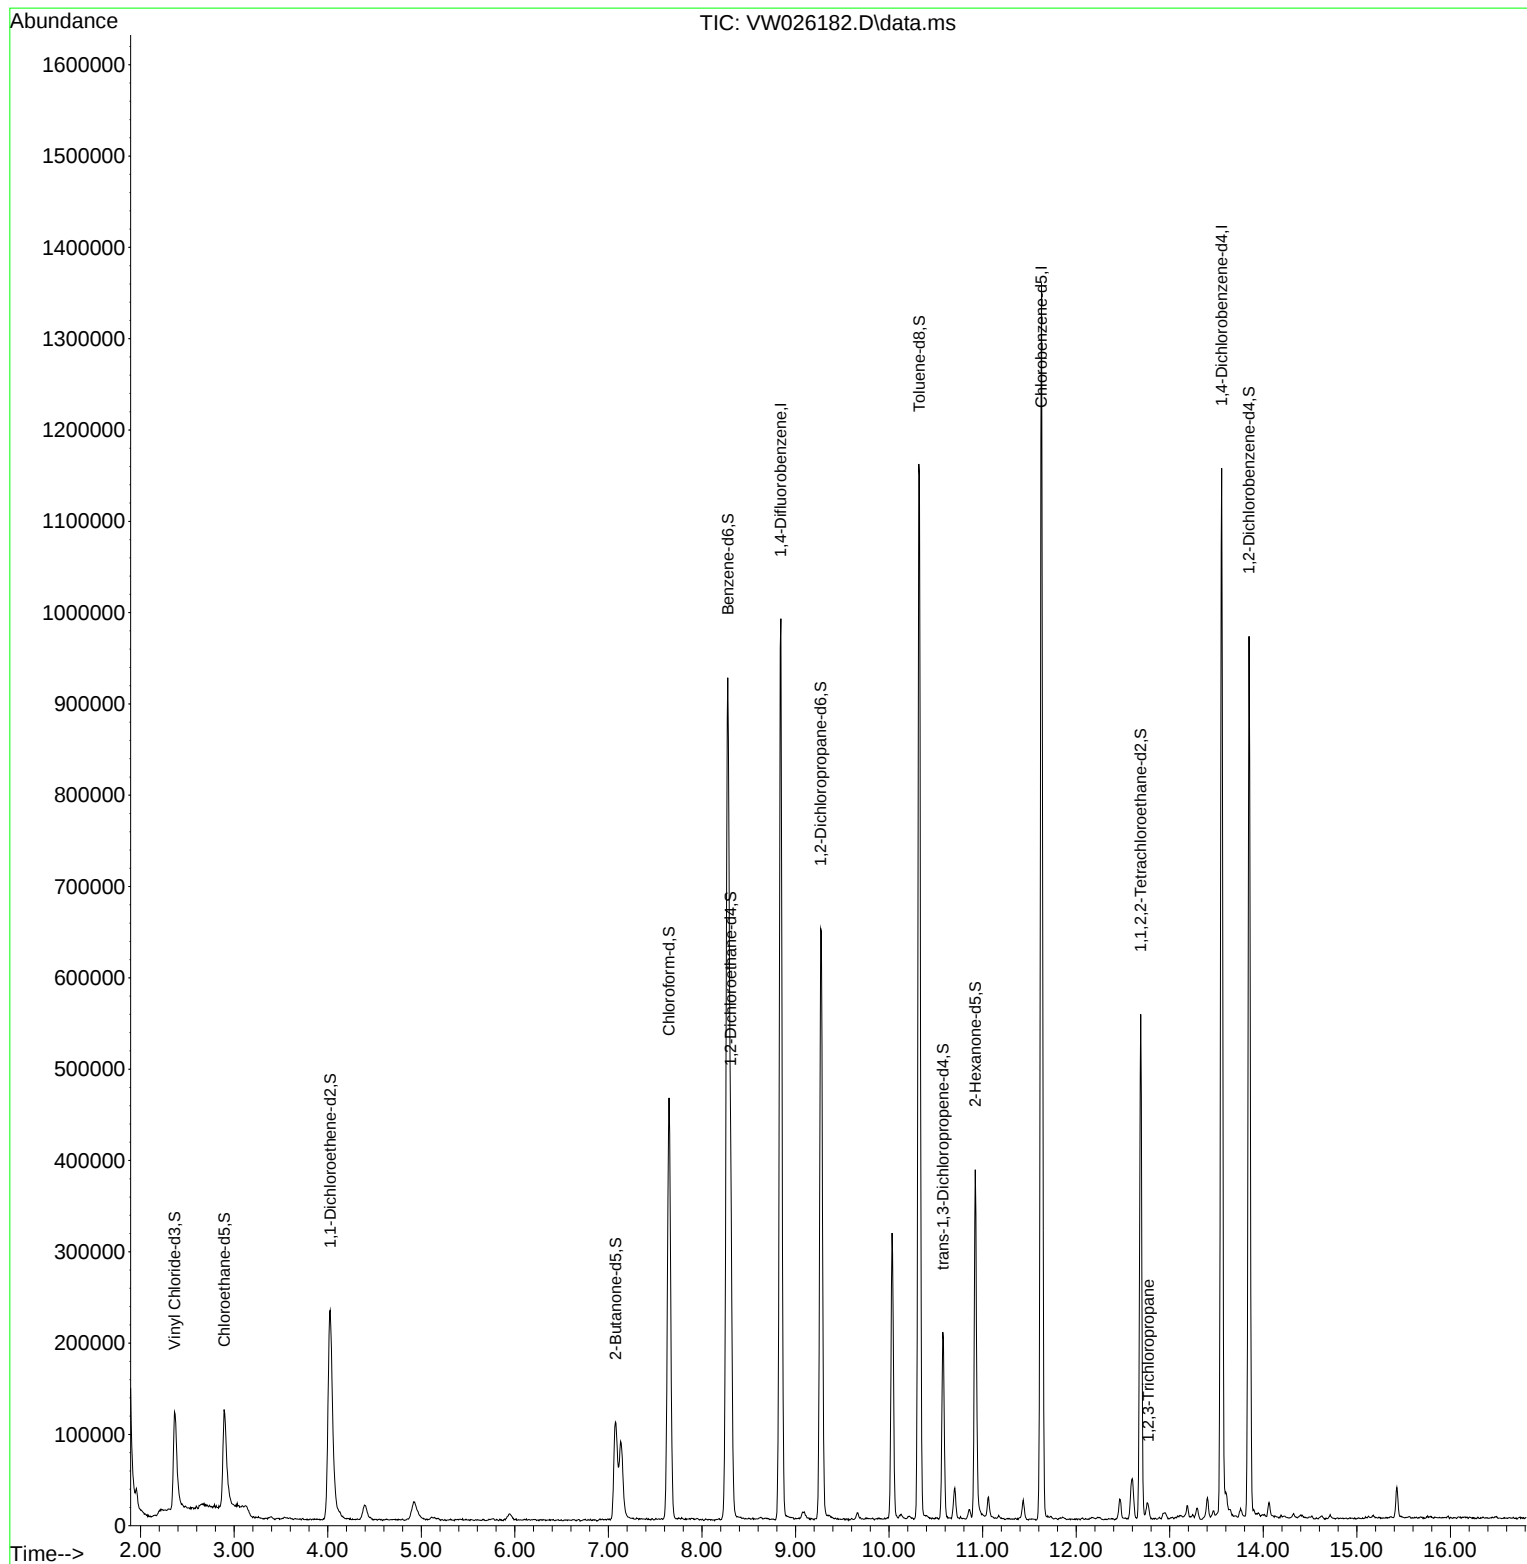

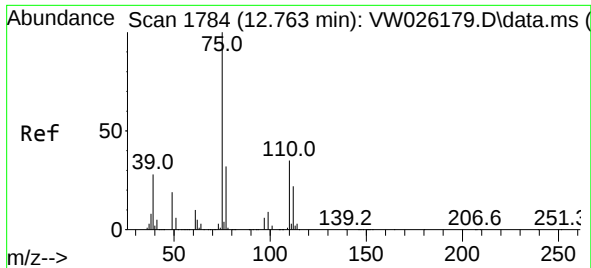

#61
 1,2,3-Trichloropropane
 Concen: 0.990 ug/L
 RT: 12.769 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VW026182.D
 Acq: 14 Jun 2023 16:51

Instrument :
 MSVOA_W
 ClientSampleId :
 YBTX0

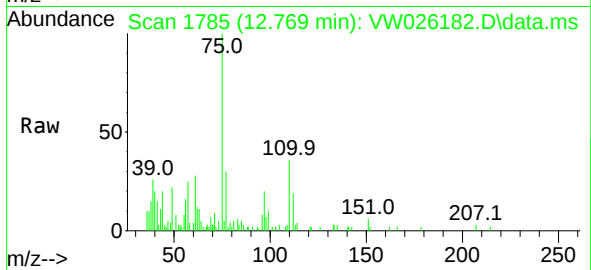

Tgt Ion: 75 Resp: 619

Ion	Ratio	Lower	Upper
75	100		
77	30.9	25.2	37.8
110	36.3	28.7	43.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/15/2023
 Supervised By :Mahesh Dadoda 06/15/2023

