

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061423\
 Data File : VW026188.D
 Acq On : 14 Jun 2023 19:15
 Operator : SY/MD
 Sample : 03234-11
 Misc : 5.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBTX7

Quant Time: Jun 14 23:27:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 14 23:24:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	844456	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	692126	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	229746	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	219220	18.453	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.800%
7) Chloroethane-d5	2.893	69	205783	23.140	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.560%
11) 1,1-Dichloroethene-d2	4.021	65	115582	19.731	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.920%
21) 2-Butanone-d5	7.075	46	184890	53.458	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.920%
24) Chloroform-d	7.648	84	543983	21.998	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	8.307	65	304774	22.539	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.160%
32) Benzene-d6	8.276	84	1074185	23.065	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.240%
36) 1,2-Dichloropropane-d6	9.276	67	362470	24.567	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.280%
41) Toluene-d8	10.319	98	867632	21.007	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.040%
43) trans-1,3-Dichloroprop...	10.575	79	104930	17.947	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.800%
47) 2-Hexanone-d5	10.922	63	112674	48.431	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.860%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	259563	24.175	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	195985	22.287	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.160%
Target Compounds						
13) Acetone	4.125	43	11856	4.430	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061423\
Data File : VW026188.D
Acq On : 14 Jun 2023 19:15
Operator : SY/MD
Sample : 03234-11
Misc : 5.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBTX7

Quant Time: Jun 14 23:27:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 14 23:24:58 2023
Response via : Initial Calibration

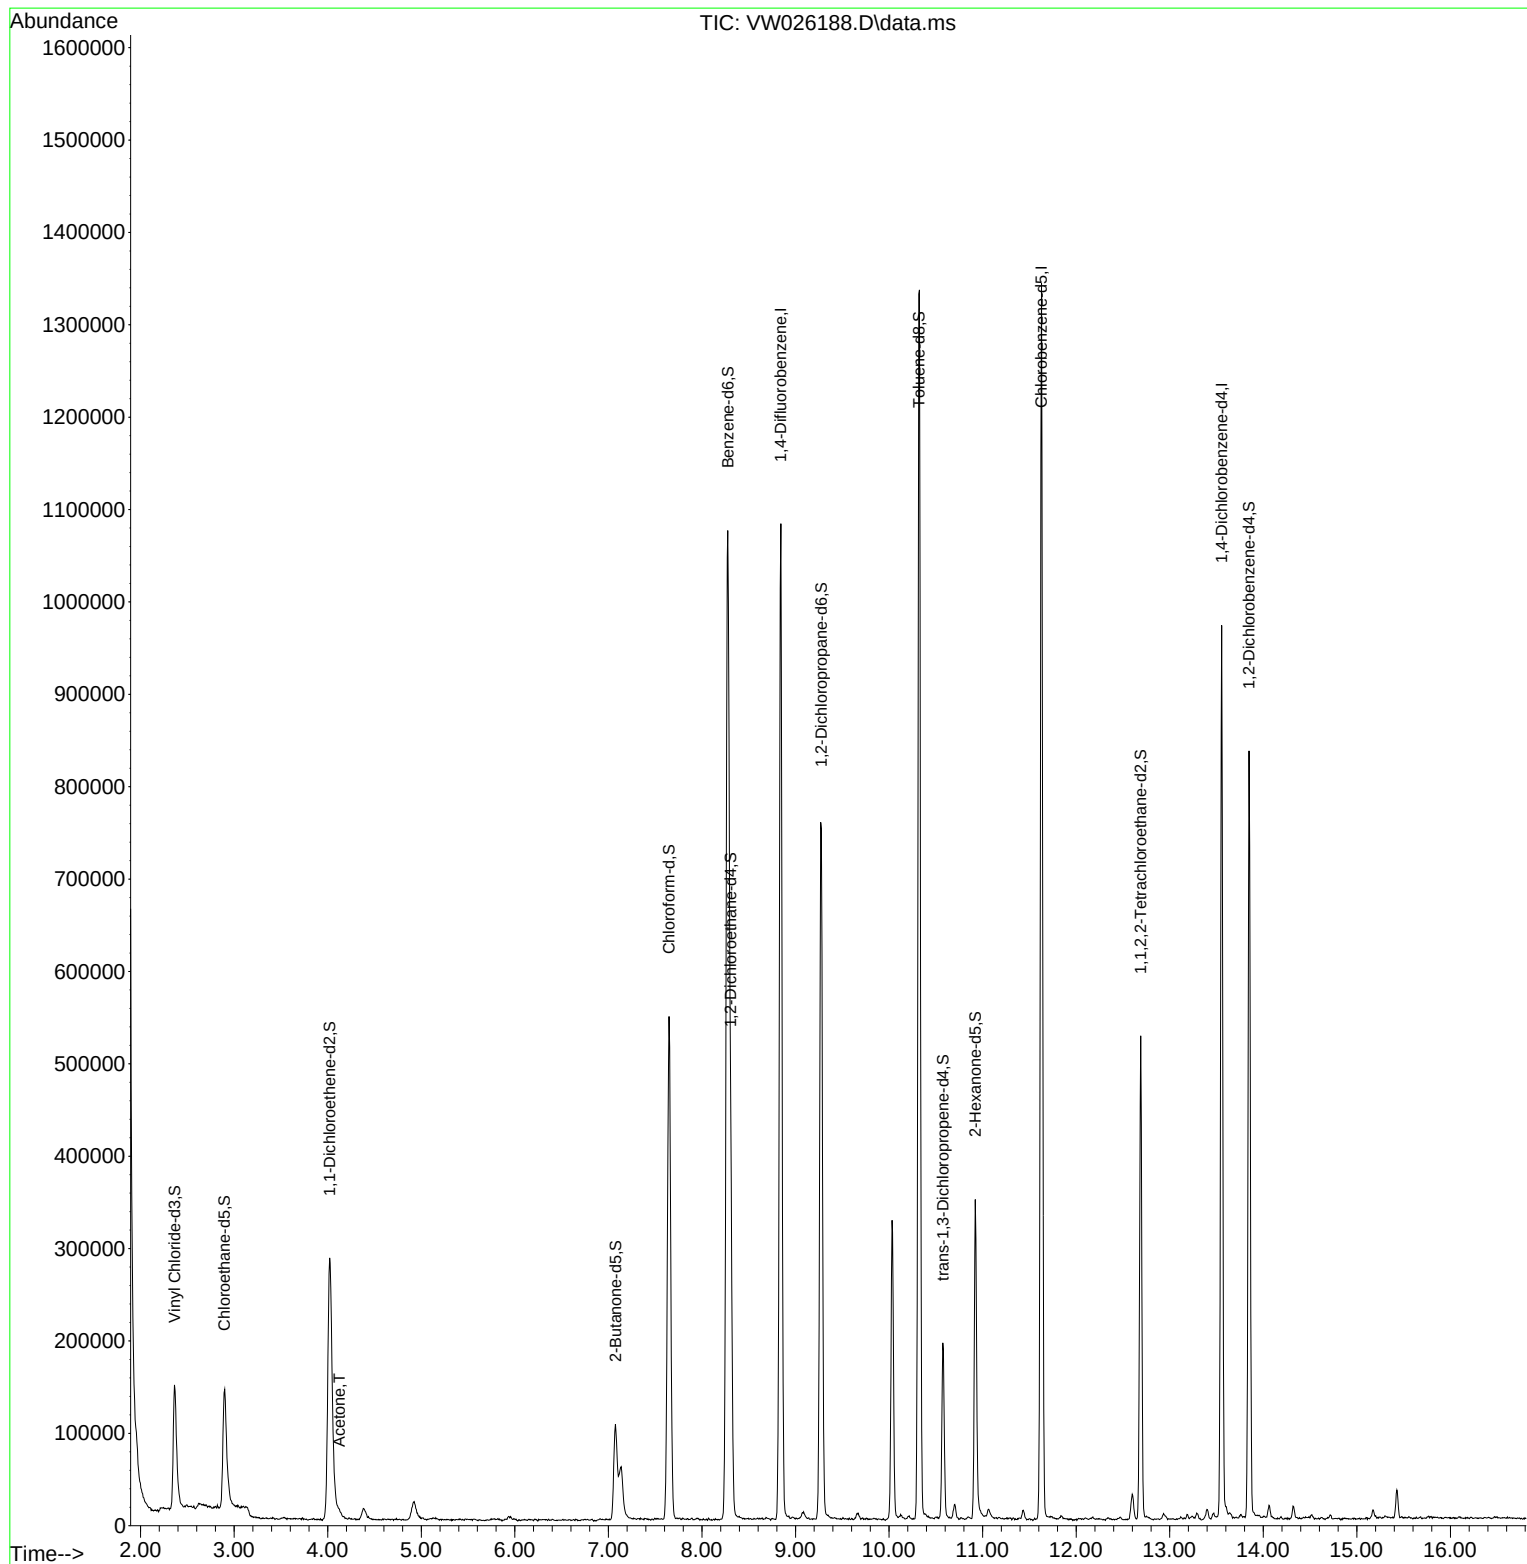

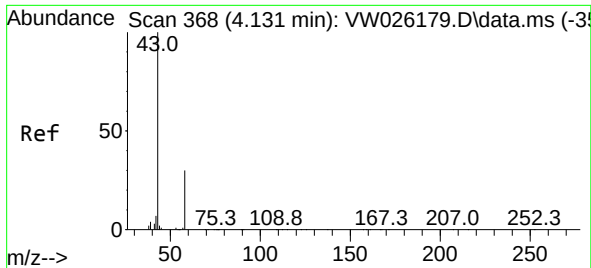

#13
 Acetone
 Concen: 4.430 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW026188.D
 Acq: 14 Jun 2023 19:15

Instrument :
 MSVOA_W
 ClientSampleId :
 YBTX7

Tgt Ion: 43 Resp: 11856
 Ion Ratio Lower Upper
 43 100
 58 31.5 0.0 58.2

