

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061424\
 Data File : VW029147.D
 Acq On : 14 Jun 2024 09:51
 Operator : SY/MD
 Sample : VW0614SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 15 00:20:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 15 00:20:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	248413	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	237208	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	106157	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	79781	20.216	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.880%
7) Chloroethane-d5	2.899	69	68260	22.525	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.080%
11) 1,1-Dichloroethene-d2	4.021	65	36746	21.185	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.760%
21) 2-Butanone-d5	7.075	46	48397	60.023	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.040%
24) Chloroform-d	7.648	84	169861	23.968	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.880%
26) 1,2-Dichloroethane-d4	8.307	65	98957	26.522	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.080%
32) Benzene-d6	8.270	84	321188	22.061	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.240%
36) 1,2-Dichloropropane-d6	9.270	67	105215	23.835	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.320%
41) Toluene-d8	10.318	98	282540	21.747	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.000%
43) trans-1,3-Dichloroprop...	10.575	79	37318	22.001	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.000%
47) 2-Hexanone-d5	10.922	63	30930	53.096	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	81485	26.571	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	93045	24.700	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.800%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3515	0.626	ug/L #	69
48) 2-Hexanone	10.922	43	4693	3.186	ug/L #	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061424\
Data File : VW029147.D
Acq On : 14 Jun 2024 09:51
Operator : SY/MD
Sample : VW0614SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 15 00:20:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 15 00:20:11 2024
Response via : Initial Calibration

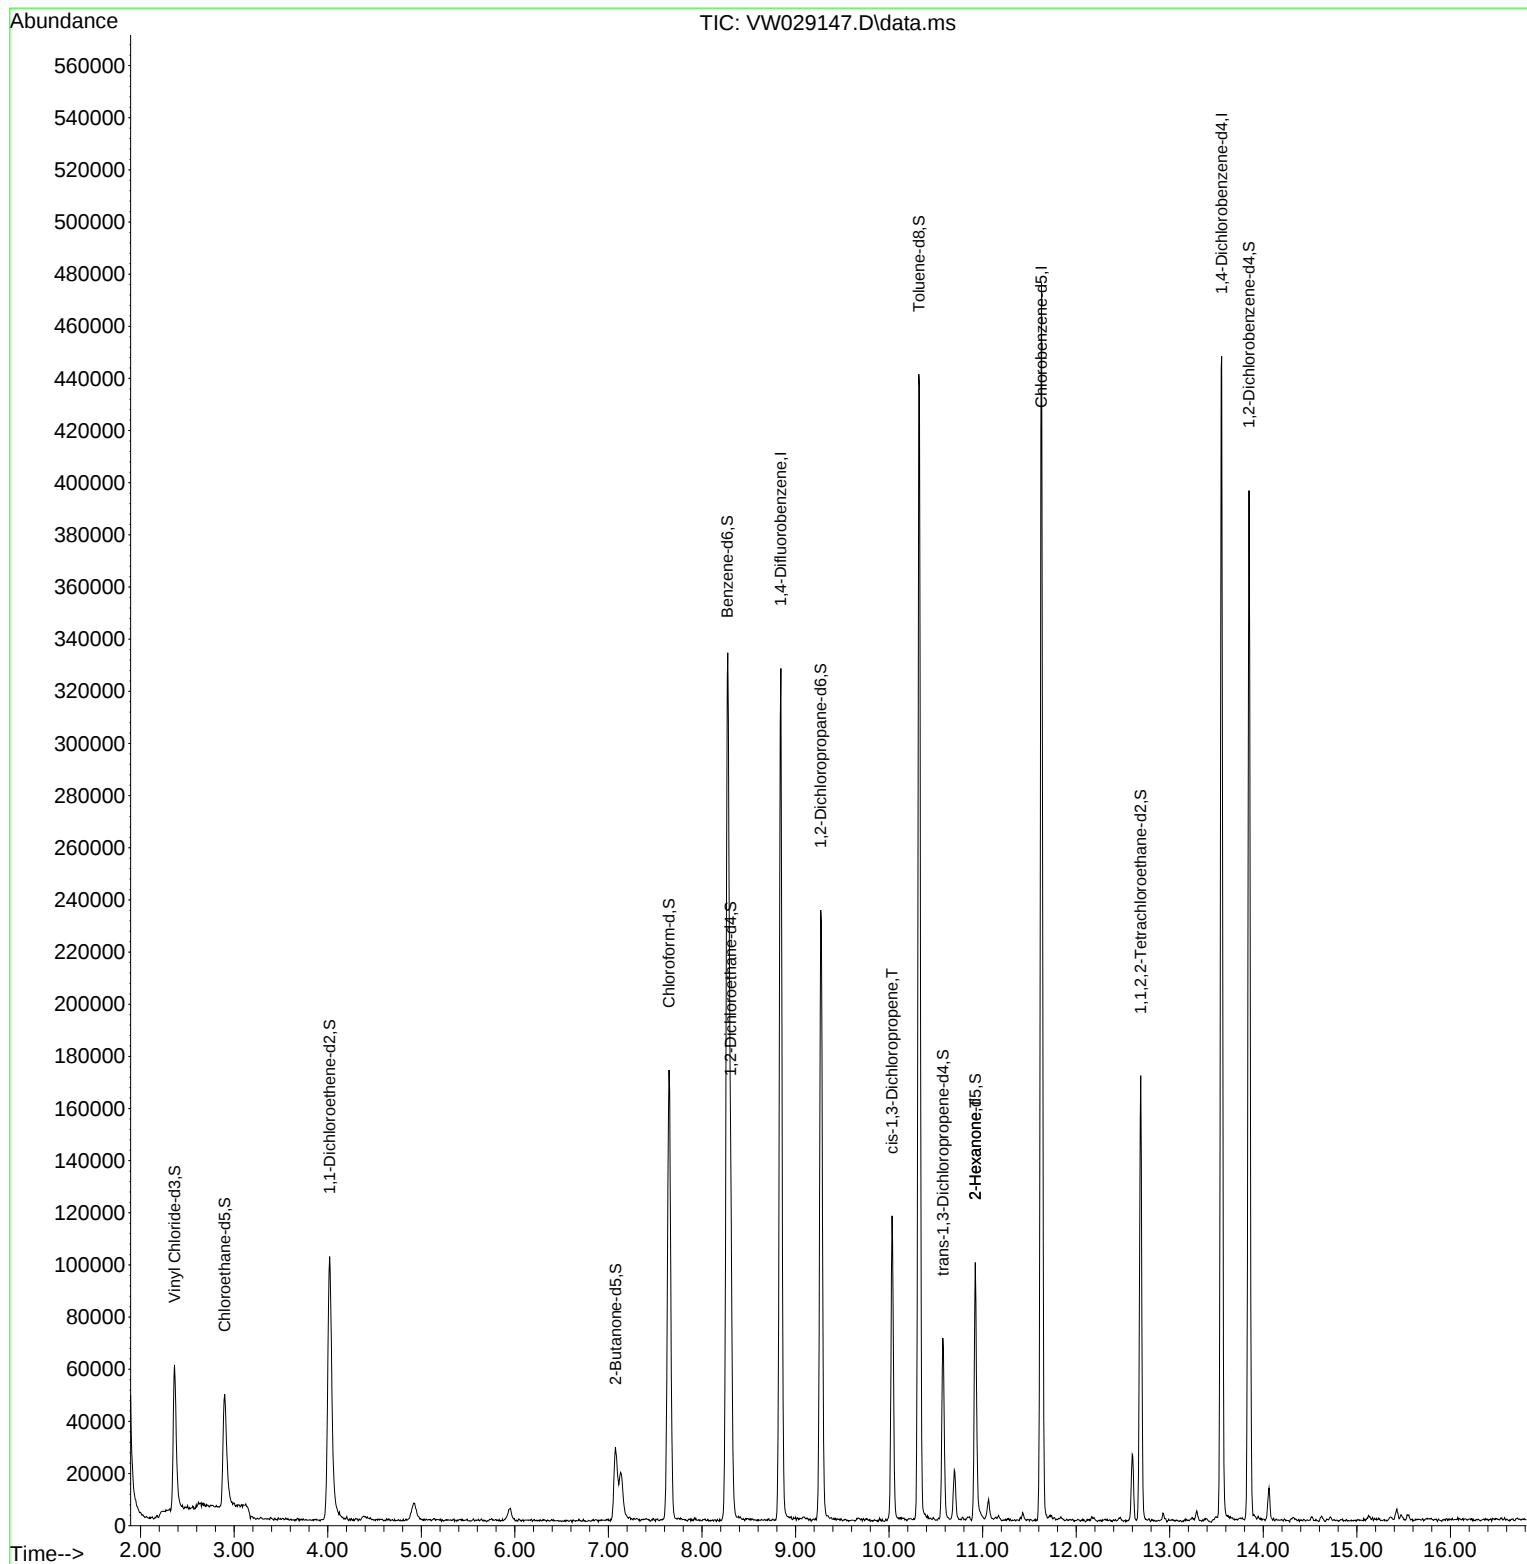

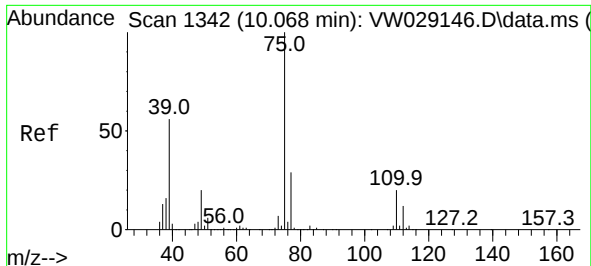

#39

cis-1,3-Dichloropropene

Concen: 0.626 ug/L

RT: 10.032 min Scan# 1482

Delta R.T. -0.036 min

Lab File: VW029147.D

Acq: 14 Jun 2024 09:51

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 3515

Ion Ratio Lower Upper

75 100

77 46.8 21.0 39.0#

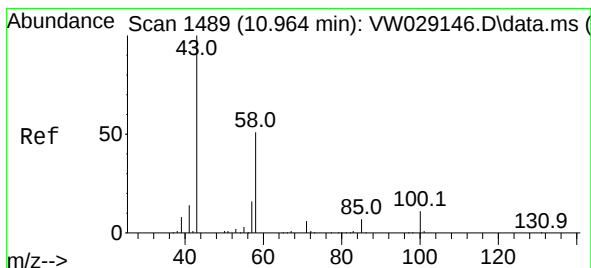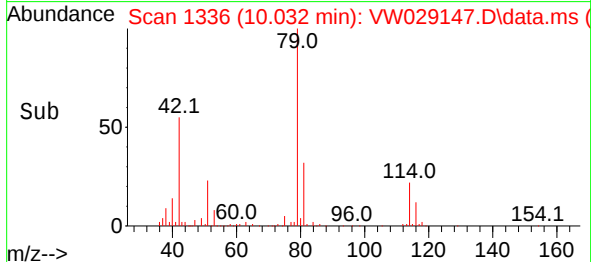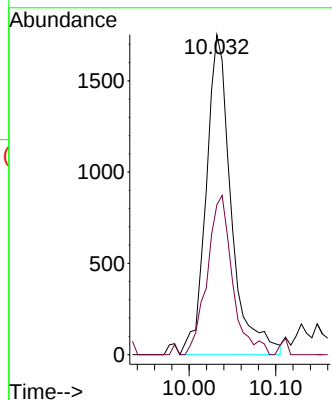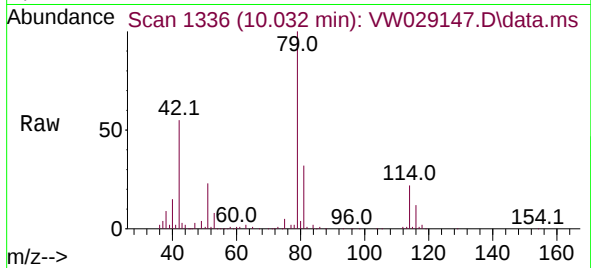

#48

2-Hexanone

Concen: 3.186 ug/L

RT: 10.922 min Scan# 1482

Delta R.T. -0.042 min

Lab File: VW029147.D

Acq: 14 Jun 2024 09:51

Tgt Ion: 43 Resp: 4693

Ion Ratio Lower Upper

43 100

58 18.5 41.4 62.0#

57 33.1 14.2 21.4#

100 2.0 9.1 13.7#

