

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
 Data File : VW029176.D
 Acq On : 18 Jun 2024 14:21
 Operator : SY/MD
 Sample : P2871-18
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 19 01:48:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 19 01:46:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	271798	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	253022	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	112991	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	69900	18.581	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.320%
7) Chloroethane-d5	2.893	69	58171	18.311	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.240%
11) 1,1-Dichloroethene-d2	4.015	65	33220	18.289	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.160%
21) 2-Butanone-d5	7.081	46	40124	35.649	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.300%
24) Chloroform-d	7.648	84	150244	18.531	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.120%
26) 1,2-Dichloroethane-d4	8.307	65	88161	18.939	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	75.760%
32) Benzene-d6	8.276	84	291043	18.938	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.760%
36) 1,2-Dichloropropane-d6	9.270	67	92413	18.916	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.680%
41) Toluene-d8	10.325	98	260893	19.187	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.760%
43) trans-1,3-Dichloroprop...	10.575	79	36447	18.513	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.040%
47) 2-Hexanone-d5	10.922	63	26620	34.759	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.520%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	69504	17.876	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	71.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	79541	20.281	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.120%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3050	0.505	ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
Data File : VW029176.D
Acq On : 18 Jun 2024 14:21
Operator : SY/MD
Sample : P2871-18
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 19 01:48:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 19 01:46:42 2024
Response via : Initial Calibration

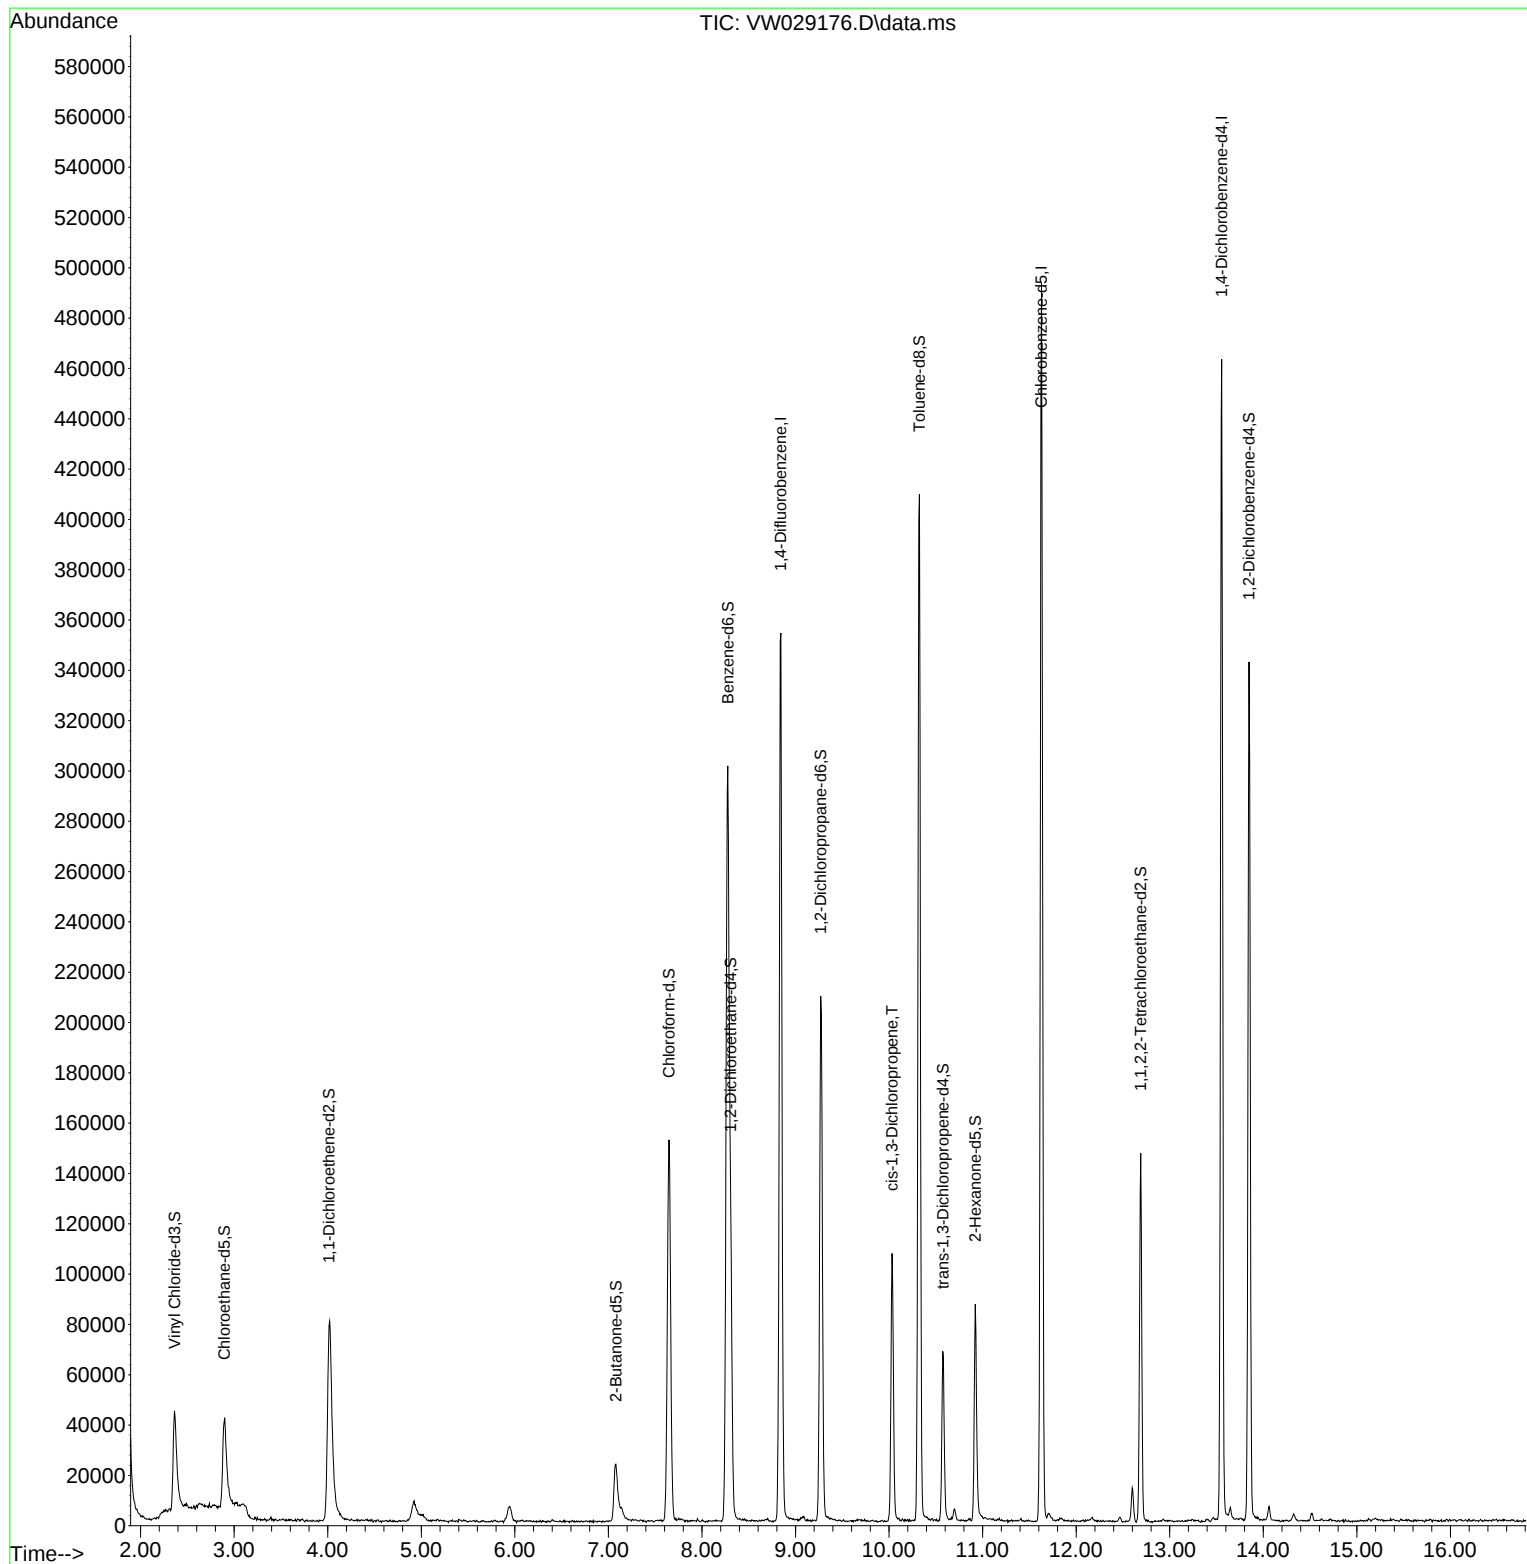

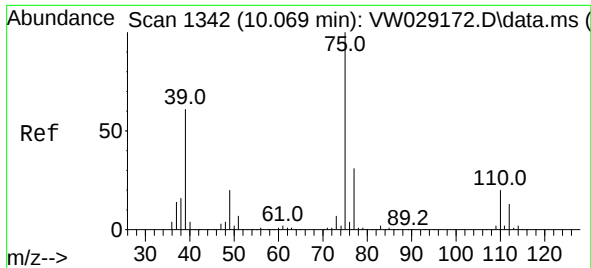

#39
 cis-1,3-Dichloropropene
 Concen: 0.505 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029176.D
 Acq: 18 Jun 2024 14:21

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3050
 Ion Ratio Lower Upper
 75 100
 77 55.4 22.7 42.1#

