
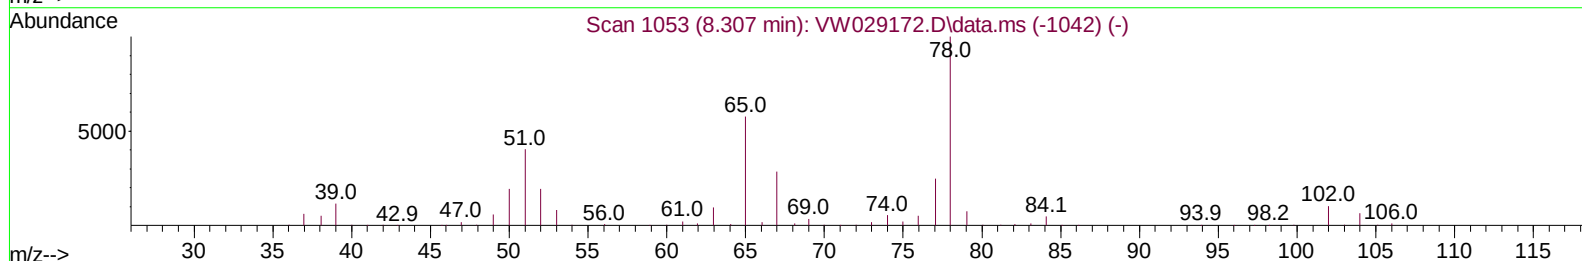
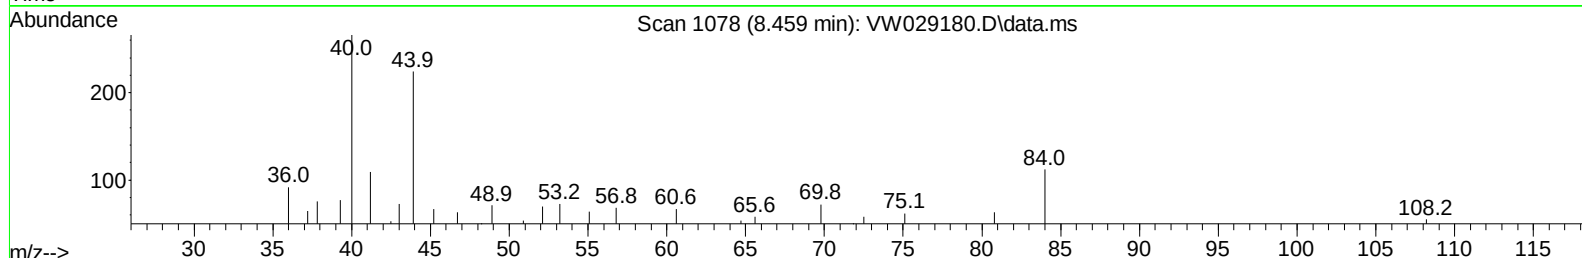


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
Data File : VW029180.D
Acq On : 18 Jun 2024 16:00
Operator : SY/MD
Sample : P2871-11RE
Misc : 5.04g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 19 01:46:42 2024
Response via : Initial Calibration

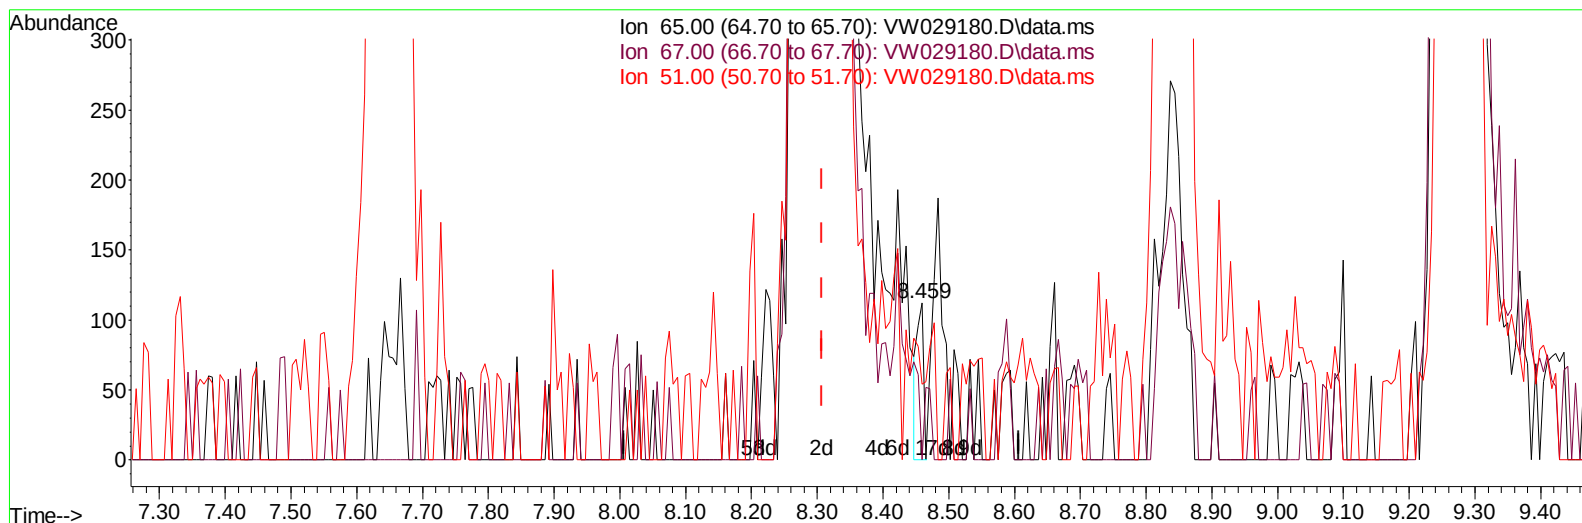

TIC: VW029180.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.459min (+ 0.153) 0.02 ug/L

response 76

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	50.00
51.00	99.20	106.58
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
Data File : VW029180.D
Acq On : 18 Jun 2024 16:00
Operator : SY/MD
Sample : P2871-11RE
Misc : 5.04g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 19 01:46:42 2024
Response via : Initial Calibration

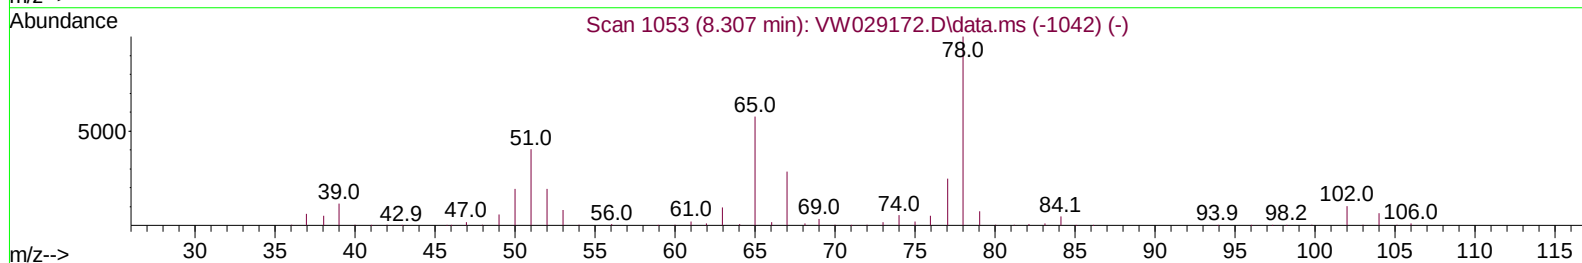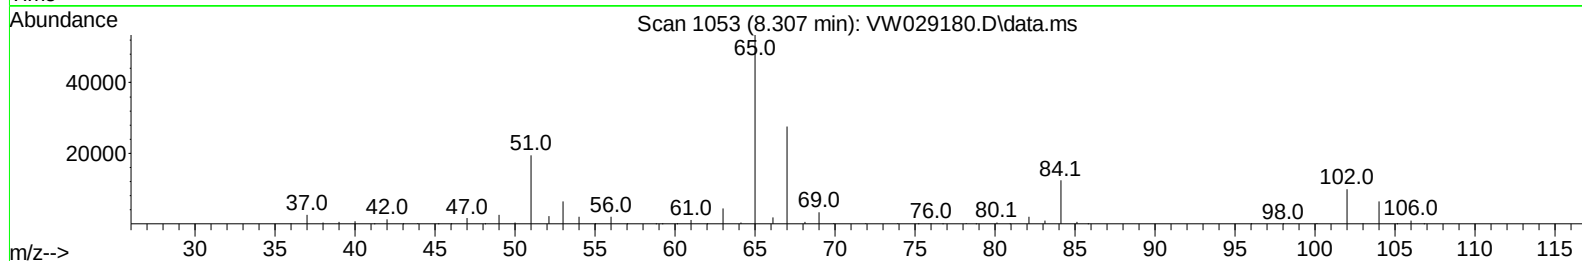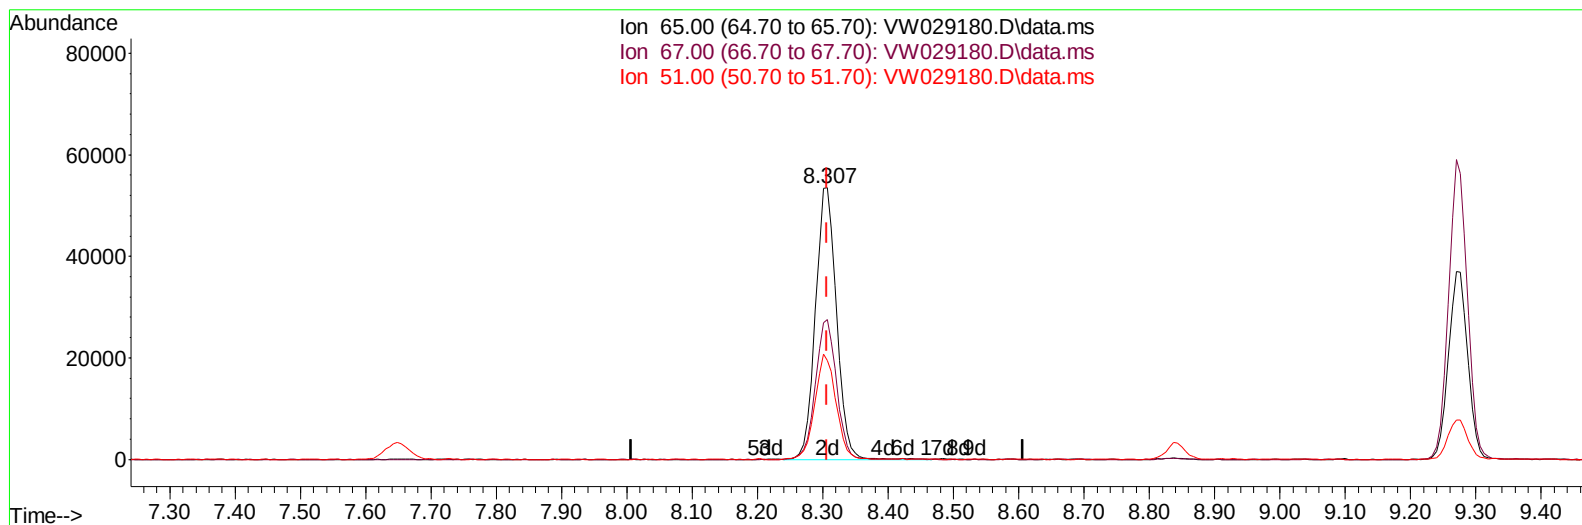

TIC: VW029180.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.000) 26.22 ug/L m****response 120005**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	0.03#
51.00	99.20	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
 Data File : VW029180.D
 Acq On : 18 Jun 2024 16:00
 Operator : SY/MD
 Sample : P2871-11RE
 Misc : 5.04g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 19 01:46:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	267192	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	195109	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	48782	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	85600	23.146	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.600%	
7) Chloroethane-d5	2.899	69	78074	24.999	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	100.000%	
11) 1,1-Dichloroethene-d2	4.021	65	36603	20.499	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	82.000%	
21) 2-Butanone-d5	7.075	46	50863	45.969	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.940%	
24) Chloroform-d	7.648	84	189254	23.744	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.960%	
26) 1,2-Dichloroethane-d4	8.307	65	120005m	26.224	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	104.880%	
32) Benzene-d6	8.270	84	333657	28.154	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	112.600%	
36) 1,2-Dichloropropane-d6	9.270	67	116869	31.023	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	124.080%#	
41) Toluene-d8	10.319	98	248434	23.694	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.760%	
43) trans-1,3-Dichloroprop...	10.575	79	32781	21.594	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	86.360%	
47) 2-Hexanone-d5	10.922	63	33434	56.615	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	113.240%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	80250	26.766	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	107.080%	
66) 1,2-Dichlorobenzene-d4	13.849	152	39189	23.144	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.560%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
Data File : VW029180.D
Acq On : 18 Jun 2024 16:00
Operator : SY/MD
Sample : P2871-11RE
Misc : 5.04g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 19 01:46:42 2024
Response via : Initial Calibration

