
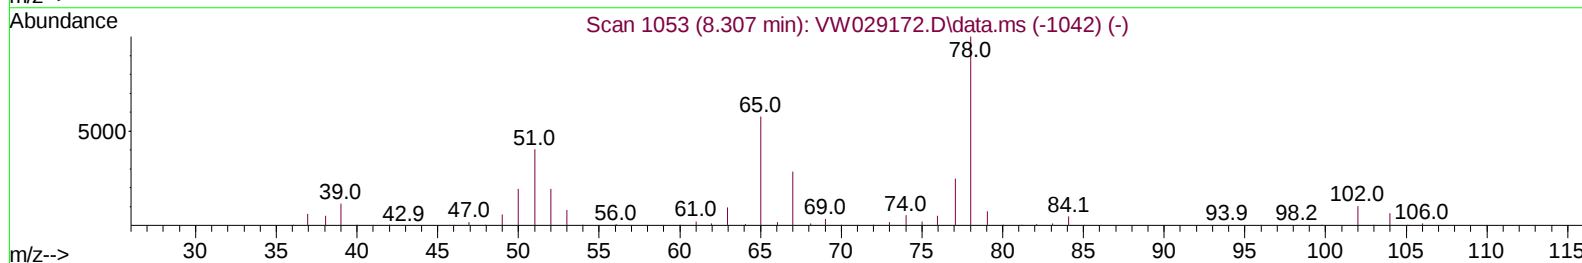
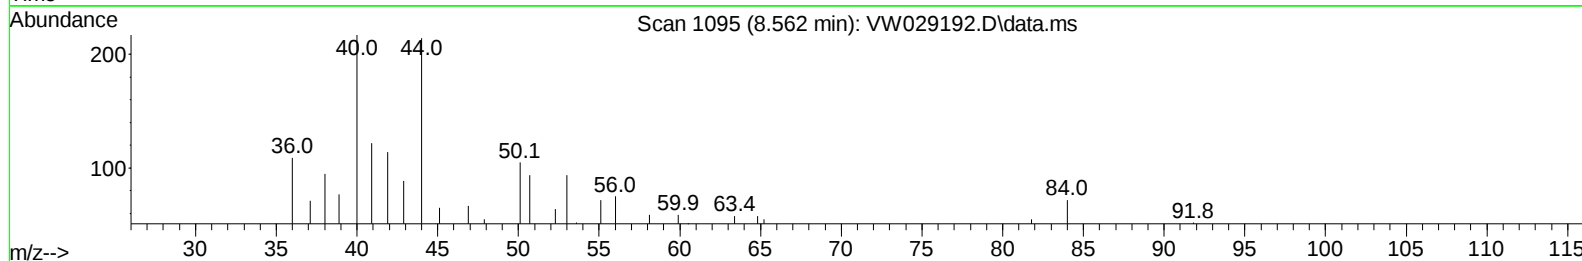


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
Data File : VW029192.D
Acq On : 18 Jun 2024 20:49
Operator : SY/MD
Sample : P2934-08
Misc : 5.58g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:52:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 19 01:46:42 2024
Response via : Initial Calibration

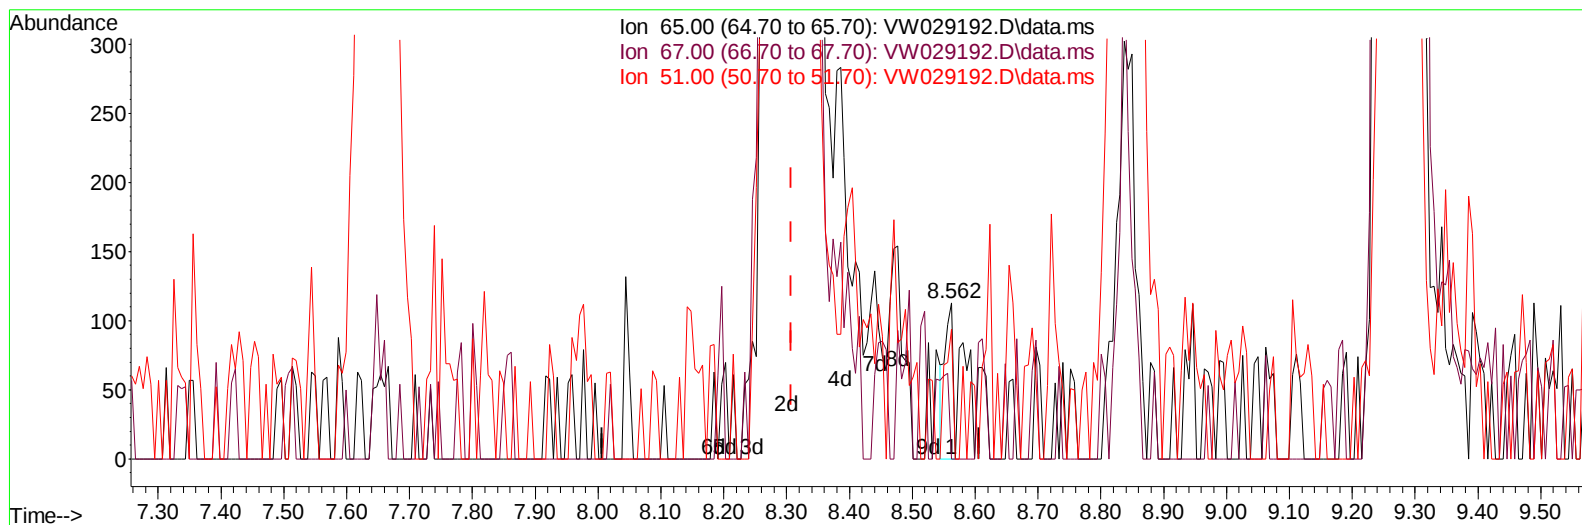

TIC: VW029192.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.562min (+ 0.256) 0.02 ug/L

response 102

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	44.12
51.00	99.20	83.33
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
 Data File : VW029192.D
 Acq On : 18 Jun 2024 20:49
 Operator : SY/MD
 Sample : P2934-08
 Misc : 5.58g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:52:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 19 01:46:42 2024
 Response via : Initial Calibration

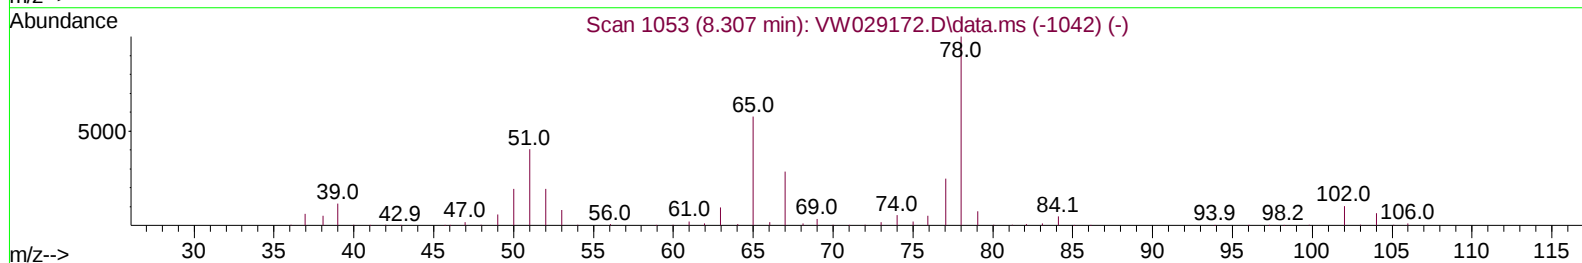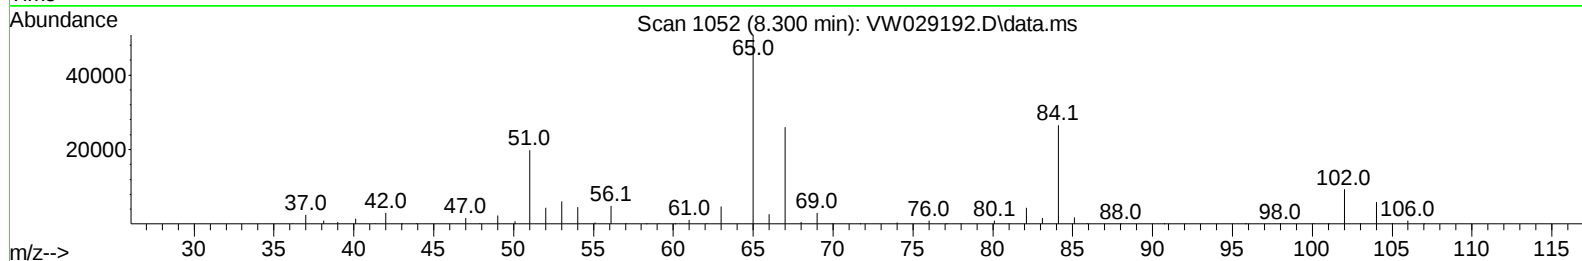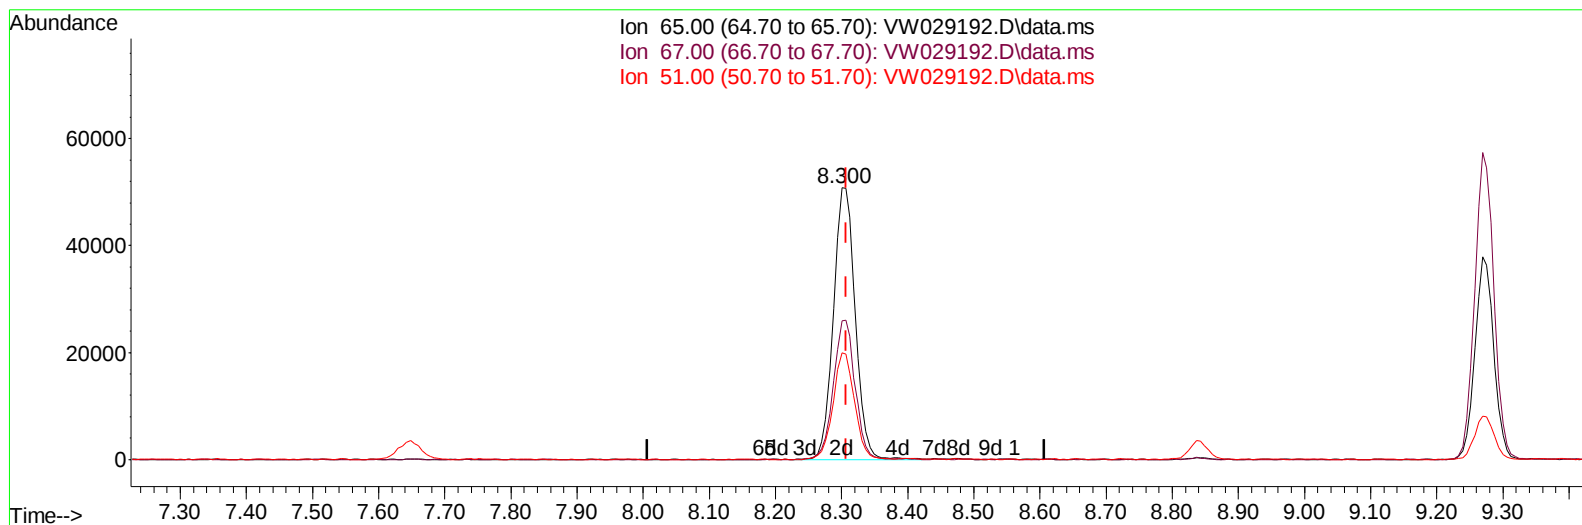

TIC: VW029192.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.300min (-0.006) 24.38 ug/L m****response 116525**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	0.04#
51.00	99.20	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
 Data File : VW029192.D
 Acq On : 18 Jun 2024 20:49
 Operator : SY/MD
 Sample : P2934-08
 Misc : 5.58g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:52:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 19 01:46:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	279083	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	195730	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	44277	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	83064	21.503	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.000%	
7) Chloroethane-d5	2.893	69	77157	23.653	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.600%	
11) 1,1-Dichloroethene-d2	4.021	65	36830	19.747	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	79.000%	
21) 2-Butanone-d5	7.075	46	42572	36.837	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	73.680%	
24) Chloroform-d	7.648	84	186839	22.443	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.760%	
26) 1,2-Dichloroethane-d4	8.300	65	116525m	24.378	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.520%	
32) Benzene-d6	8.276	84	333223	28.029	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	112.120%	
36) 1,2-Dichloropropane-d6	9.270	67	116060	30.711	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	122.840%#	
41) Toluene-d8	10.318	98	240778	22.891	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	91.560%	
43) trans-1,3-Dichloroprop...	10.580	79	27299	17.926	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.720%	
47) 2-Hexanone-d5	10.922	63	27281	46.050	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.100%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	77257	25.686	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.760%	
66) 1,2-Dichlorobenzene-d4	13.848	152	35431	23.054	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.200%	
Target Compounds						
					Qvalue	
13) Acetone	4.130	43	4621	4.705	ug/L	85
16) Methylene chloride	4.923	84	18707	3.812	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061824\
Data File : VW029192.D
Acq On : 18 Jun 2024 20:49
Operator : SY/MD
Sample : P2934-08
Misc : 5.58g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:52:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 19 01:46:42 2024
Response via : Initial Calibration

