




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061923\
 Data File : VW026252.D
 Acq On : 19 Jun 2023 17:07
 Operator : SY/MD
 Sample : 03307-16
 Misc : 5.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW34

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

Quant Time: Jun 20 03:18:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 23:58:43 2023
 Response via : Initial Calibration

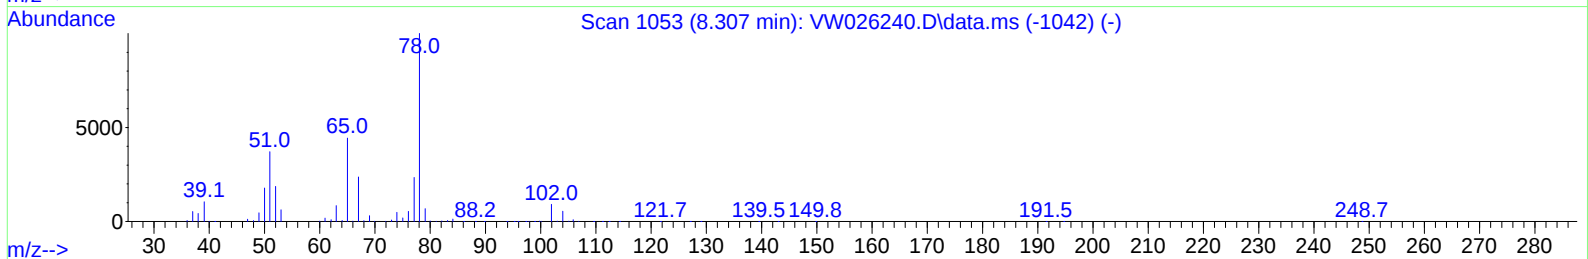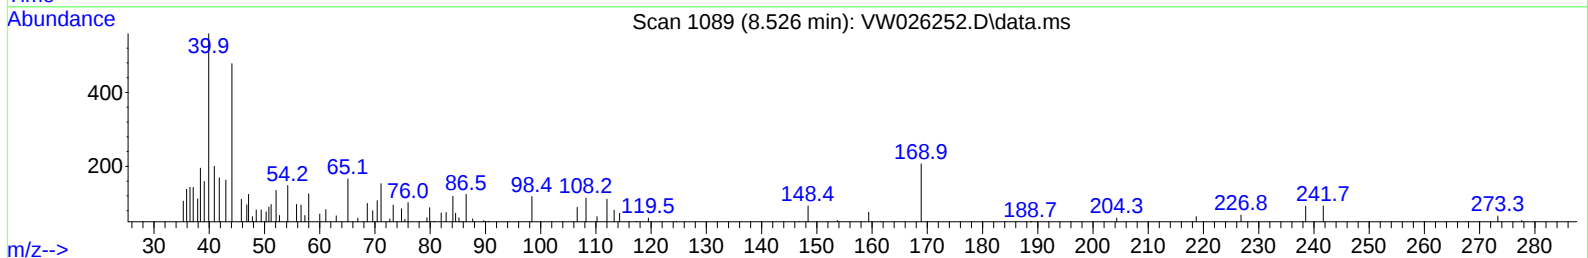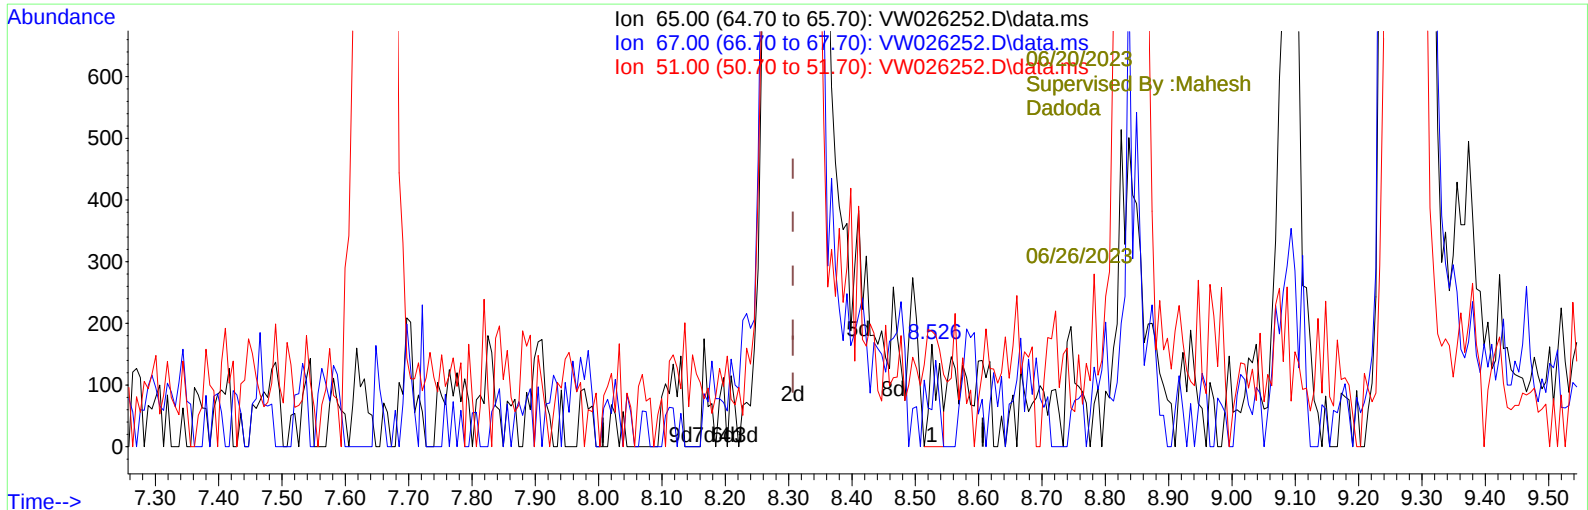

TIC: VW026252.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.526min (+ 0.219) 0.02 ug/L

response 178

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	43.82
51.00	106.50	119.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061923\
 Data File : VW026252.D
 Acq On : 19 Jun 2023 17:07
 Operator : SY/MD
 Sample : 03307-16
 Misc : 5.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW34

Manual IntegrationsAPPROVED

Quant Time: Jun 20 03:18:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 23:58:43 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

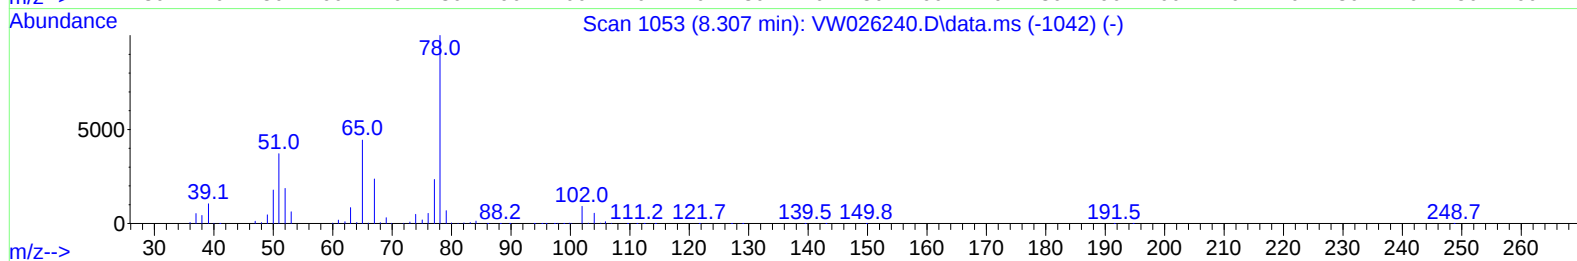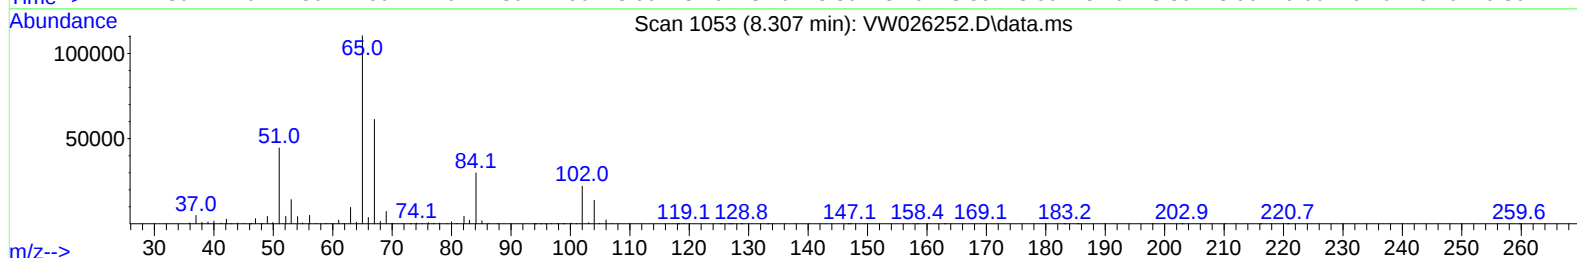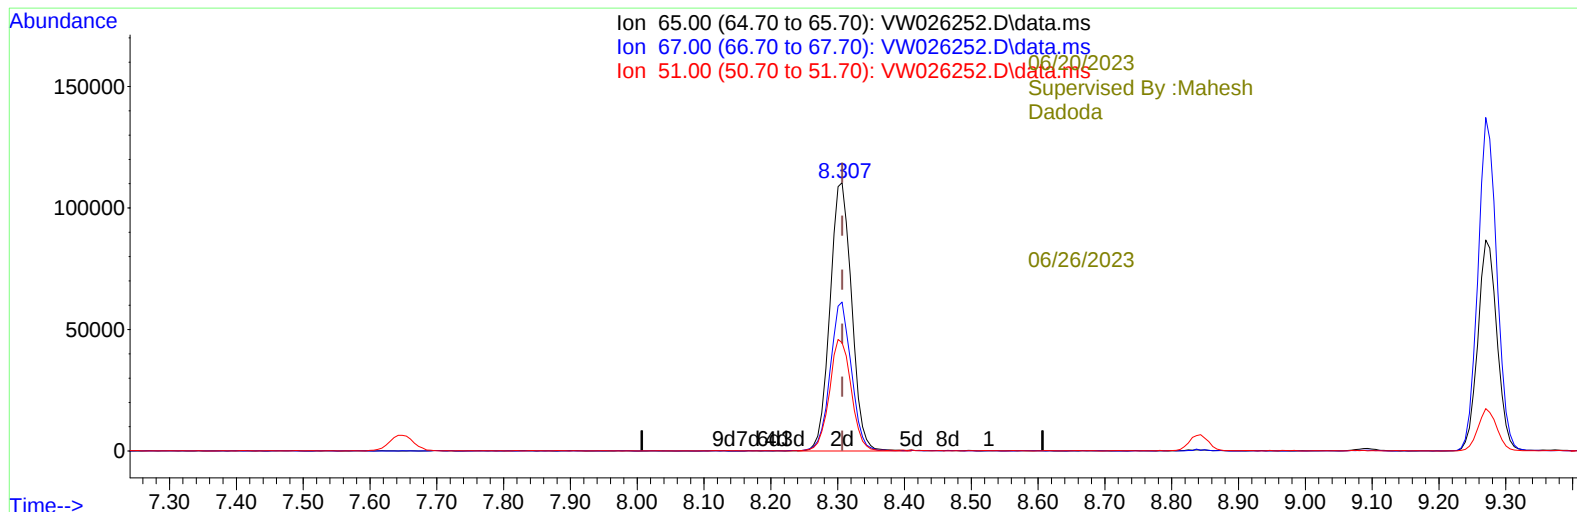

TIC: VW026252.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 25.74 ug/L m

response 249485

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.03#
51.00	106.50	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061923\
 Data File : VW026252.D
 Acq On : 19 Jun 2023 17:07
 Operator : SY/MD
 Sample : 03307-16
 Misc : 5.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW34

Manual IntegrationsAPPROVED

Quant Time: Jun 20 03:18:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 23:58:43 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	605274	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	530151	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	186416	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	147545	17.328	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	69.320%		
7) Chloroethane-d5	2.893	69	141449	22.191	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	88.760%		
11) 1,1-Dichloroethene-d2	4.027	65	78782	18.764	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	75.040%		
21) 2-Butanone-d5	7.075	46	217014	87.541	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	175.080%#		
24) Chloroform-d	7.648	84	400082	22.572	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	90.280%		
26) 1,2-Dichloroethane-d4	8.307	65	249485m	25.741	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	102.960%		
32) Benzene-d6	8.276	84	771880	21.638	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	86.560%		
36) 1,2-Dichloropropane-d6	9.270	67	269542	23.850	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	95.400%		
41) Toluene-d8	10.325	98	619412	19.579	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	78.320%		
43) trans-1,3-Dichloroprop...	10.581	79	93292	20.831	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	83.320%		
47) 2-Hexanone-d5	10.922	63	137097	76.933	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	153.860%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	267179	32.487	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	129.960%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	169264	23.722	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	94.880%		
Target Compounds						
					Qvalue	
13) Acetone	4.118	43	9239	4.817	ug/L	70
16) Methylene chloride	4.917	84	81675	8.454	ug/L	96
20) cis-1,2-Dichloroethene	7.173	96	218143	23.818	ug/L	96
34) Trichloroethene	9.093	95	100844	10.844	ug/L	95
46) Tetrachloroethene	10.861	164	11370	1.729	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061923\
Data File : VW026252.D
Acq On : 19 Jun 2023 17:07
Operator : SY/MD
Sample : 03307-16
Misc : 5.80g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBW34

Manual IntegrationsAPPROVED

Quant Time: Jun 20 03:18:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 23:58:43 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

