




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
Data File : VW029202.D
Acq On : 19 Jun 2024 10:09
Operator : SY/MD
Sample : P2844-03
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/20/2024
Supervised By :Mahesh Dadoda 06/20/2024

06/20/2024
Supervised By :Mahesh

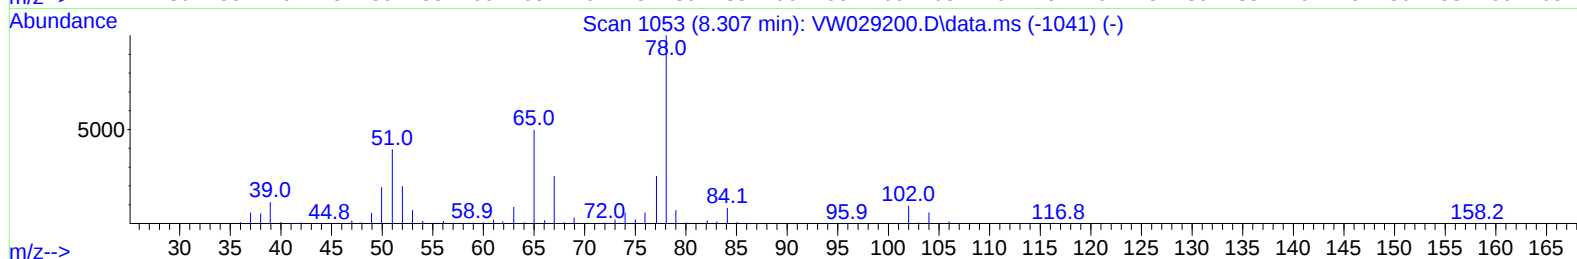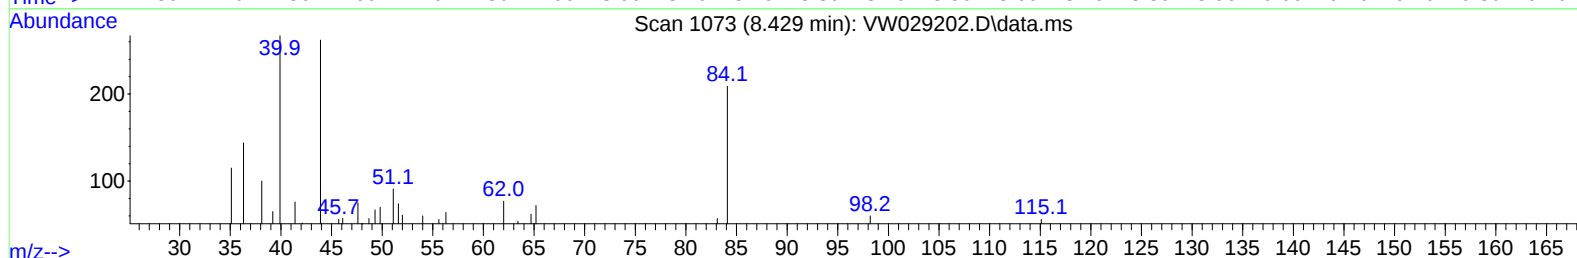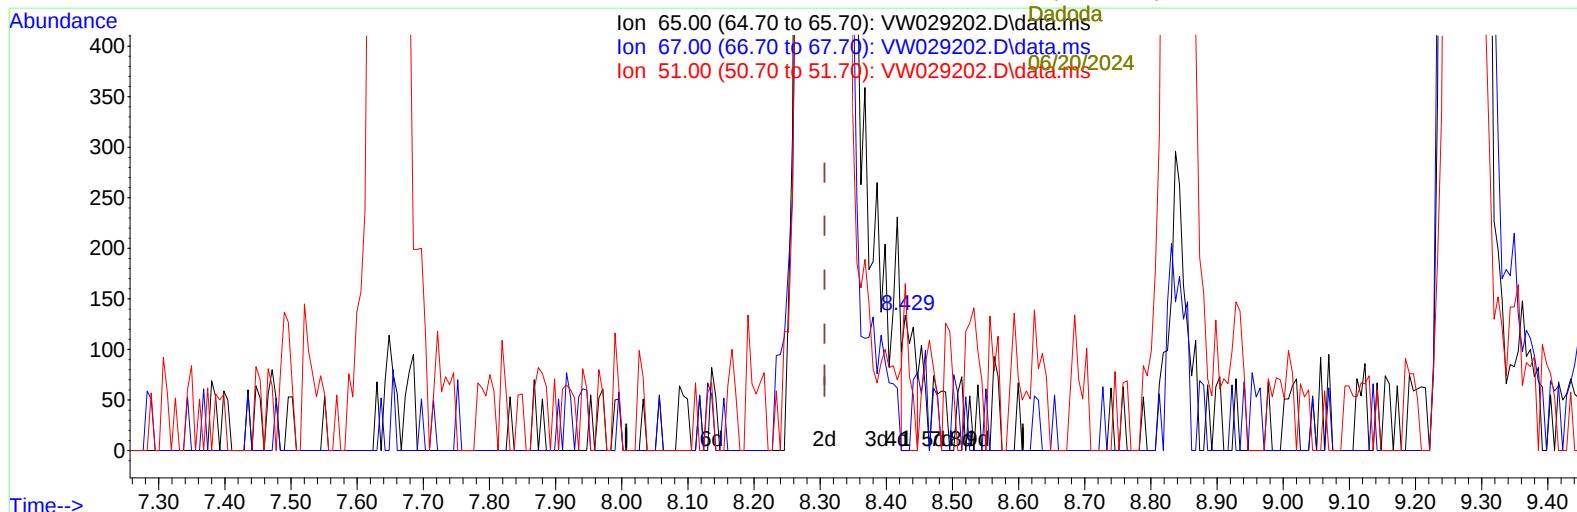

TIC: VW029202.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.429min (+ 0.122) 0.04 ug/L

response 158

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	46.84
51.00	99.20	86.71
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
Data File : VW029202.D
Acq On : 19 Jun 2024 10:09
Operator : SY/MD
Sample : P2844-03
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/20/2024
Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 20 01:54:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 20 00:39:34 2024
Response via : Initial Calibration

06/20/2024
Supervised By :Mahesh
Dadoda

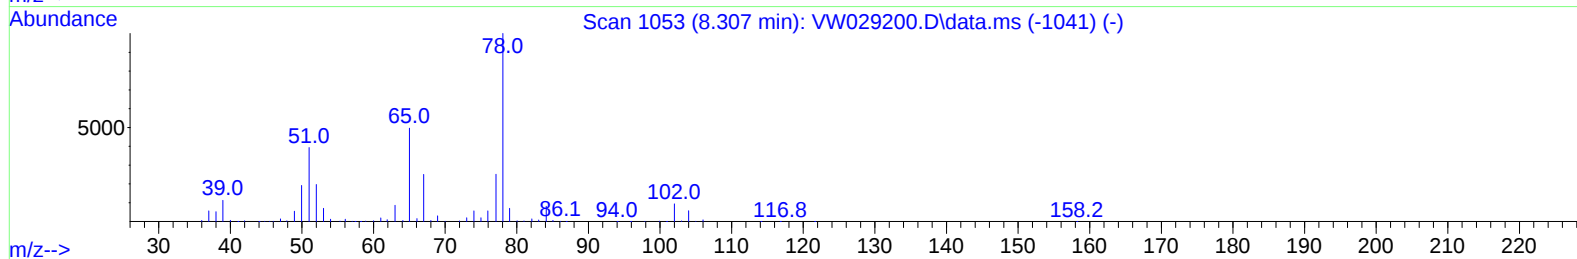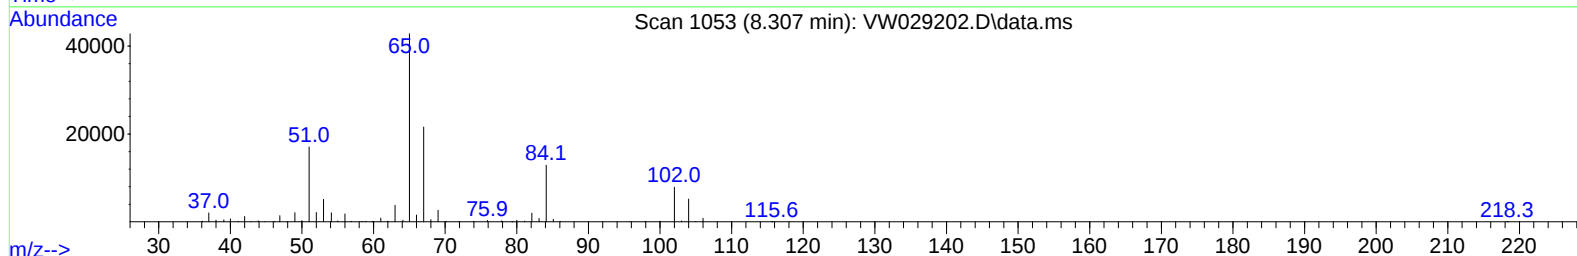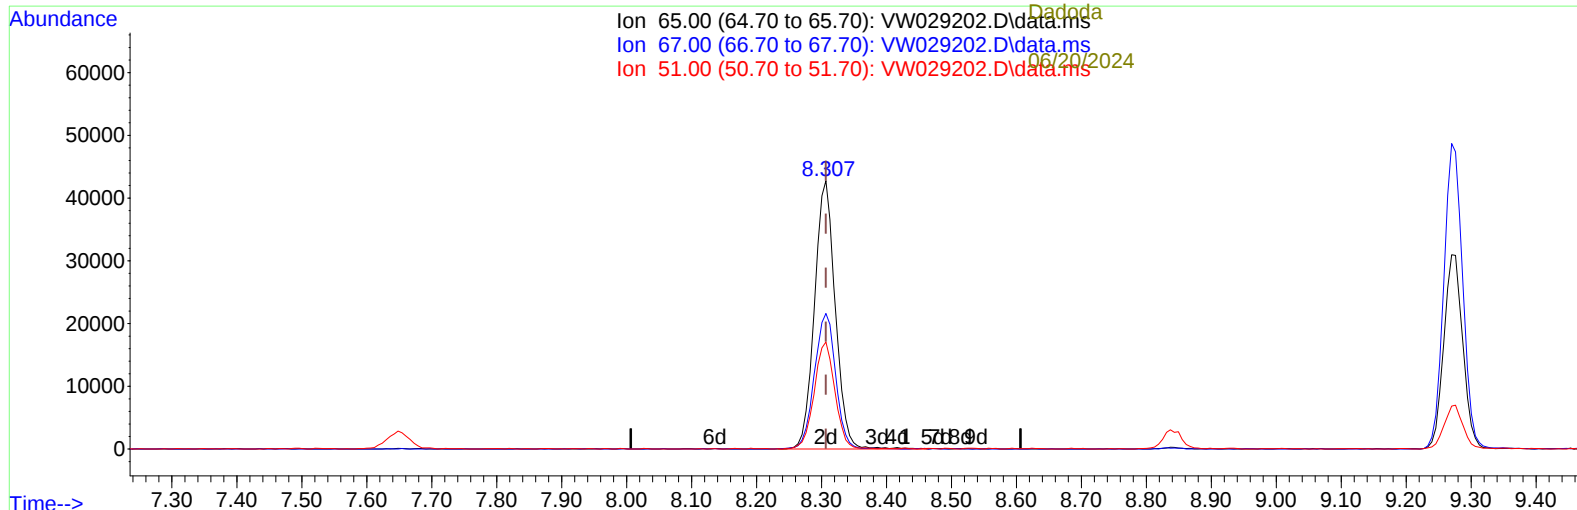

TIC: VW029202.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 22.58 ug/L m

response 94951

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.50	0.08#
51.00	99.20	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
 Data File : VW029202.D
 Acq On : 19 Jun 2024 10:09
 Operator : SY/MD
 Sample : P2844-03
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/20/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 20 01:54:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 20 00:39:34 2024
 Response via : Initial Calibration

06/20/2024
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	245489	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	228768	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	103680	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	74184	21.833	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.320%
7) Chloroethane-d5	2.899	69	59732	20.817	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.280%
11) 1,1-Dichloroethene-d2	4.015	65	34849	21.242	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.960%
21) 2-Butanone-d5	7.075	46	44577	43.850	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.700%
24) Chloroform-d	7.648	84	155007	21.167	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.680%
26) 1,2-Dichloroethane-d4	8.307	65	94951m	22.583	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.320%
32) Benzene-d6	8.276	84	305554	21.990	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.960%
36) 1,2-Dichloropropane-d6	9.270	67	98217	22.236	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.960%
41) Toluene-d8	10.325	98	270516	22.004	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	10.575	79	38071	21.389	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.560%
47) 2-Hexanone-d5	10.922	63	30293	43.749	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	76115	21.651	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	88992	24.728	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.920%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
Data File : VW029202.D
Acq On : 19 Jun 2024 10:09
Operator : SY/MD
Sample : P2844-03
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/20/2024
Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 20 01:54:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 20 00:39:34 2024
Response via : Initial Calibration

06/20/2024
Supervised By :Mahesh
Dadoda

06/20/2024

