

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
 Data File : VW029220.D
 Acq On : 19 Jun 2024 17:23
 Operator : SY/MD
 Sample : P2934-03
 Misc : 5.79g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4B61

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/20/2024
 Supervised By :Mahesh Dadoda 06/20/2024

Quant Time: Jun 20 01:56:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 20 00:39:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	340658	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	243945	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	72822	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	78126	16.569	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.280%		
7) Chloroethane-d5	2.893	69	70725	17.762	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.040%		
11) 1,1-Dichloroethene-d2	4.021	65	35640	15.655	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.640%		
21) 2-Butanone-d5	7.075	46	74526	52.830	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.660%		
24) Chloroform-d	7.648	84	179030	17.618	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	70.480%		
26) 1,2-Dichloroethane-d4	8.301	65	116988m	20.051	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.200%		
32) Benzene-d6	8.270	84	319384	21.555	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.200%		
36) 1,2-Dichloropropane-d6	9.270	67	113480	24.093	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.360%		
41) Toluene-d8	10.319	98	230392	17.575	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	70.280%		
43) trans-1,3-Dichloroprop...	10.575	79	27273	14.369	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	57.480%		
47) 2-Hexanone-d5	10.922	63	32194	43.602	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.200%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	84278	22.482	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	89.920%		
66) 1,2-Dichlorobenzene-d4	13.848	152	39168	15.495	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	62.000%#		
Target Compounds					Qvalue	
13) Acetone	4.125	43	6713	5.600	ug/L	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
Data File : VW029220.D
Acq On : 19 Jun 2024 17:23
Operator : SY/MD
Sample : P2934-03
Misc : 5.79g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4B61

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 06/20/2024
Supervised By : Mahesh Dadoda 06/20/2024


Quant Time: Jun 20 01:56:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 20 00:39:34 2024
Response via : Initial Calibration

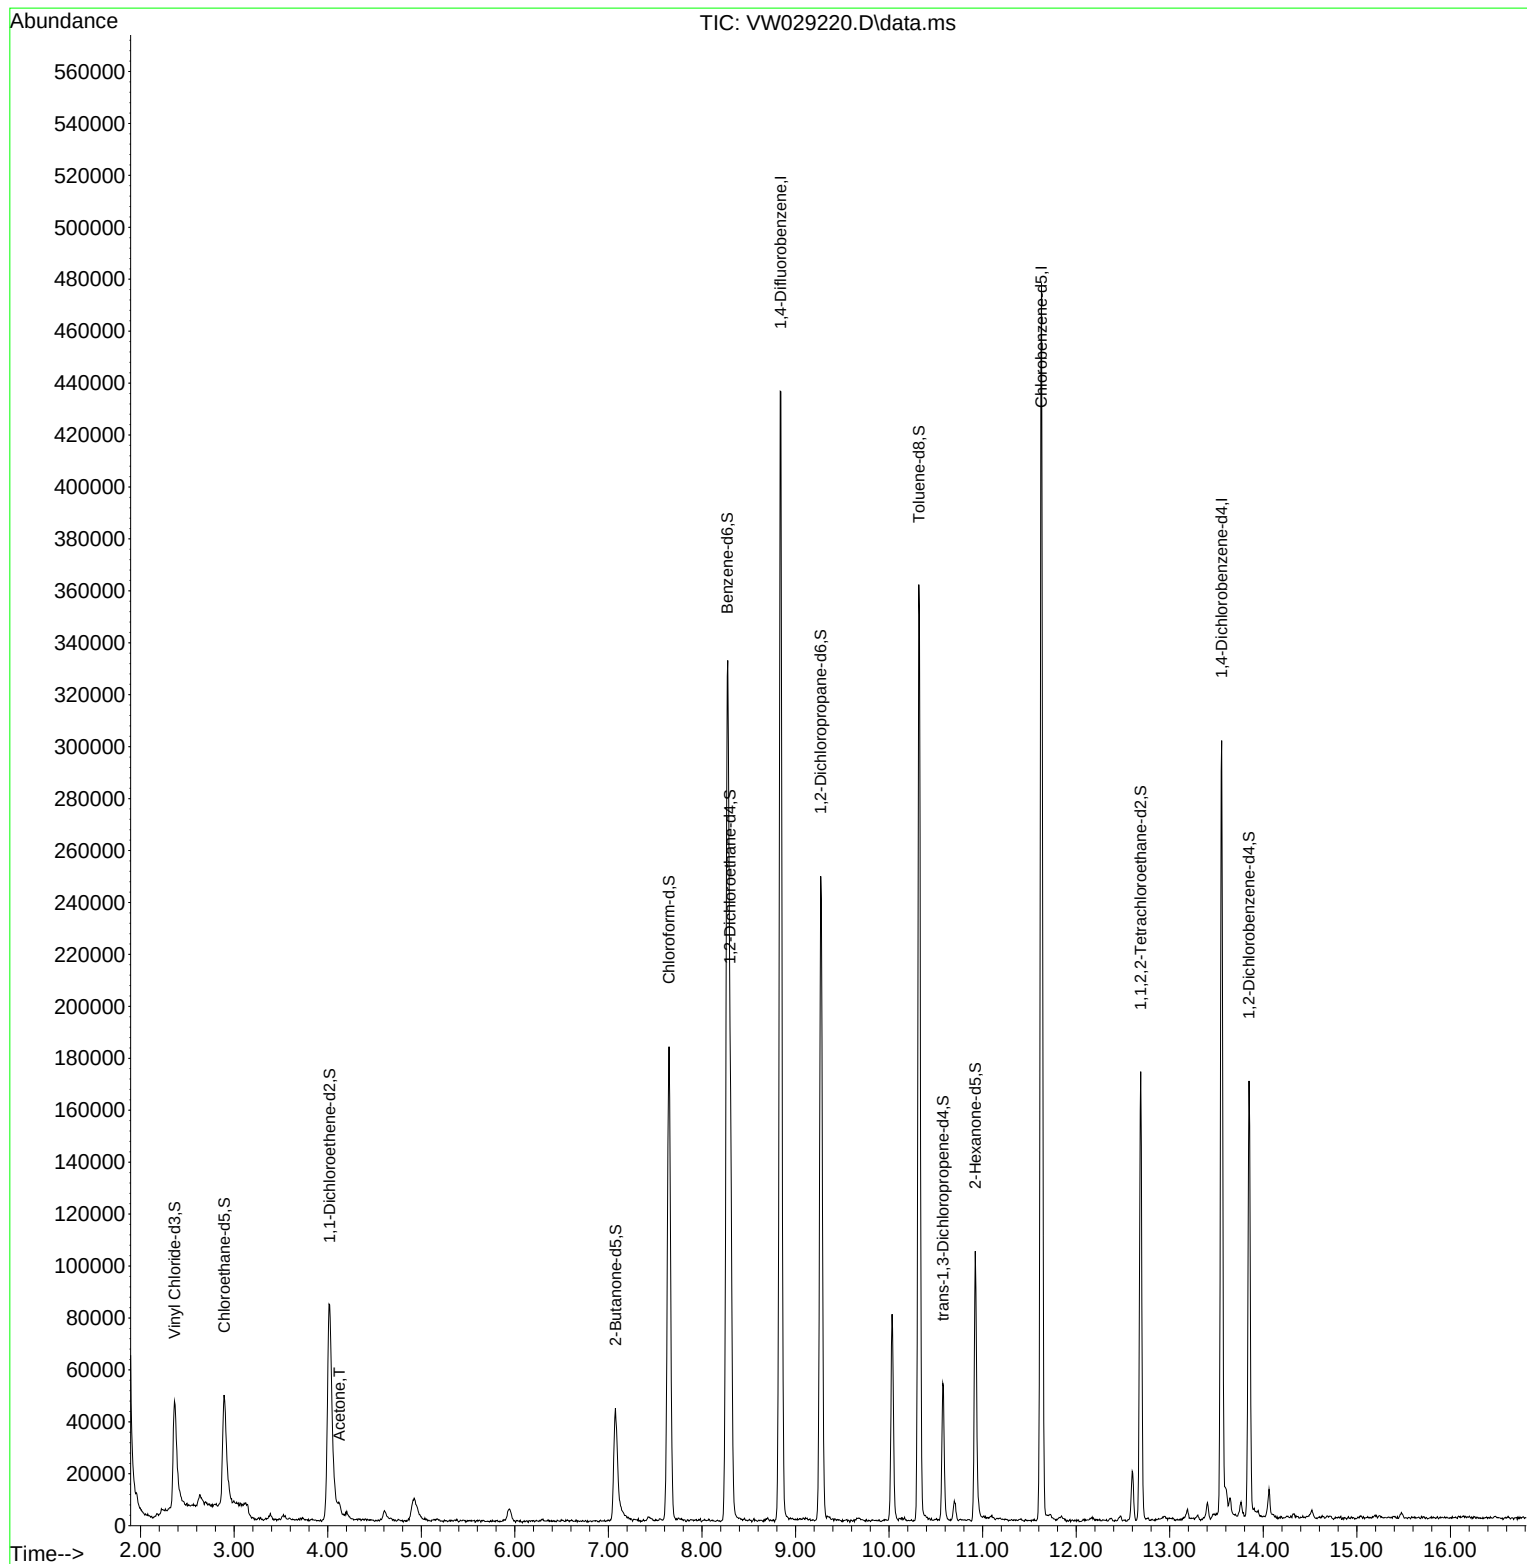

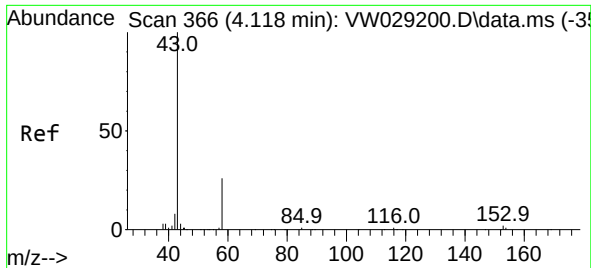

#13
Acetone
Concen: 5.600 ug/L
RT: 4.125 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW029220.D
Acq: 19 Jun 2024 17:23

Instrument :
MSVOA_W
ClientSampleId :
A4B61

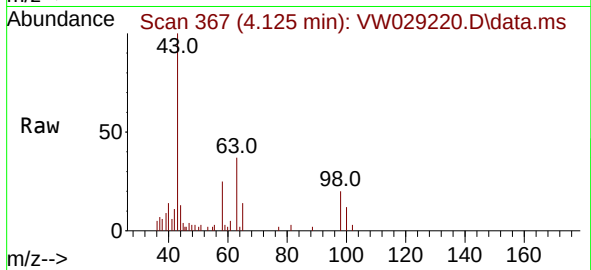

Tgt Ion: 43 Resp: 671
Ion Ratio Lower Upper
43 100
58 17.2 0.0 61.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/20/2024
Supervised By :Mahesh Dadoda 06/20/2024

