

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
 Data File : VW029229.D
 Acq On : 19 Jun 2024 21:52
 Operator : SY/MD
 Sample : P2963-06
 Misc : 6.22g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CQ7

Quant Time: Jun 20 01:57:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 20 00:39:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	314031	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	196850	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	43908	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	84032	19.333	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.320%
7) Chloroethane-d5	2.893	69	76746	20.909	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.640%
11) 1,1-Dichloroethene-d2	4.021	65	37792	18.008	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.040%
21) 2-Butanone-d5	7.075	46	56388	43.362	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.720%
24) Chloroform-d	7.648	84	192162	20.513	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.040%
26) 1,2-Dichloroethane-d4	8.307	65	110438	20.533	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.120%
32) Benzene-d6	8.270	84	335414	28.052	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	112.200%
36) 1,2-Dichloropropane-d6	9.270	67	119602	31.468	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	125.880%#
41) Toluene-d8	10.319	98	231634	21.897	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	10.575	79	24047	15.700	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.800%
47) 2-Hexanone-d5	10.922	63	20460	34.339	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75598	24.991	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.960%
66) 1,2-Dichlorobenzene-d4	13.849	152	32859	21.560	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.240%
Target Compounds					Qvalue	
13) Acetone	4.125	43	5992	5.422	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061924\
Data File : VW029229.D
Acq On : 19 Jun 2024 21:52
Operator : SY/MD
Sample : P2963-06
Misc : 6.22g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CQ7

Quant Time: Jun 20 01:57:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 20 00:39:34 2024
Response via : Initial Calibration

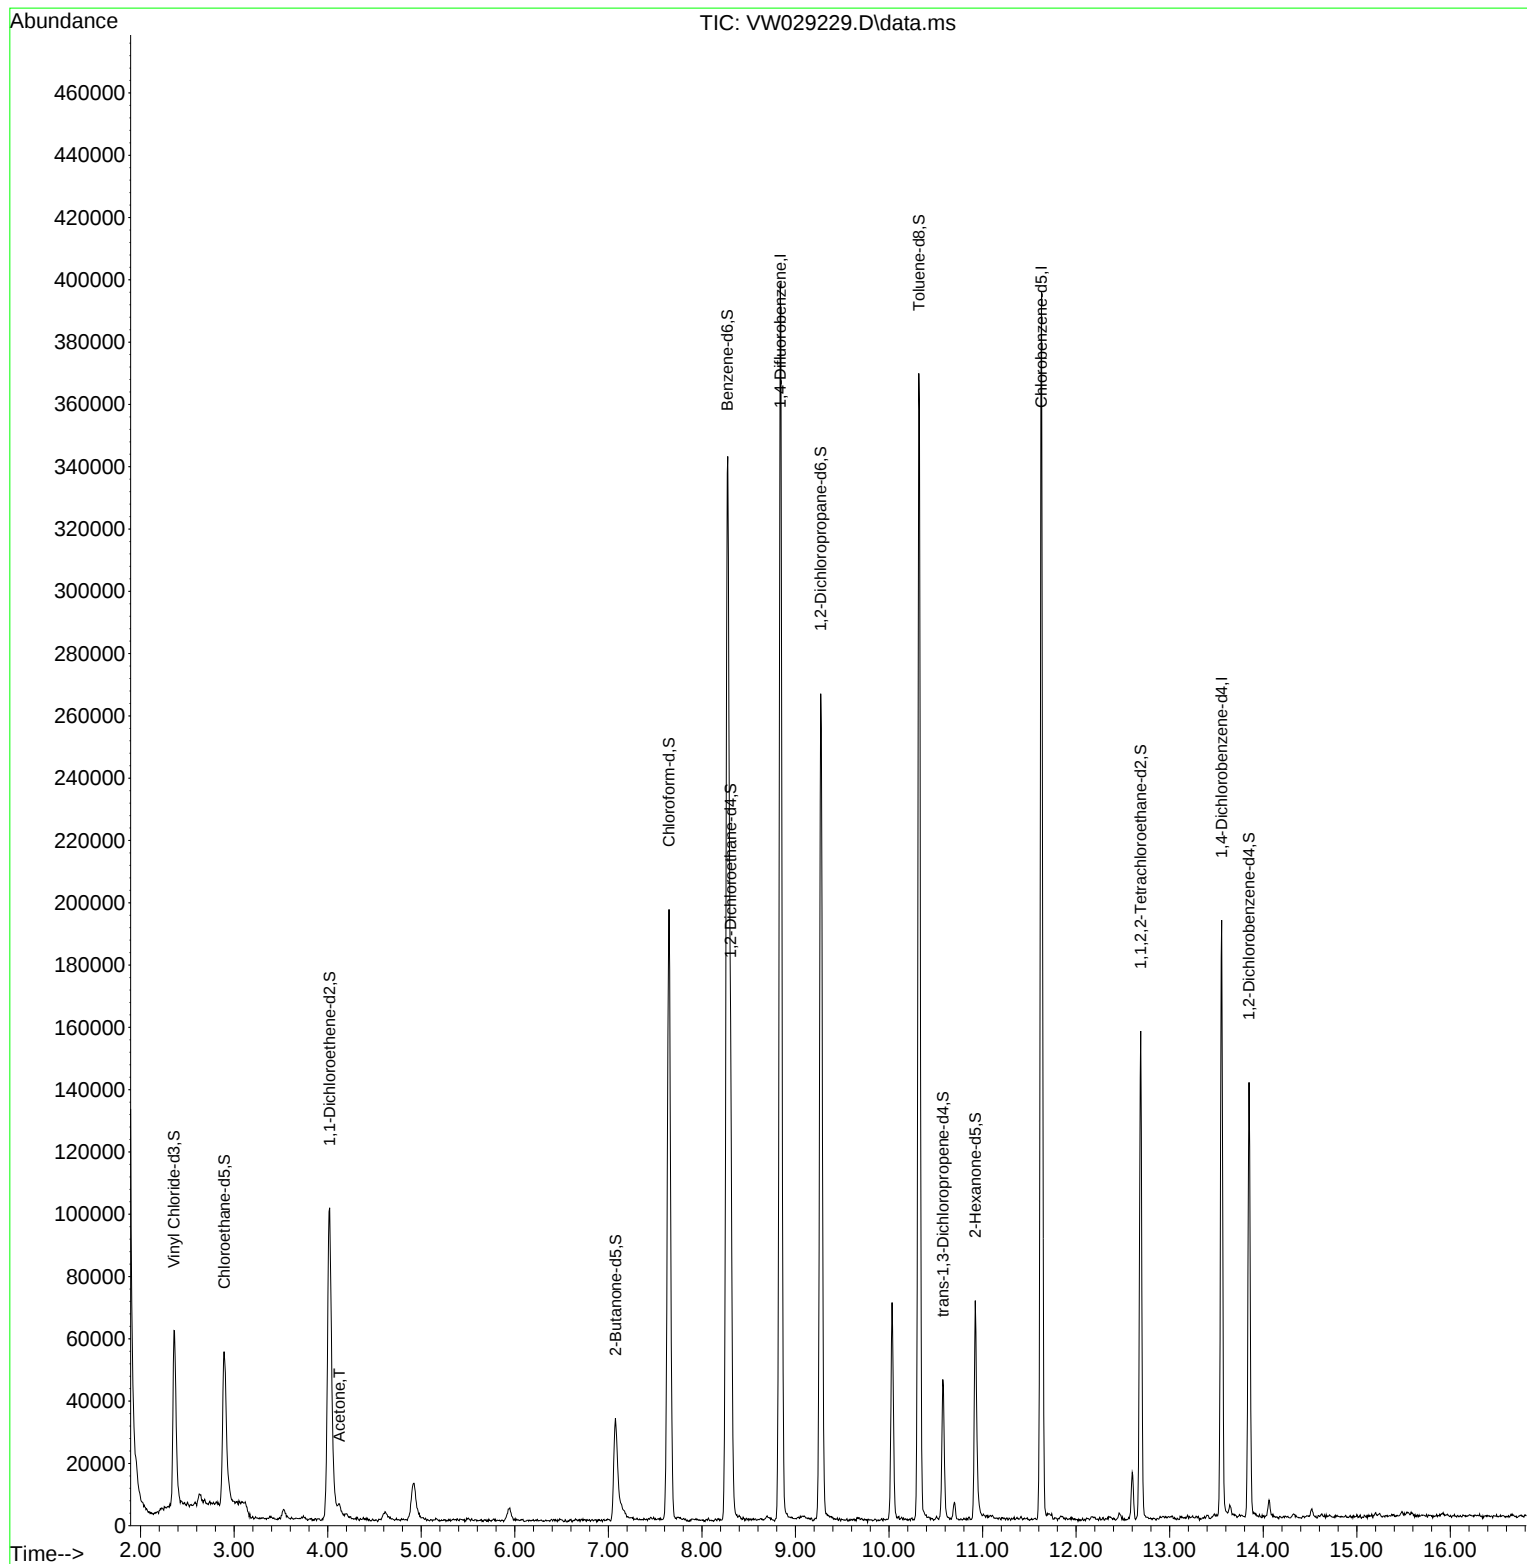

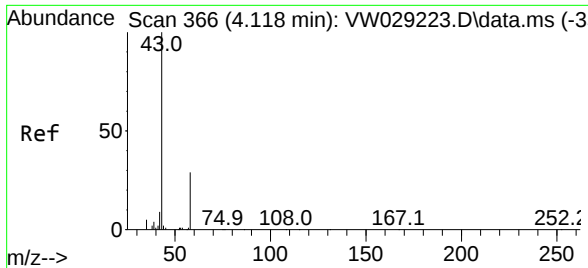

#13
 Acetone
 Concen: 5.422 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW029229.D
 Acq: 19 Jun 2024 21:52

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CQ7

Tgt Ion: 43	Resp: 5992
Ion Ratio	Lower Upper
43	100
58	34.3 0.0 61.4

