

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
 Data File : VW029288.D
 Acq On : 21 Jun 2024 04:07
 Operator : SY/MD
 Sample : P2964-18
 Misc : 5.49g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 21 04:53:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 02:43:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	515401	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	470908	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	211041	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.375	65	113602	15.925	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.680%
7) Chloroethane-d5	2.905	69	104444	17.337	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.360%
11) 1,1-Dichloroethene-d2	4.027	65	58084	16.863	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.440%
21) 2-Butanone-d5	7.075	46	102006	47.794	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.580%
24) Chloroform-d	7.648	84	306504	19.936	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.760%
26) 1,2-Dichloroethane-d4	8.307	65	174103	19.723	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.880%
32) Benzene-d6	8.276	84	566002	19.788	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.160%
36) 1,2-Dichloropropane-d6	9.276	67	192502	21.172	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.680%
41) Toluene-d8	10.325	98	485867	19.200	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.800%
43) trans-1,3-Dichloroprop...	10.575	79	64793	17.684	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.720%
47) 2-Hexanone-d5	10.922	63	71769	50.353	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.700%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	159878	22.093	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	175567	23.967	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	5048	0.449	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
Data File : VW029288.D
Acq On : 21 Jun 2024 04:07
Operator : SY/MD
Sample : P2964-18
Misc : 5.49g/10mL/MSVOA_W/SOIL/A
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 21 04:53:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 02:43:08 2024
Response via : Initial Calibration

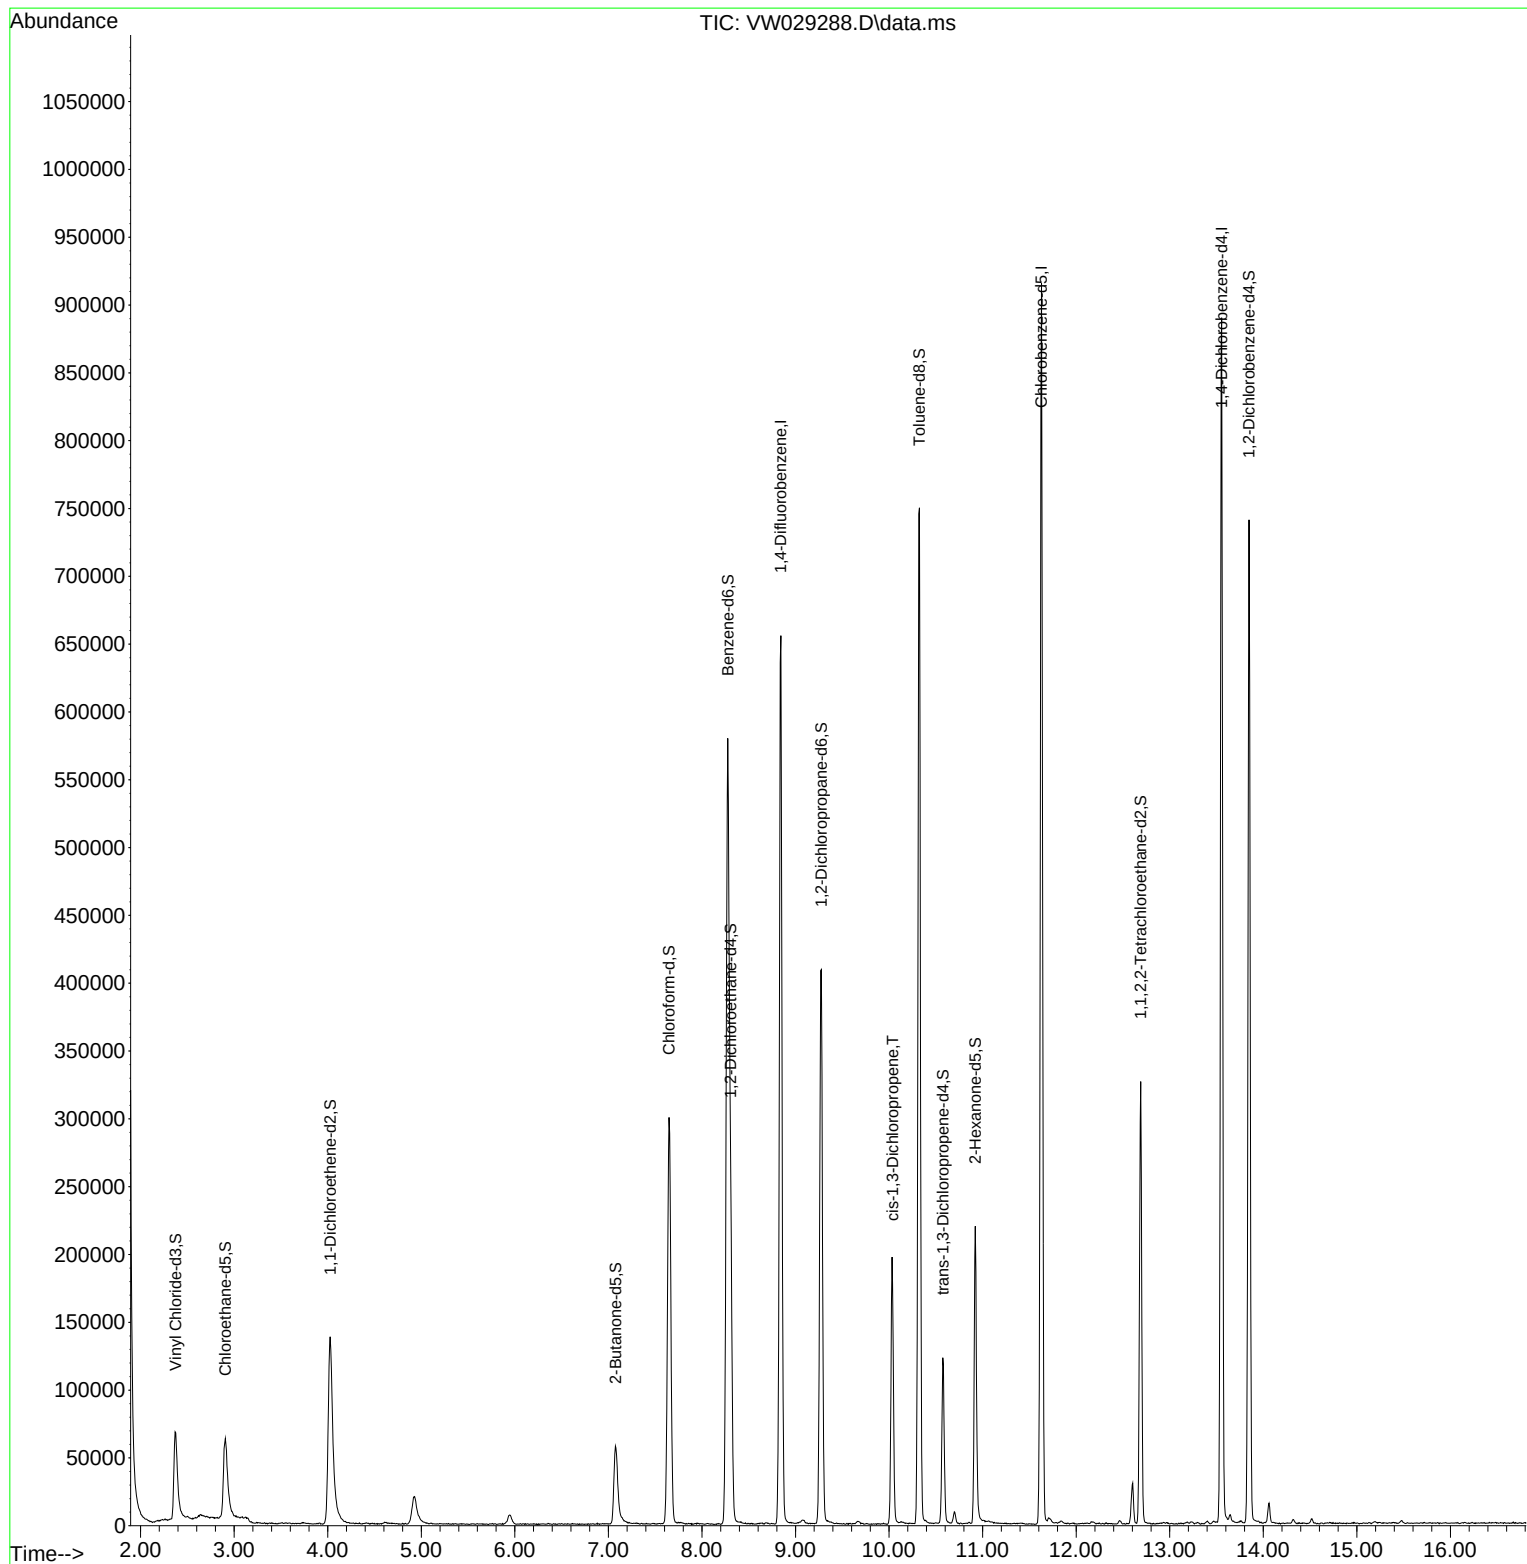

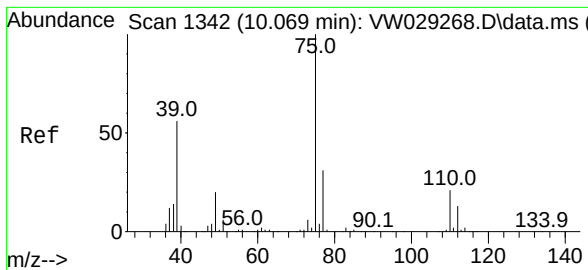

#39
 cis-1,3-Dichloropropene
 Concen: 0.449 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW029288.D
 Acq: 21 Jun 2024 04:07

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5048
 Ion Ratio Lower Upper
 75 100
 77 40.8 22.7 42.1

