
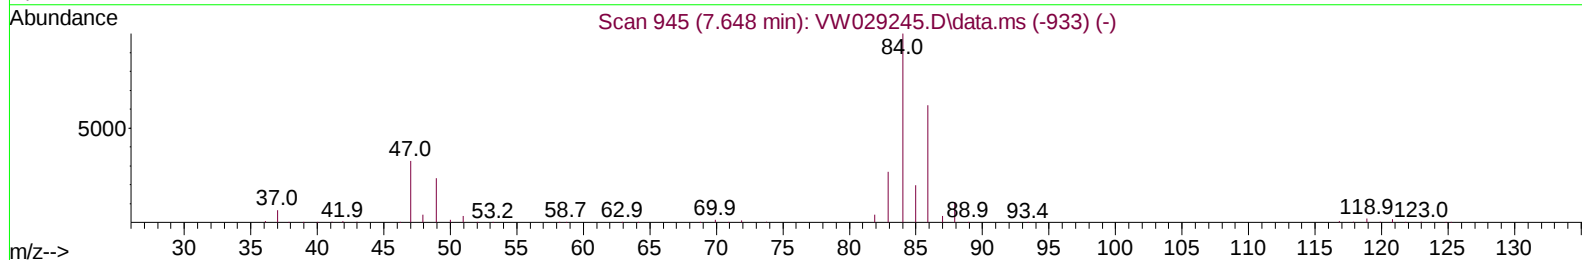
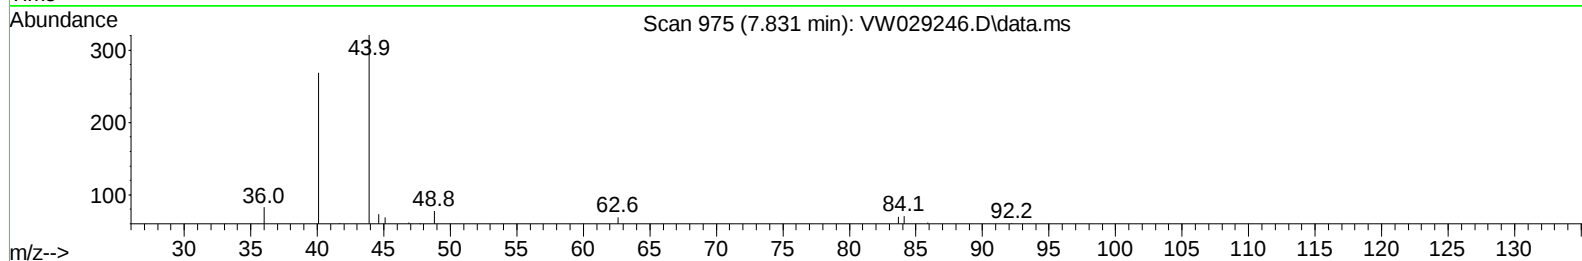


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
Data File : VW029246.D
Acq On : 20 Jun 2024 10:19
Operator : SY/MD
Sample : VW0620SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 21 01:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 01:26:21 2024
Response via : Initial Calibration

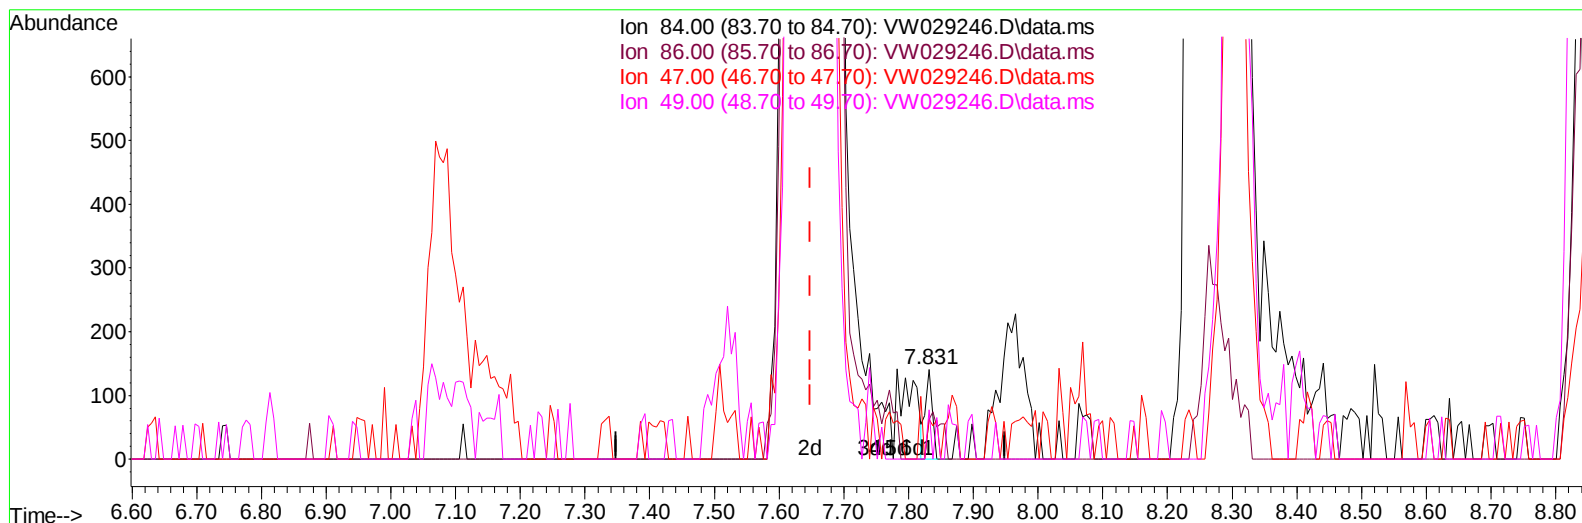

TIC: VW029246.D\data.ms

(24) Chloroform-d (S)




7.831min (+ 0.183) 0.01 ug/L

response 101

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.50	67.33
47.00	49.90	63.37
49.00	29.20	28.71

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
Data File : VW029246.D
Acq On : 20 Jun 2024 10:19
Operator : SY/MD
Sample : VW0620SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 21 01:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 01:26:21 2024
Response via : Initial Calibration

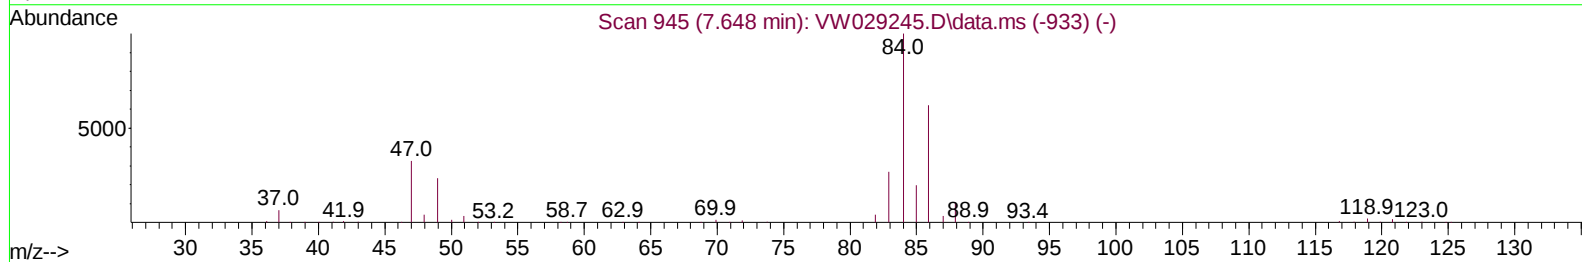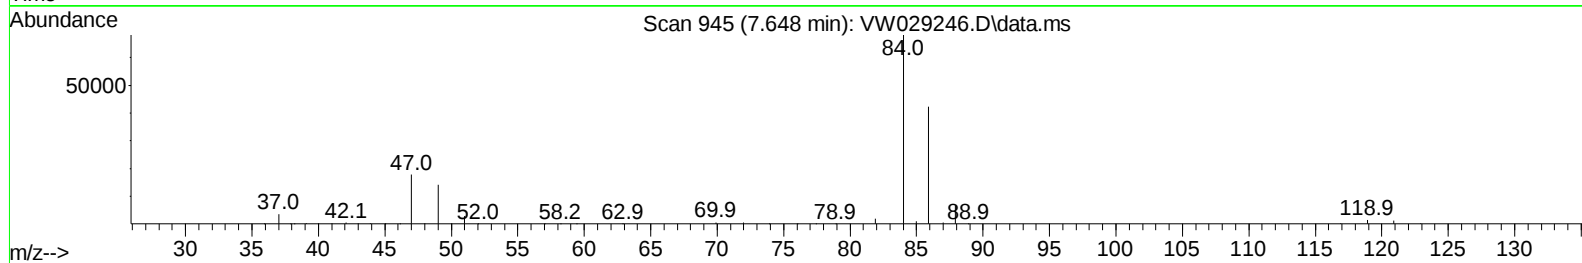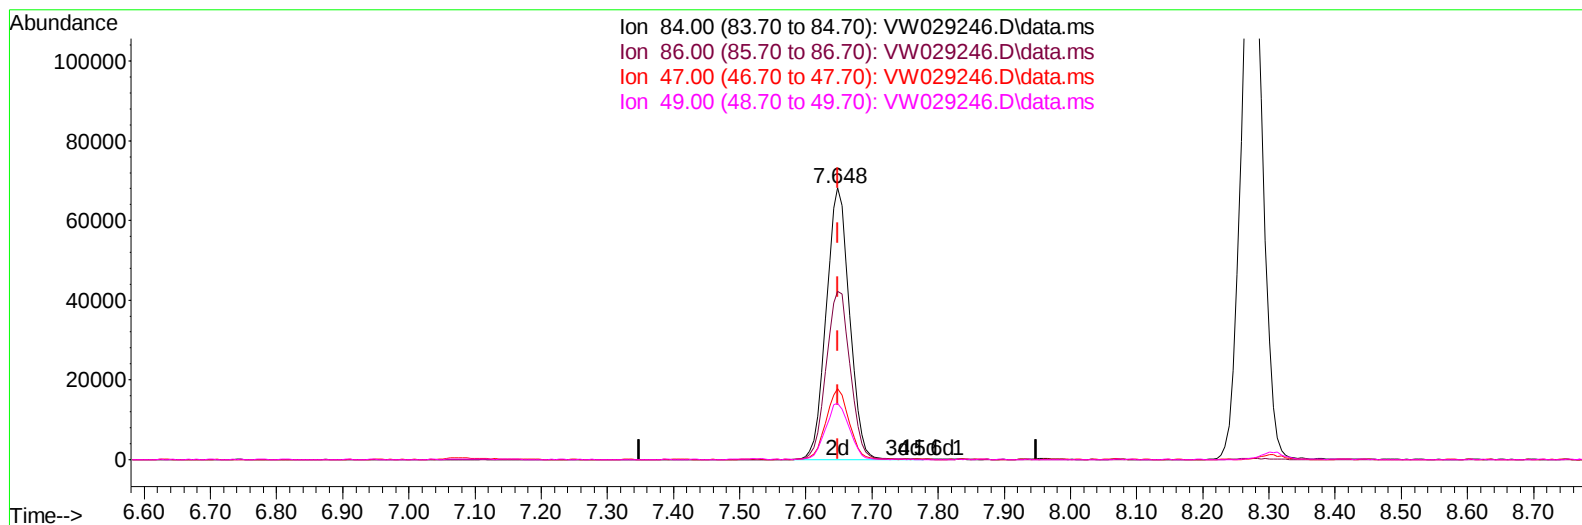

TIC: VW029246.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 18.23 ug/L m

response 165834

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.50	0.04#
47.00	49.90	0.04#
49.00	29.20	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
 Data File : VW029246.D
 Acq On : 20 Jun 2024 10:19
 Operator : SY/MD
 Sample : VW0620SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 21 01:30:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 01:26:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	304872	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	282603	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	130157	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	74995	17.772	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.080%	
7) Chloroethane-d5	2.899	69	60791	17.059	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.240%	
11) 1,1-Dichloroethene-d2	4.021	65	36783	18.054	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.200%	
21) 2-Butanone-d5	7.075	46	50795	40.234	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	80.460%	
24) Chloroform-d	7.648	84	165834m	18.235	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	72.920%	
26) 1,2-Dichloroethane-d4	8.307	65	100538	19.254	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	77.000%	
32) Benzene-d6	8.276	84	328862	19.159	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	76.640%	
36) 1,2-Dichloropropane-d6	9.276	67	107022	19.614	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	78.440%	
41) Toluene-d8	10.319	98	300168	19.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.080%	
43) trans-1,3-Dichloroprop...	10.581	79	40464	18.402	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	73.600%	
47) 2-Hexanone-d5	10.922	63	34264	40.057	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	80.120%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	86792	19.985	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	79.960%	
66) 1,2-Dichlorobenzene-d4	13.848	152	98211	21.738	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	86.960%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
Data File : VW029246.D
Acq On : 20 Jun 2024 10:19
Operator : SY/MD
Sample : VW0620SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 21 01:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 01:26:21 2024
Response via : Initial Calibration

