

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
 Data File : VW029258.D
 Acq On : 20 Jun 2024 15:17
 Operator : SY/MD
 Sample : P2963-15RE
 Misc : 5.31g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CR9RE

Quant Time: Jun 21 01:32:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 01:26:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	346725	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	237932	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	63336	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	91084	18.979	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.920%		
7) Chloroethane-d5	2.899	69	80194	19.788	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.160%		
11) 1,1-Dichloroethene-d2	4.021	65	41107	17.740	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	70.960%		
21) 2-Butanone-d5	7.081	46	60835	42.370	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	84.740%		
24) Chloroform-d	7.648	84	214509	20.740	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.960%		
26) 1,2-Dichloroethane-d4	8.307	65	135873	22.880	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.520%		
32) Benzene-d6	8.276	84	389189	26.930	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	107.720%		
36) 1,2-Dichloropropane-d6	9.270	67	136505	29.714	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	118.840%		
41) Toluene-d8	10.319	98	274809	21.493	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.960%		
43) trans-1,3-Dichloroprop...	10.575	79	30724	16.596	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.400%		
47) 2-Hexanone-d5	10.922	63	34066	47.303	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.600%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	95047	25.995	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	104.000%		
66) 1,2-Dichlorobenzene-d4	13.855	152	46439	21.124	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.480%		
Target Compounds					Qvalue	
13) Acetone	4.131	43	5662	4.640	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
Data File : VW029258.D
Acq On : 20 Jun 2024 15:17
Operator : SY/MD
Sample : P2963-15RE
Misc : 5.31g/10mL/MSVOA_W/SOIL/B
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CR9RE

Quant Time: Jun 21 01:32:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 01:26:21 2024
Response via : Initial Calibration

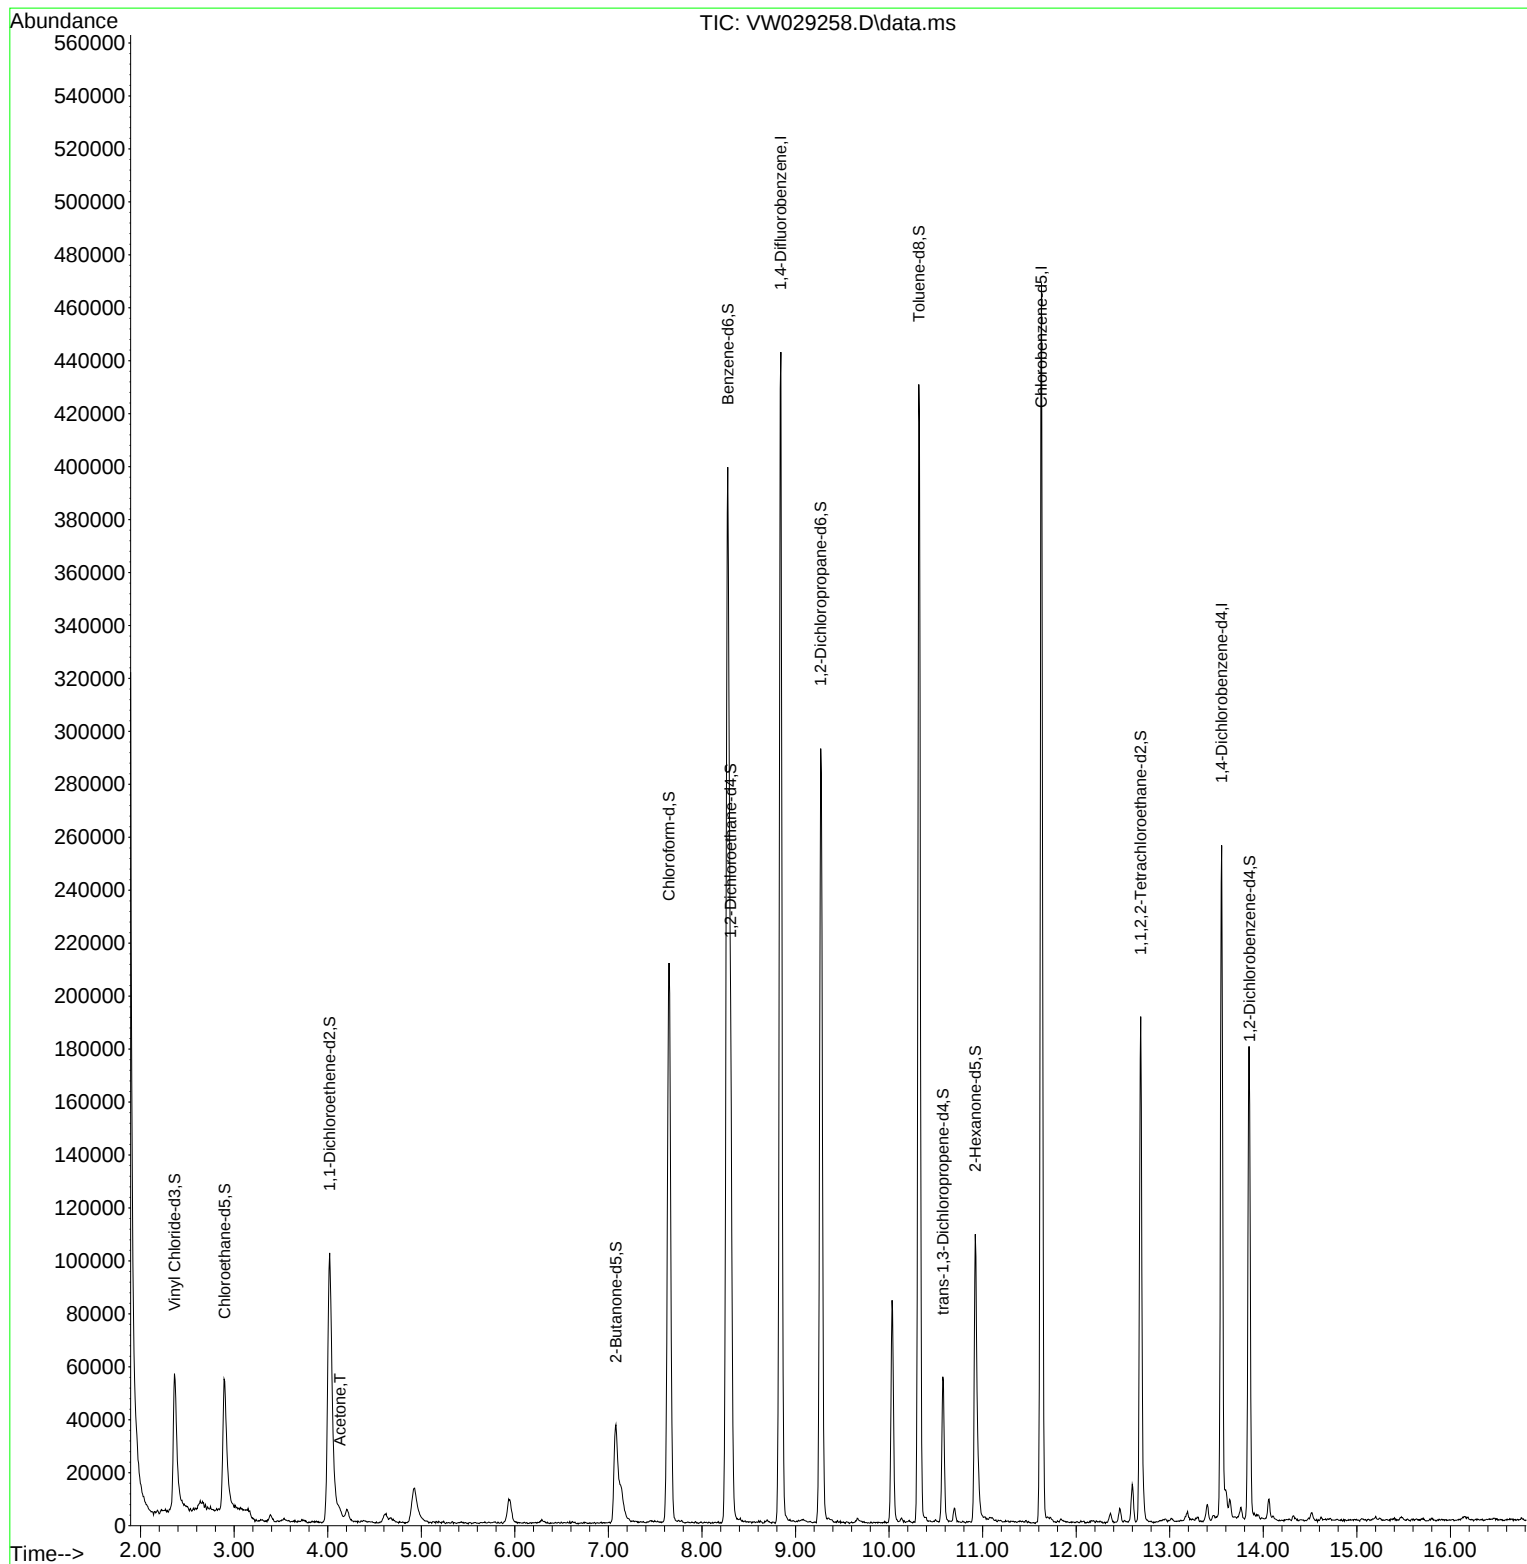

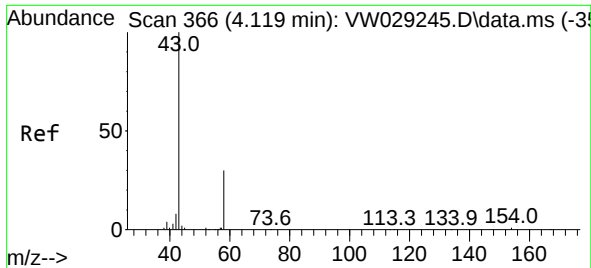

#13

Acetone

Concen: 4.640 ug/L

RT: 4.131 min Scan# 3

Delta R.T. 0.012 min

Lab File: VW029258.D

Acq: 20 Jun 2024 15:17

Instrument :

MSVOA_W

ClientSampleId :

A4CR9RE

Tgt Ion: 43 Resp: 5662

Ion Ratio Lower Upper

43 100

58 28.8 0.0 61.4

