

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
 Data File : VW029259.D
 Acq On : 20 Jun 2024 15:42
 Operator : SY/MD
 Sample : P2963-16RE
 Misc : 5.11g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CS7RE

Quant Time: Jun 21 01:33:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 01:26:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	376864	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	237438	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	53071	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	94821	18.178	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.720%
7) Chloroethane-d5	2.893	69	82312	18.686	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.760%
11) 1,1-Dichloroethene-d2	4.021	65	43305	17.194	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.760%
21) 2-Butanone-d5	7.081	46	60693	38.891	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.780%
24) Chloroform-d	7.648	84	223525	19.883	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.520%
26) 1,2-Dichloroethane-d4	8.300	65	131964	20.445	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.760%
32) Benzene-d6	8.270	84	406963	28.218	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	112.880%
36) 1,2-Dichloropropane-d6	9.276	67	139359	30.398	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	121.600%#
41) Toluene-d8	10.318	98	285567	22.381	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.520%
43) trans-1,3-Dichloroprop...	10.574	79	24119	13.055	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	52.240%
47) 2-Hexanone-d5	10.922	63	31103	43.279	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.560%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	79357	21.749	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	34798	18.890	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.560%
Target Compounds						
13) Acetone	4.124	43	7295	5.500	ug/L	Qvalue 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062024\
Data File : VW029259.D
Acq On : 20 Jun 2024 15:42
Operator : SY/MD
Sample : P2963-16RE
Misc : 5.11g/10mL/MSVOA_W/SOIL/B
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CS7RE

Quant Time: Jun 21 01:33:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 01:26:21 2024
Response via : Initial Calibration

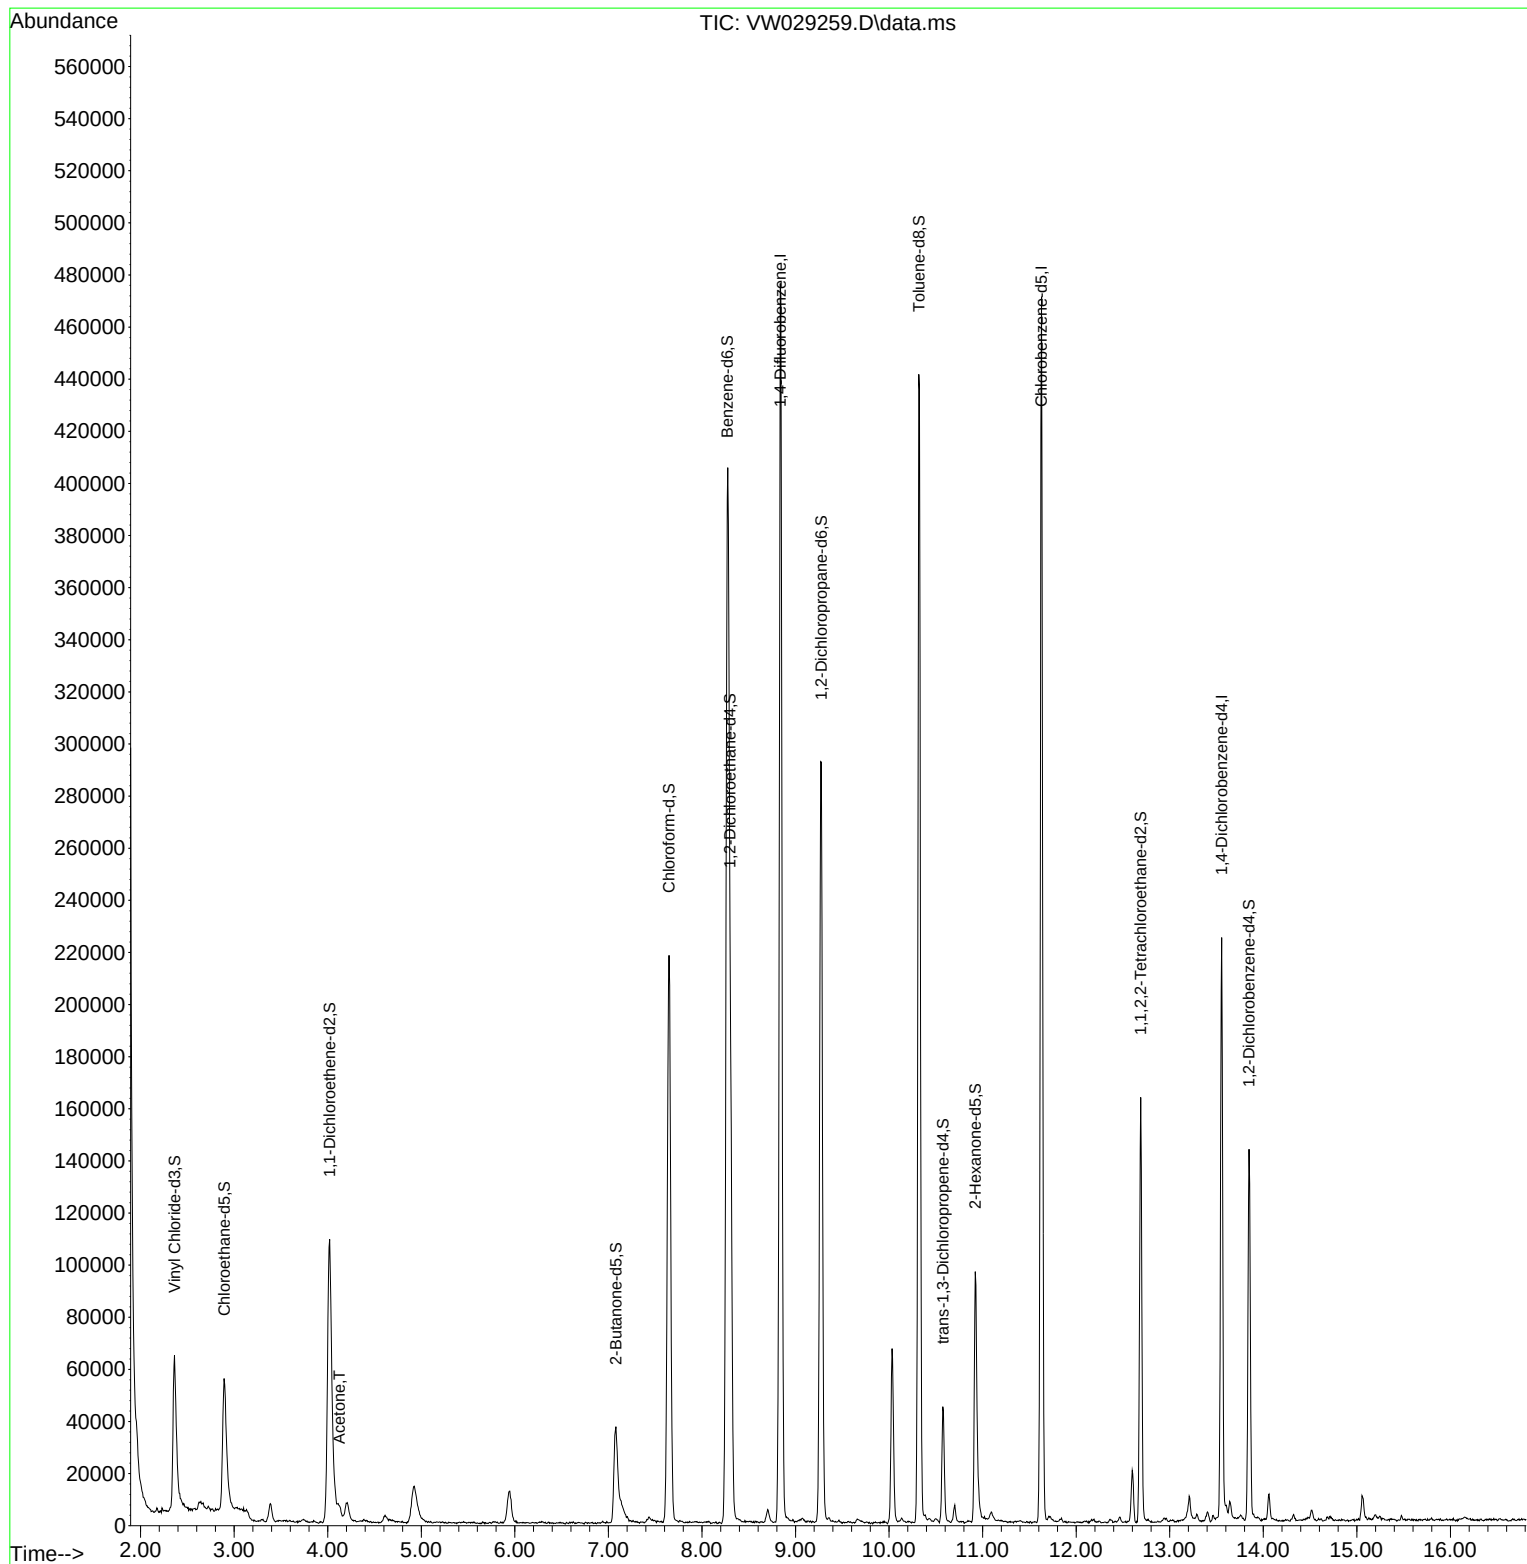

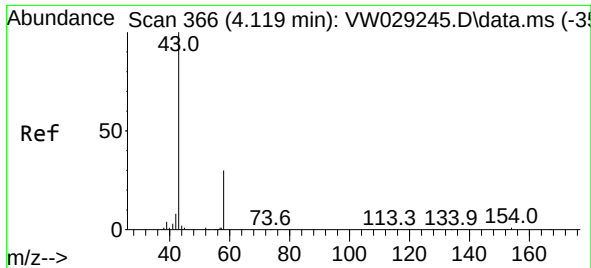

#13
 Acetone
 Concen: 5.500 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW029259.D
 Acq: 20 Jun 2024 15:42

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CS7RE

Tgt Ion: 43 Resp: 7295
 Ion Ratio Lower Upper
 43 100
 58 16.0 0.0 61.4

