

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062118\
 Data File : VW003384.D
 Acq On : 21 Jun 2018 13:45
 Operator : SY/AP
 Sample : J3569-10
 Misc : 3.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXR1RE

Quant Time: Jun 22 04:55:39 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 22 04:53:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	178606	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	87542	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	11576	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	115342	47.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	190.48%#
7) Chloroethane-d5	2.89	69	96779	47.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	191.56%#
10) 1,1-Dichloroethene-d2	4.01	63	163361	33.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	135.84%#
20) 2-Butanone-d5	7.09	46	66131	86.64	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	173.28%#
24) Chloroform-d	7.65	84	226066	48.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	192.48%#
26) 1,2-Dichloroethane-d4	8.31	65	136730	48.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	195.88%#
29) Benzene-d6	8.27	84	311580	67.08	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	268.32%#
33) 1,2-Dichloropropane-d6	9.28	67	138694	94.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	377.32%#
37) Toluene-d8	10.33	98	214083	48.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	192.84%#
38) trans-1,3-Dichloropropene-	10.58	79	47070	68.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	272.76%#
39) 2-Hexanone-d5	10.93	63	44385	147.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	295.38%#
48) 1,1,2,2-Tetrachloroethane-	12.70	84	107816	78.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	315.24%#
61) 1,2-Dichlorobenzene-d4	13.86	152	13539	30.97	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	123.88%#


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.16	43	2900	3.564	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW062118\
Data File : VW003384.D
Acq On : 21 Jun 2018 13:45
Operator : SY/AP
Sample : J3569-10
Misc : 3.39G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAXR1RE

Quant Time: Jun 22 04:55:39 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 22 04:53:24 2018
Response via : Initial Calibration

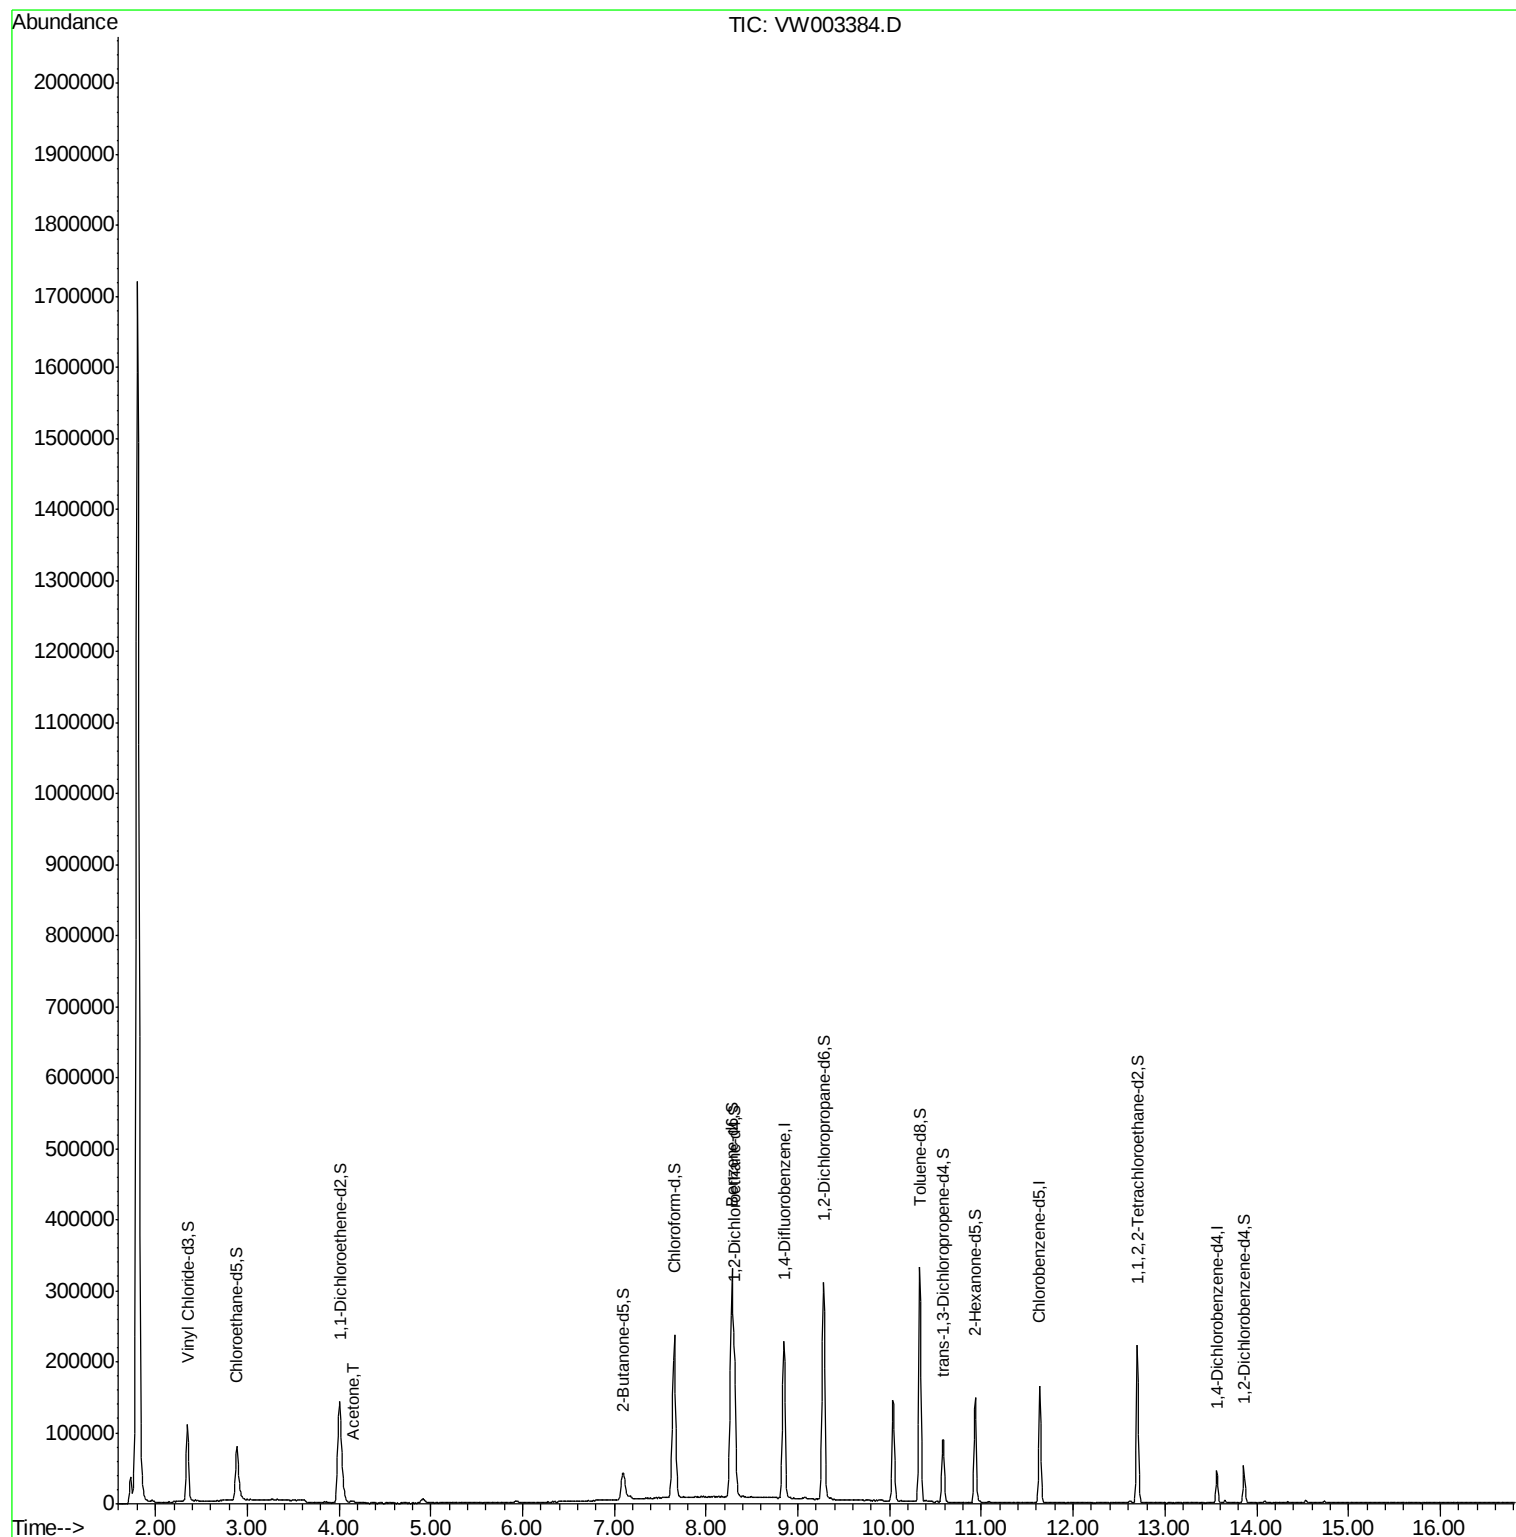

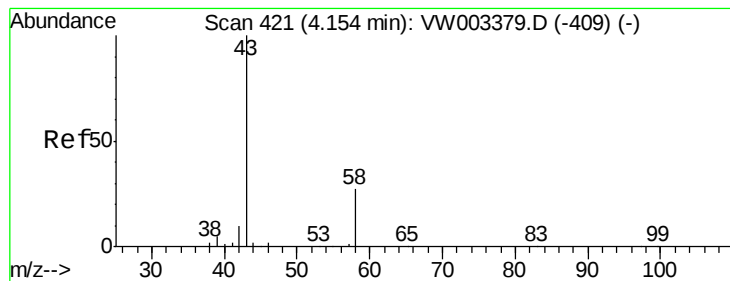

#13

Acetone

Concen: 3.564 ug/L

RT: 4.16 min Scan# 422

Delta R.T. 0.01 min

Lab File: VW003384.D

Acq: 21 Jun 2018 13:45

Instrument :
MSVOA_W
ClientSampleId :
DAXR1RE

Tgt Ion: 43 Resp: 2900

Ion Ratio Lower Upper

43 100

58 18.8 0.0 58.6

