

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062118\
 Data File : VW003383.D
 Acq On : 21 Jun 2018 13:19
 Operator : SY/AP
 Sample : J3569-09RE
 Misc : 3.54G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXR0RE

Quant Time: Jun 22 05:02:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 22 04:53:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	190688	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	106496	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	18881	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	109491	42.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	169.36%#
7) Chloroethane-d5	2.89	69	95854	44.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	177.68%#
10) 1,1-Dichloroethene-d2	4.01	63	160820	31.32	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	125.28%#
20) 2-Butanone-d5	7.09	46	83206	102.10	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	204.20%#
24) Chloroform-d	7.65	84	220562	43.97	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	175.88%#
26) 1,2-Dichloroethane-d4	8.31	65	130273	43.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	174.84%#
29) Benzene-d6	8.28	84	329635	58.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	233.36%#
33) 1,2-Dichloropropane-d6	9.28	67	136349	76.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	304.92%#
37) Toluene-d8	10.33	98	240905	44.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	178.36%#
38) trans-1,3-Dichloropropene-	10.58	79	37024	44.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	176.36%#
39) 2-Hexanone-d5	10.93	63	52559	143.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	287.52%#
48) 1,1,2,2-Tetrachloroethane-	12.70	84	115649	69.49	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	277.96%#
61) 1,2-Dichlorobenzene-d4	13.86	152	22968	32.21	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	128.84%#


Target Compounds					Ovalue
13) Acetone	4.15	43	29064	33.46 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062118\
Data File : VW003383.D
Acq On : 21 Jun 2018 13:19
Operator : SY/AP
Sample : J3569-09RE
Misc : 3.54G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAXR0RE

Quant Time: Jun 22 05:02:36 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 22 04:53:24 2018
Response via : Initial Calibration

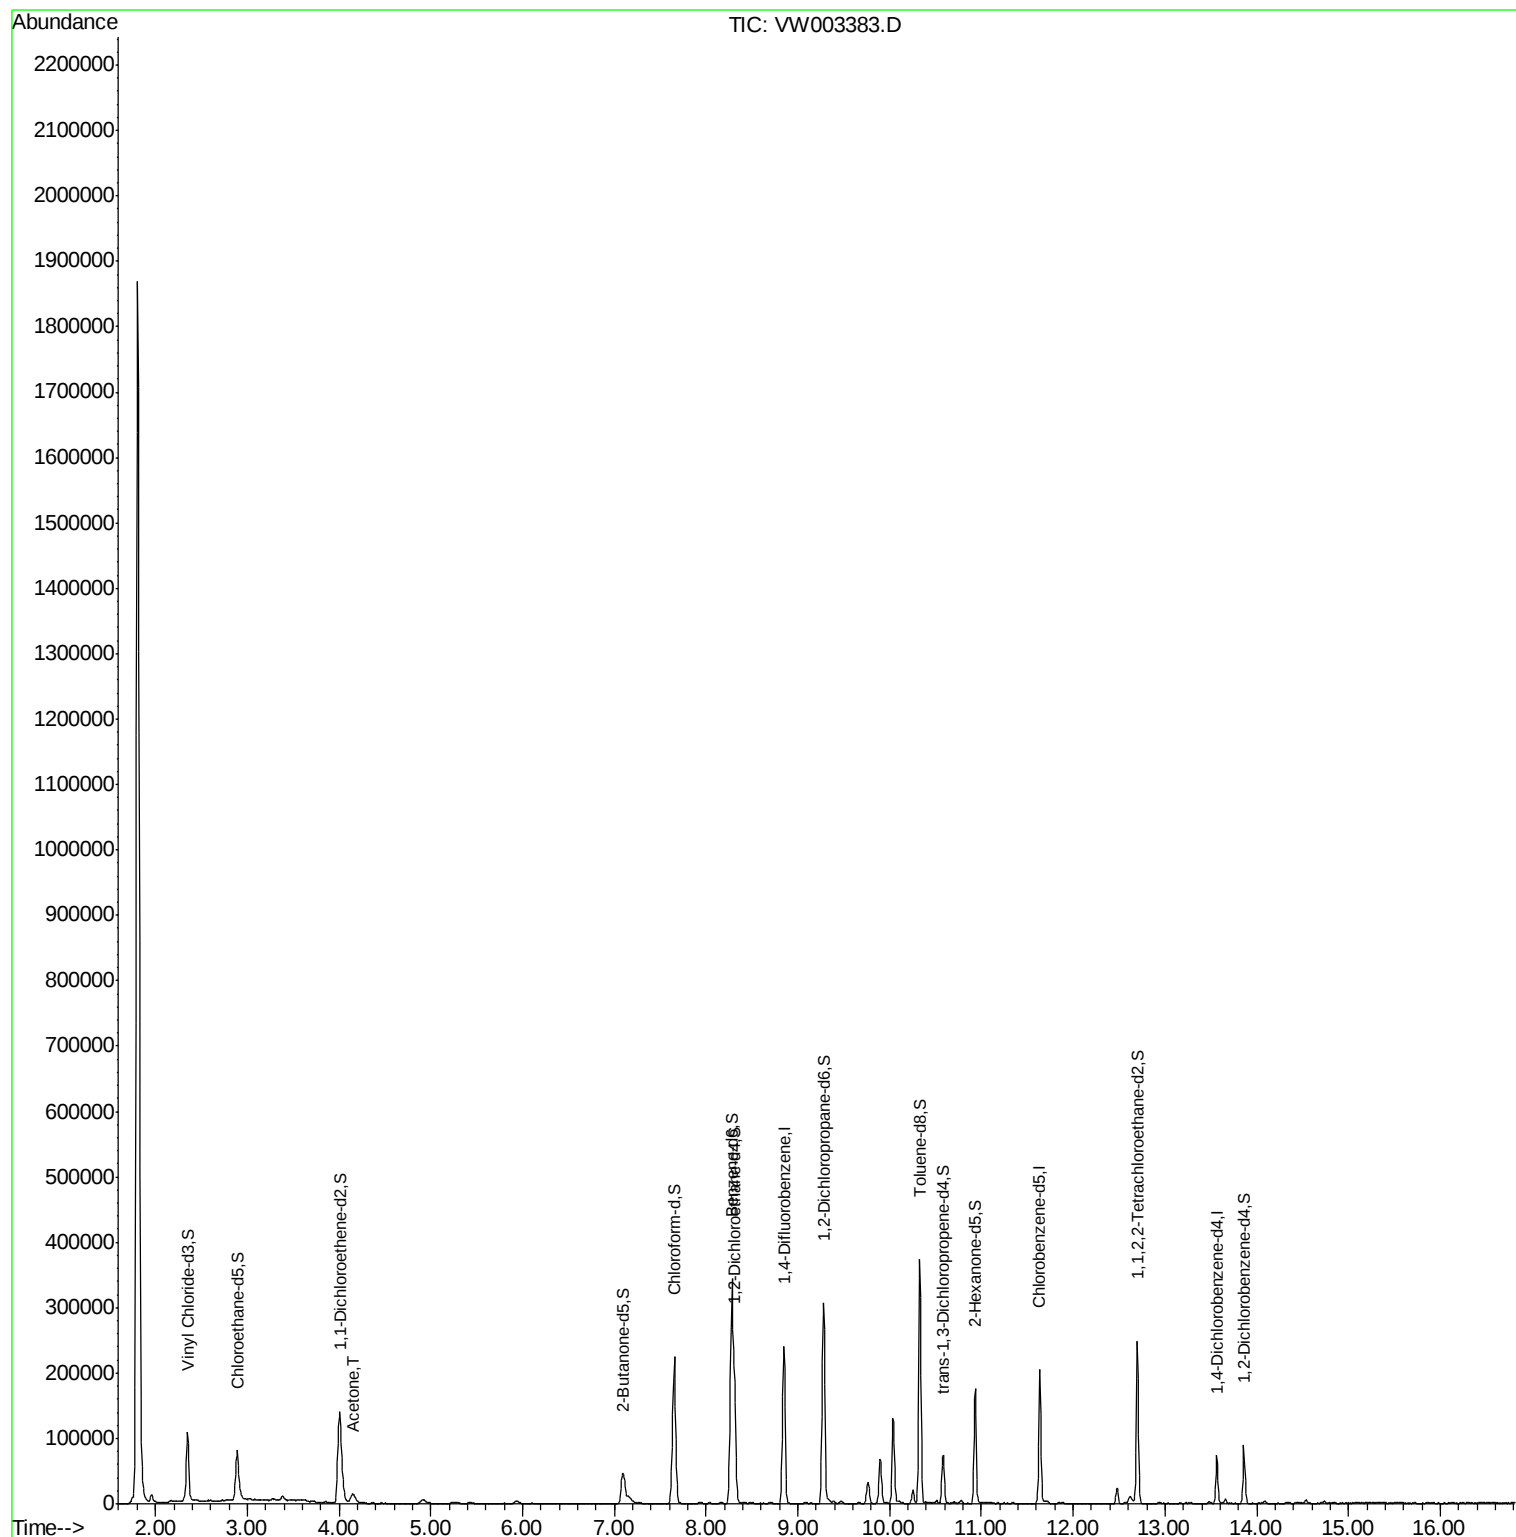

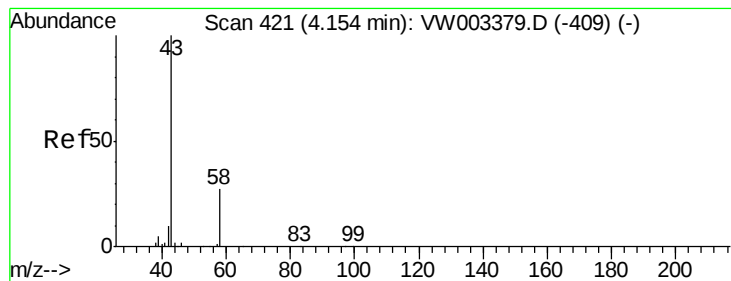

#13
 Acetone
 Concen: 33.46 ug/L
 RT: 4.15 min Scan# 420
 Delta R.T. -0.01 min
 Lab File: VW003383.D
 Acq: 21 Jun 2018 13:19

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXR0RE

Tot Ion: 43 Resp: 29064
 Ion Ratio Lower Upper
 43 100
 58 28.4 0.0 58.6

