

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
 Data File : VW003432.D
 Acq On : 22 Jun 2018 17:55
 Operator : SY/AP
 Sample : J3621-10
 Misc : 6.82G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAZ62

Quant Time: Jun 23 02:16:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 23 02:14:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	303611	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	300084	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	138304	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	85365	20.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.92%
7) Chloroethane-d5	2.89	69	70915	20.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.56%
10) 1,1-Dichloroethene-d2	4.01	63	130645	15.98	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.92%
20) 2-Butanone-d5	7.09	46	56671	43.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.36%
24) Chloroform-d	7.65	84	182927	22.90	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	8.31	65	111395	23.47	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.88%
29) Benzene-d6	8.28	84	331890	20.84	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.36%
33) 1,2-Dichloropropane-d6	9.28	67	112067	22.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.92%
37) Toluene-d8	10.33	98	307507	20.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.80%
38) trans-1,3-Dichloropropene-	10.58	79	46313	19.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.28%
39) 2-Hexanone-d5	10.93	63	41249	40.04	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.08%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	99131	21.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.56%
61) 1,2-Dichlorobenzene-d4	13.87	152	122000	23.36	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.44%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	13.57	75	17982	5.294	ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
Data File : VW003432.D
Acq On : 22 Jun 2018 17:55
Operator : SY/AP
Sample : J3621-10
Misc : 6.82G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAZ62

Quant Time: Jun 23 02:16:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 23 02:14:03 2018
Response via : Initial Calibration

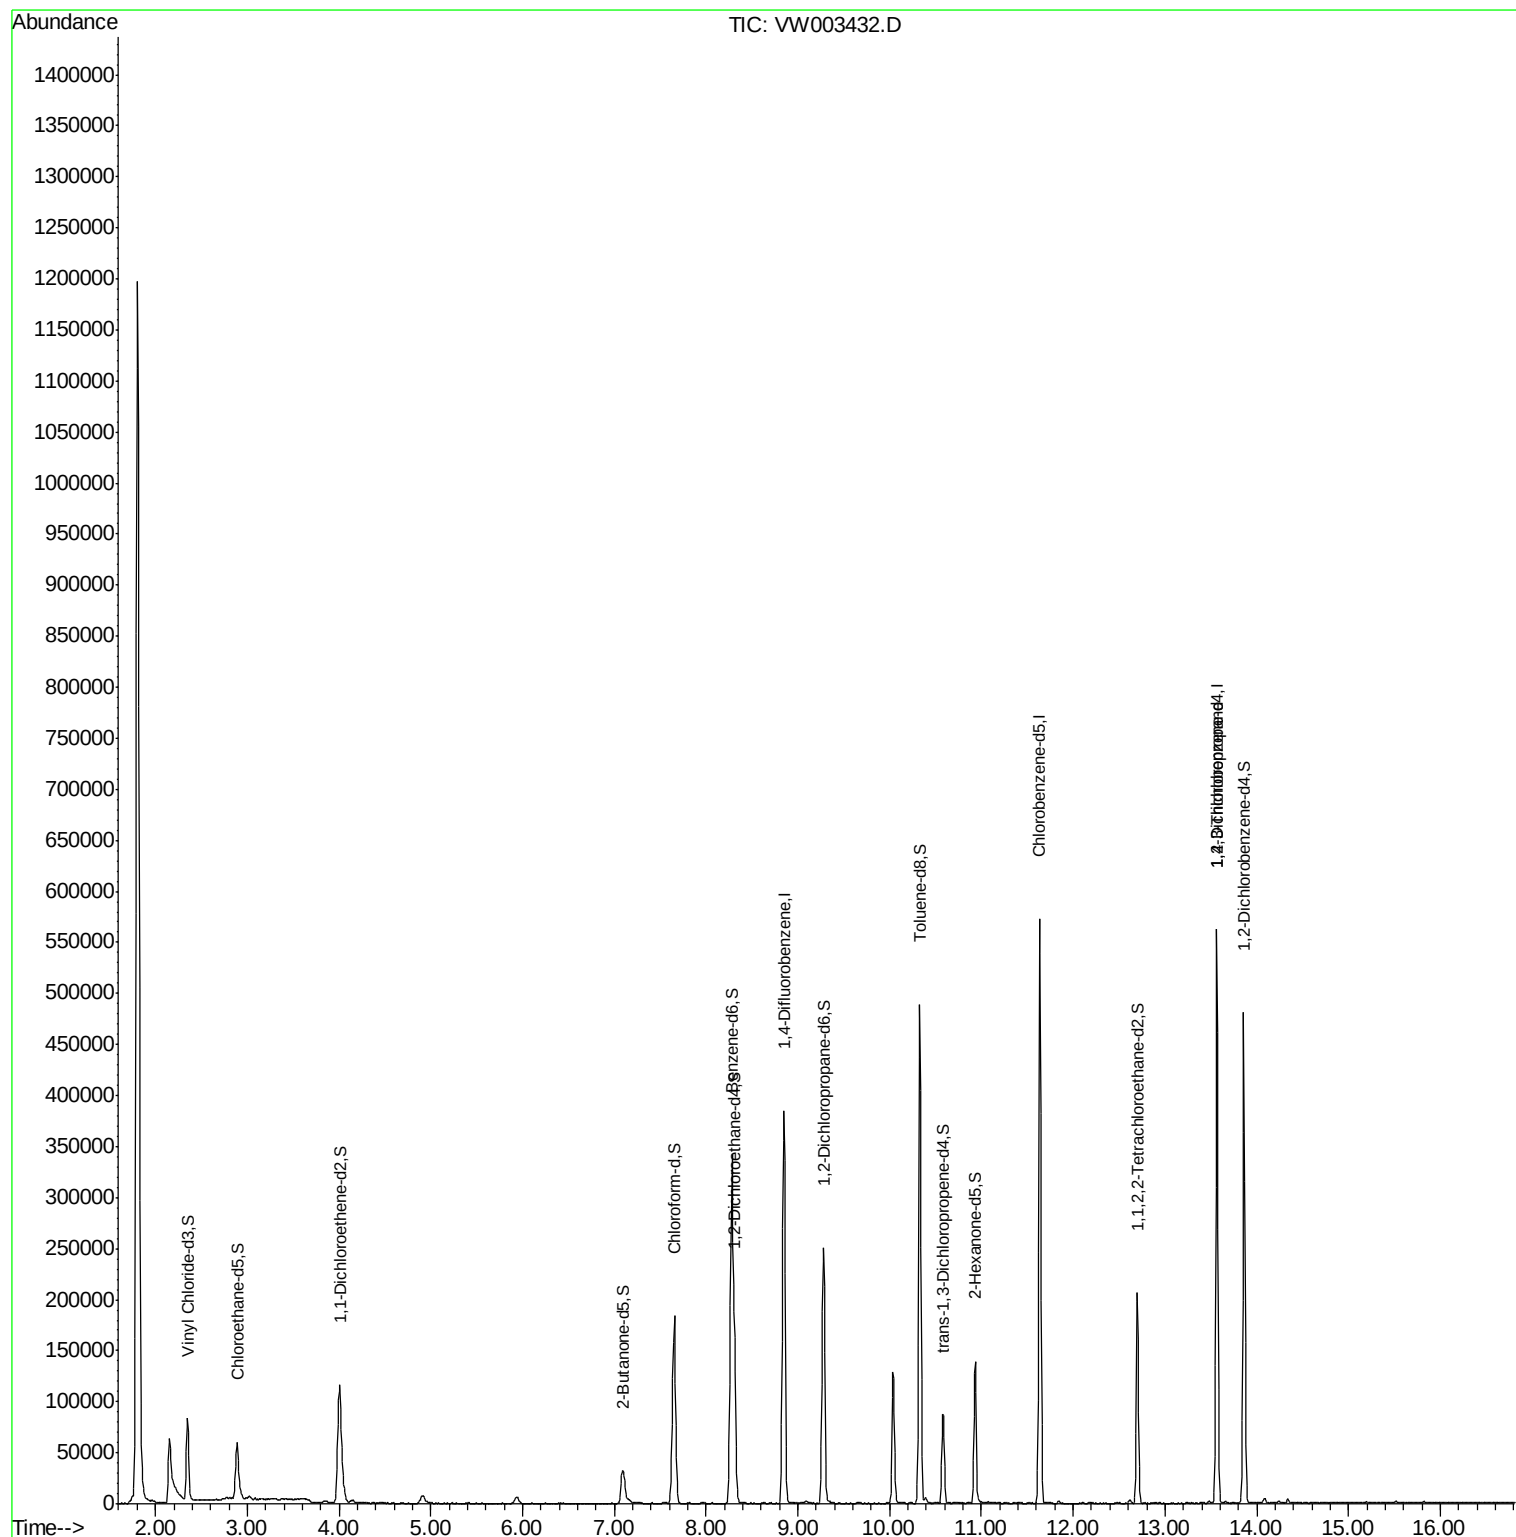

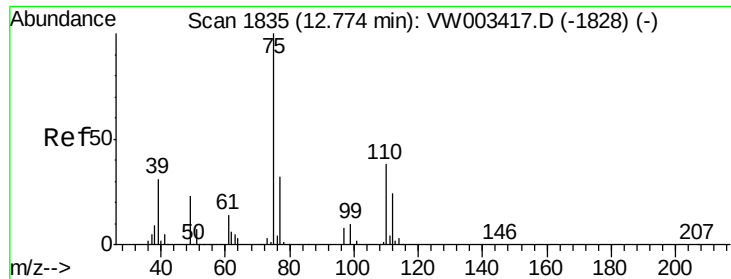

#59

1,2,3-Trichloropropane

Concen: 5.294 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW003432.D

Acq: 22 Jun 2018 17:55

Instrument :

MSVOA_W

ClientSampleId :

DAZ62

Tgt Ion: 75 Resp: 17982

Ion Ratio Lower Upper

75 100

77 39.5 26.0 39.0#

