

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
 Data File : VW003433.D
 Acq On : 22 Jun 2018 18:21
 Operator : SY/AP
 Sample : J3621-11
 Misc : 7.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAZ65

Quant Time: Jun 23 02:16:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 23 02:14:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	322341	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	318636	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	147499	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	83298	19.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.20%
7) Chloroethane-d5	2.89	69	71209	19.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.08%
10) 1,1-Dichloroethene-d2	4.01	63	128397	14.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.16%
20) 2-Butanone-d5	7.09	46	64062	46.51	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.02%
24) Chloroform-d	7.65	84	186985	22.05	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	8.31	65	119232	23.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.64%
29) Benzene-d6	8.27	84	338536	20.02	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.08%
33) 1,2-Dichloropropane-d6	9.28	67	116127	21.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.80%
37) Toluene-d8	10.33	98	311759	19.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.16%
38) trans-1,3-Dichloropropene-	10.58	79	49502	19.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.80%
39) 2-Hexanone-d5	10.93	63	46603	42.60	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.20%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	107598	21.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.44%
61) 1,2-Dichlorobenzene-d4	13.86	152	128057	22.99	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.96%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	13.57	75	19739	5.473	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
Data File : VW003433.D
Acq On : 22 Jun 2018 18:21
Operator : SY/AP
Sample : J3621-11
Misc : 7.17G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAZ65

Quant Time: Jun 23 02:16:49 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 23 02:14:03 2018
Response via : Initial Calibration

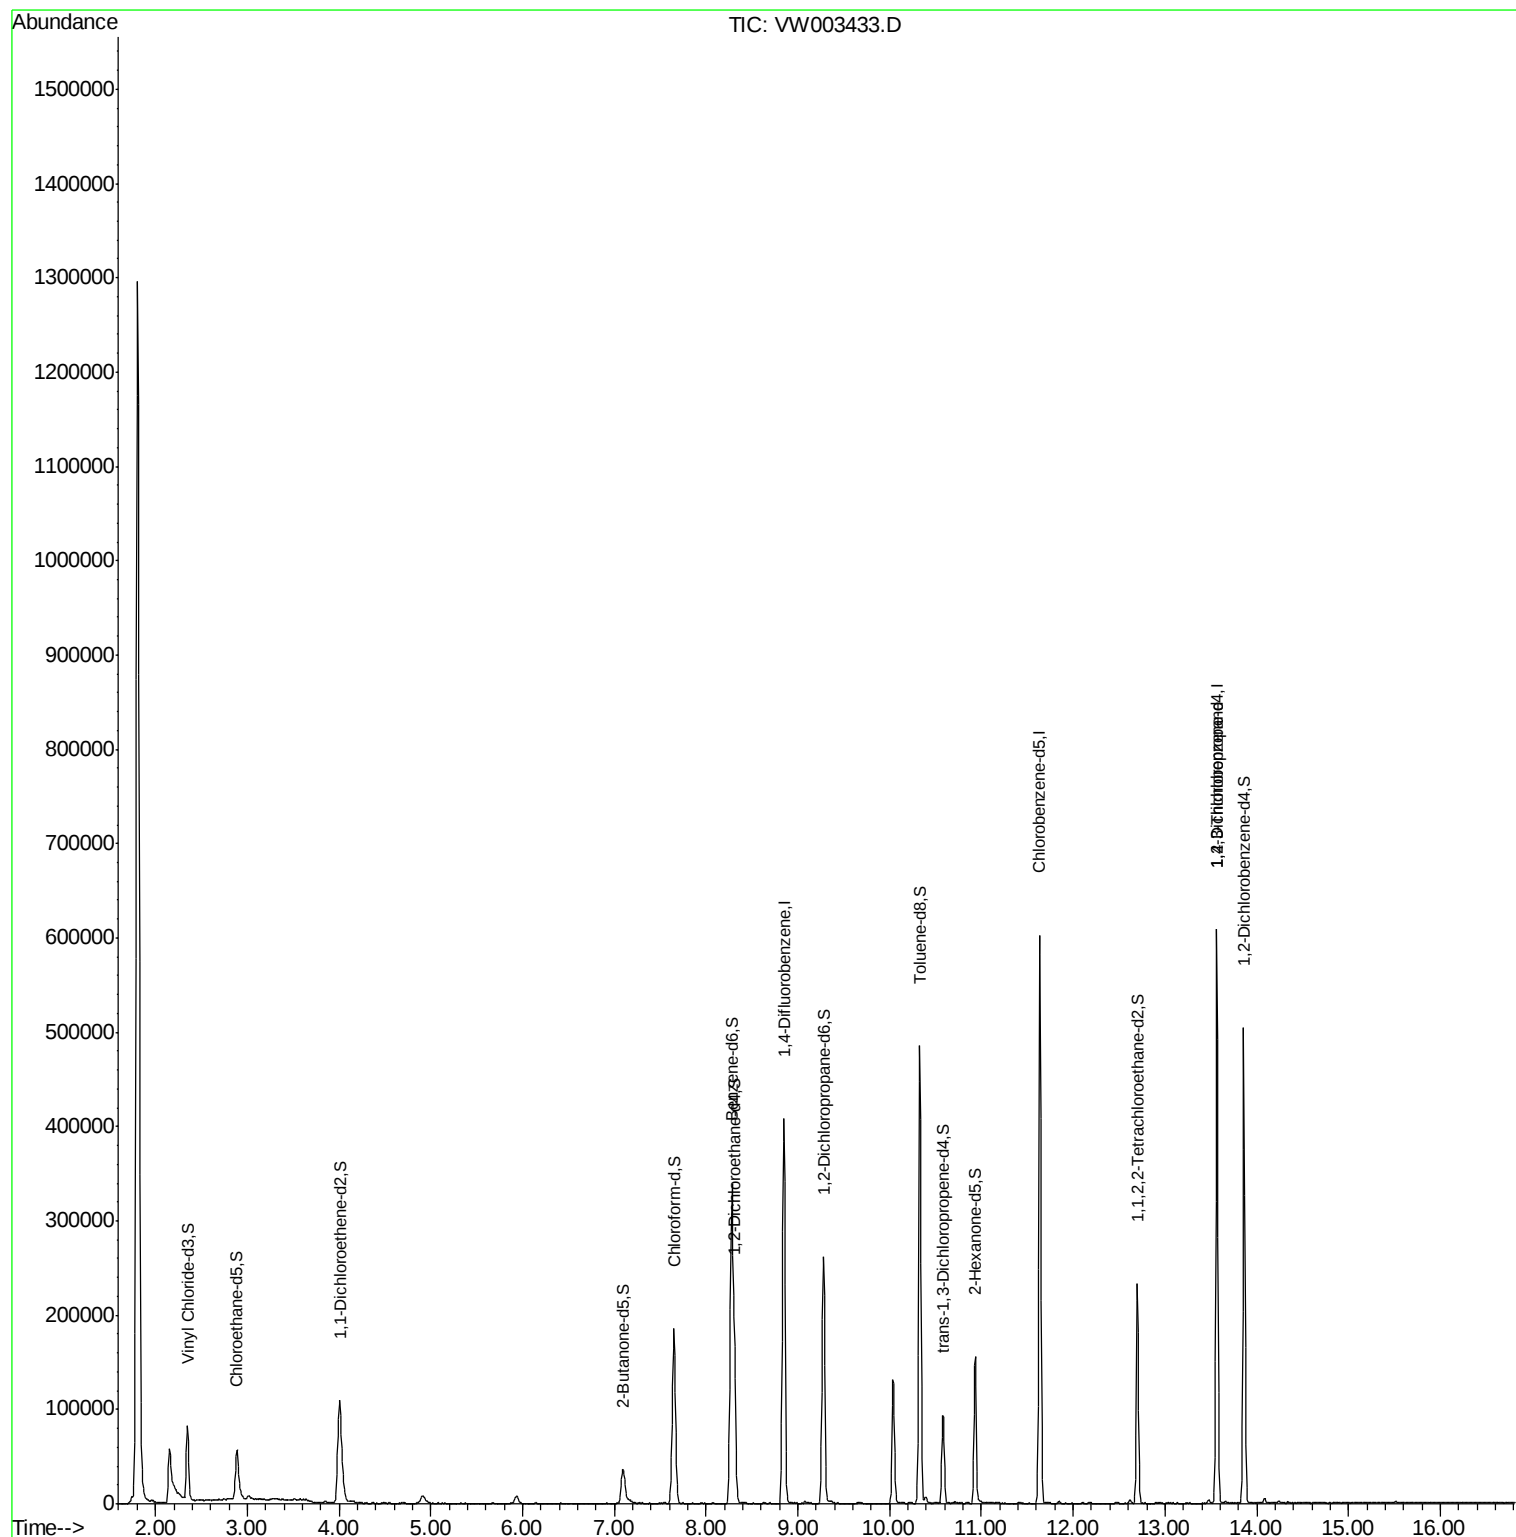

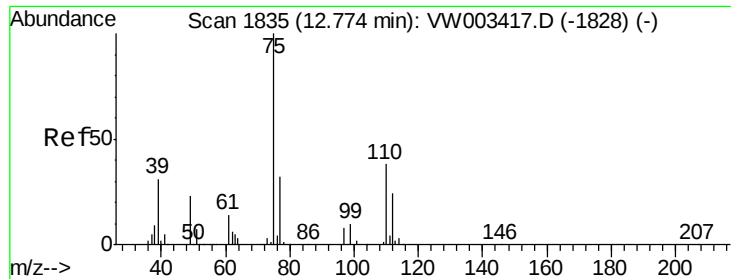

#59

1,2,3-Trichloropropane

Concen: 5.473 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW003433.D

Acq: 22 Jun 2018 18:21

Instrument :

MSVOA_W

ClientSampleId :

DAZ65

Tgt Ion: 75 Resp: 19739

Ion Ratio Lower Upper

75 100

77 36.5 26.0 39.0

