


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
Data File : VW003421.D
Acq On : 22 Jun 2018 12:38
Operator : SY/AP
Sample : J3619-01
Misc : 7.165G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 03:24:45 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 23 02:14:03 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
DAZ63

Manual Integrations
APPROVED

MMDadoda
6/26/2018 12:02:43 PM

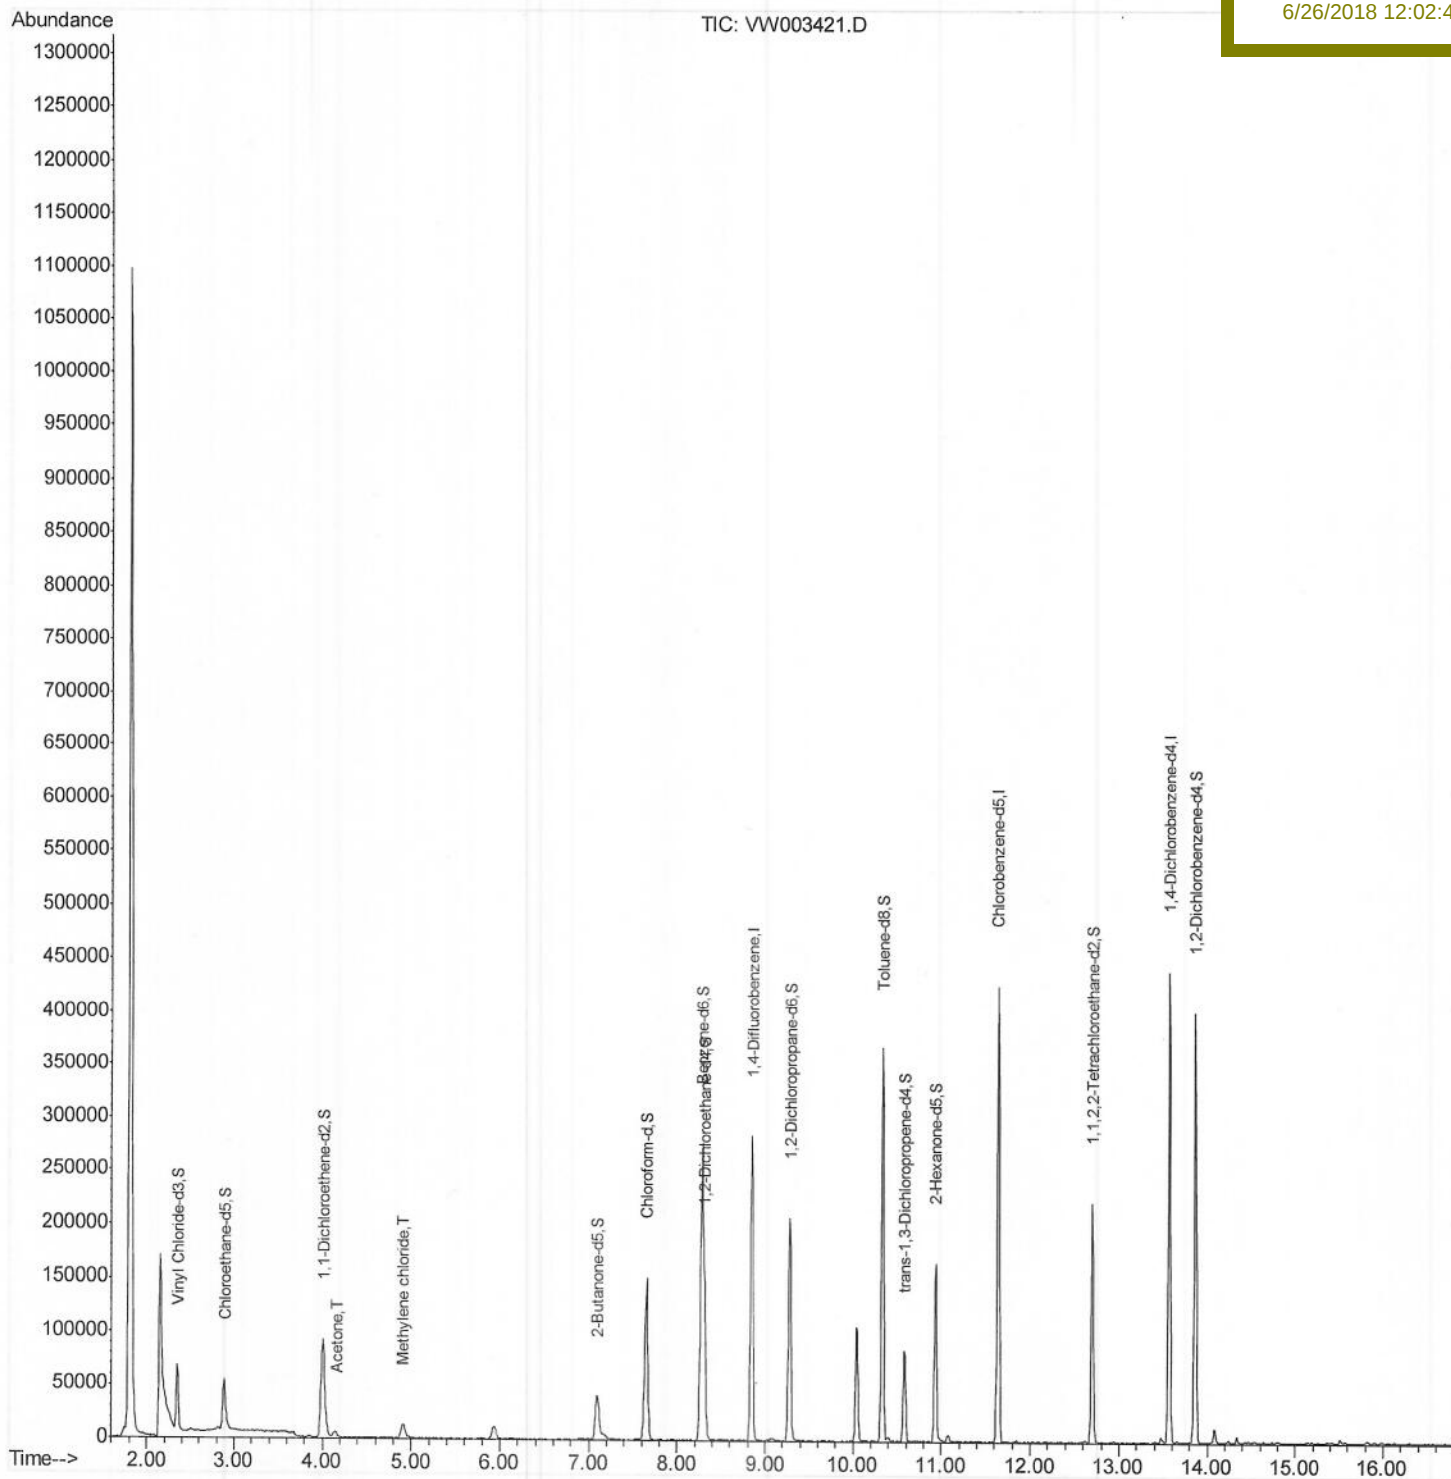

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
 Data File : VW003421.D
 Acq On : 22 Jun 2018 12:38
 Operator : SY/AP
 Sample : J3619-01
 Misc : 7.165G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 02:15:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 23 02:14:03 2018
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 ClientSampled :
 DAZ63

Manual Integrations
 APPROVED

MMDadoda
 6/26/2018 12:02:43 PM

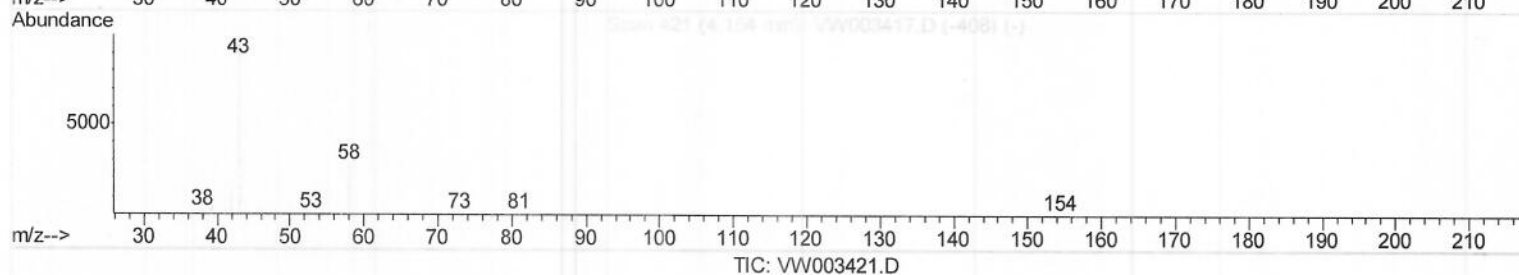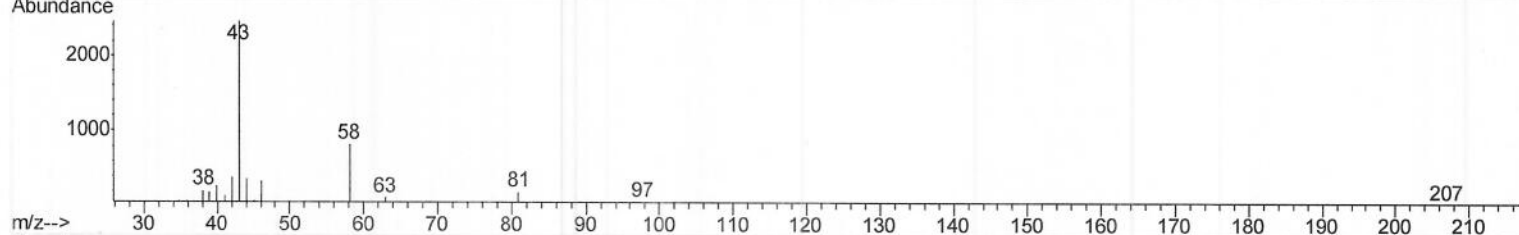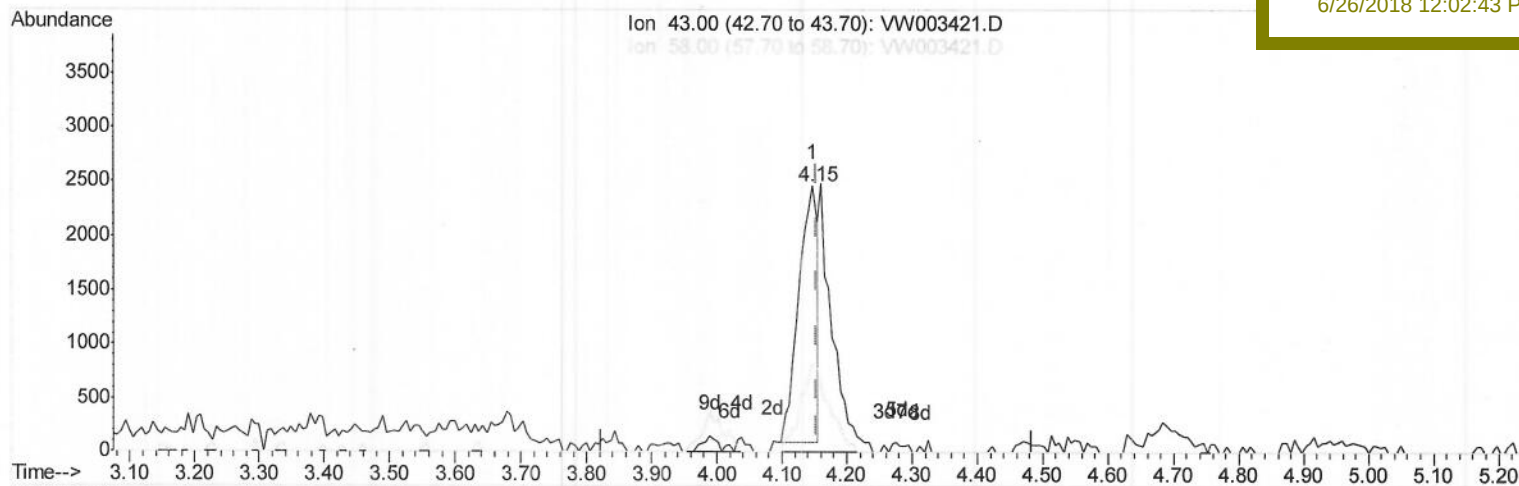

(13) Acetone (T)

4.148min (-0.006) 4.59ug/L

response 4645

Ion	Exp%	Act%
43.00	100	100
58.00	29.30	53.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
Data File : VW003421.D
Acq On : 22 Jun 2018 12:38
Operator : SY/AP
Sample : J3619-01
Misc : 7.165G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 02:15:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 23 02:14:03 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sample Id :
DAZ63

Manual Integrations
APPROVED

MMDadoda
6/26/2018 12:02:43 PM

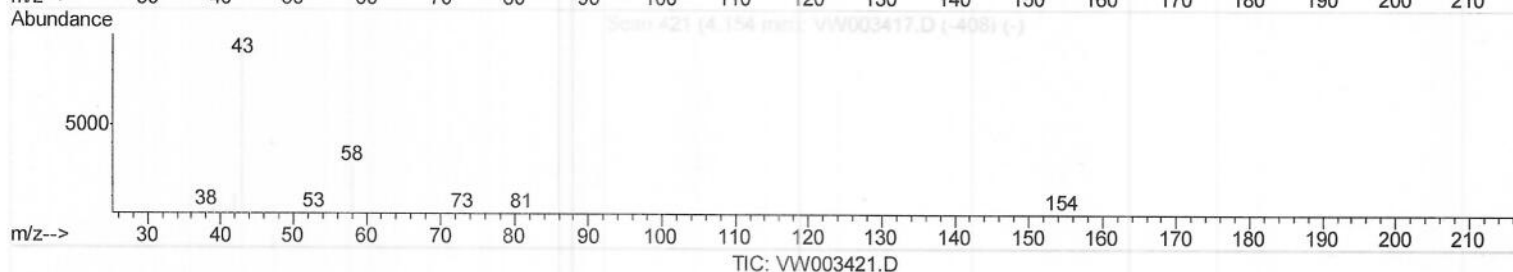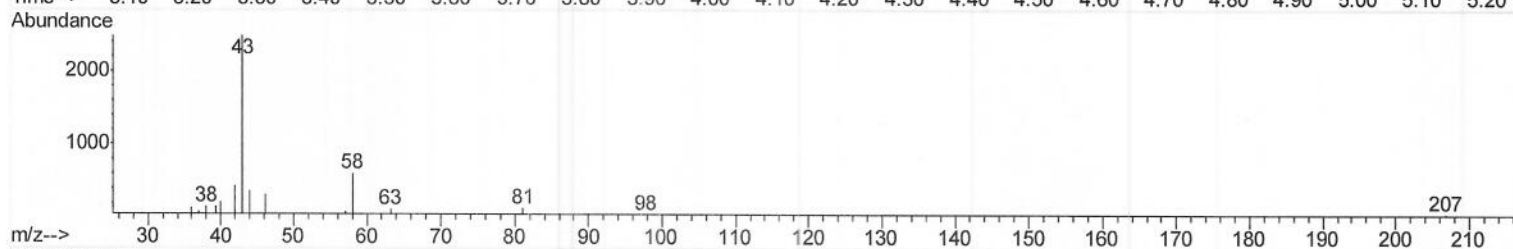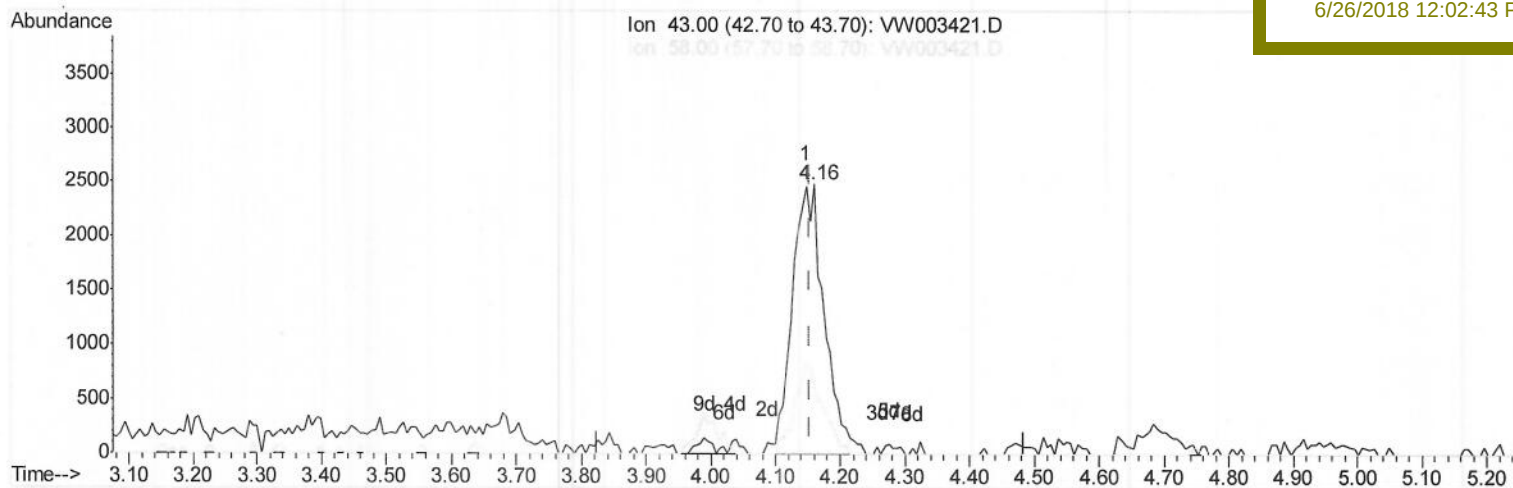

(13) Acetone (T)

4.160min (+0.006) 8.49ug/L m

response 8590

Ion	Exp%	Act%
43.00	100	100
58.00	29.30	29.00
0.00	0.00	0.00
0.00	0.00	0.00

MD
06/30/18

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062218\
 Data File : VW003421.D
 Acq On : 22 Jun 2018 12:38
 Operator : SY/AP
 Sample : J3619-01
 Misc : 7.165G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 DAZ63

Quant Time: Jun 23 03:24:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 23 02:14:03 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/26/2018 12:02:43 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	222052	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	228938	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	108220	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	67030	22.26	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.04%		
7) Chloroethane-d5	2.89	69	58328	23.21	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.84%		
10) 1,1-Dichloroethene-d2	4.01	63	101725	17.01	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	68.04%		
20) 2-Butanone-d5	7.09	46	70787	74.60	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	149.20%#		
24) Chloroform-d	7.65	84	147600	25.27	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	101.08%		
26) 1,2-Dichloroethane-d4	8.31	65	103831	29.91	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	119.64%		
29) Benzene-d6	8.28	84	268832	22.13	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.52%		
33) 1,2-Dichloropropane-d6	9.27	67	93557	24.33	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.32%		
37) Toluene-d8	10.33	98	240765	20.73	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.92%		
38) trans-1,3-Dichloropropene-	10.58	79	42427	23.50	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	94.00%		
39) 2-Hexanone-d5	10.93	63	48676	61.93	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	123.86%		
48) 1,1,2,2-Tetrachloroethane-	12.70	84	104901	29.32	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	117.28%		
61) 1,2-Dichlorobenzene-d4	13.87	152	104809	25.64	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.56%		

Target Compounds

13) Acetone	4.16	43	8590m)	8.492	ug/L	Qvalue
16) Methylene chloride	4.90	84	10261	3.354	ug/L	95

MD
 06/30/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed