
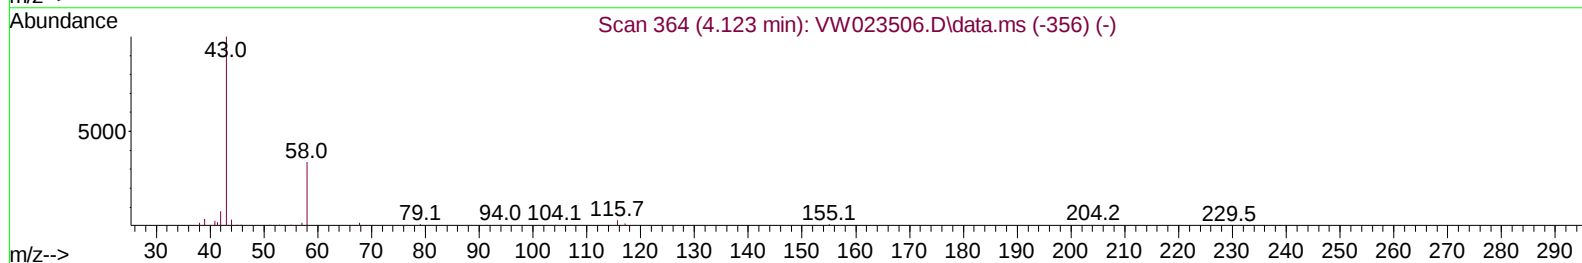
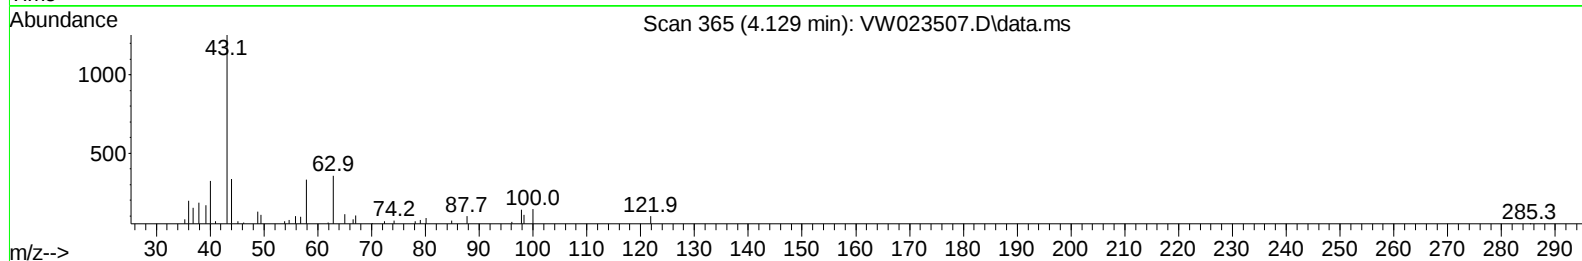


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
 Data File : VW023507.D
 Acq On : 22 Jun 2022 13:38
 Operator : SY/VA
 Sample : VW0622SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:22:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 23 01:21:32 2022
 Response via : Initial Calibration

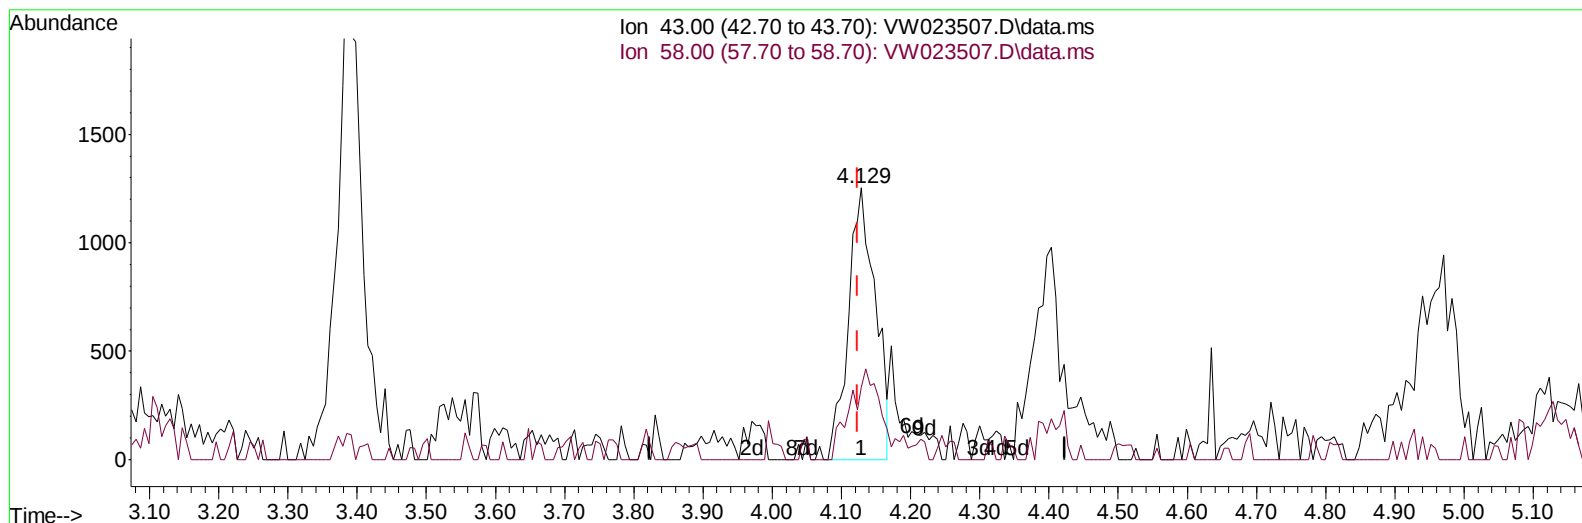

TIC: VW023507.D\data.ms

(13) Acetone (T)




4.129min (+ 0.006) 3.96 ug/L

response 3384

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	23.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
Data File : VW023507.D
Acq On : 22 Jun 2022 13:38
Operator : SY/VA
Sample : VW0622SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:22:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 23 01:21:32 2022
Response via : Initial Calibration

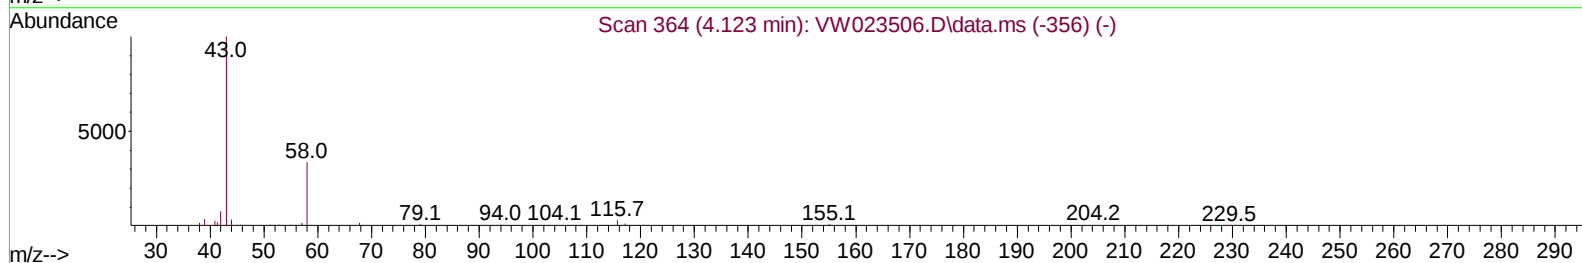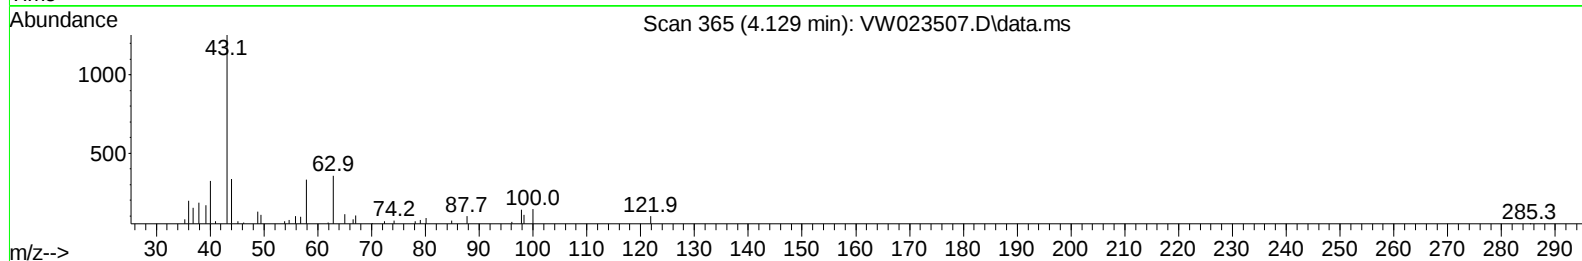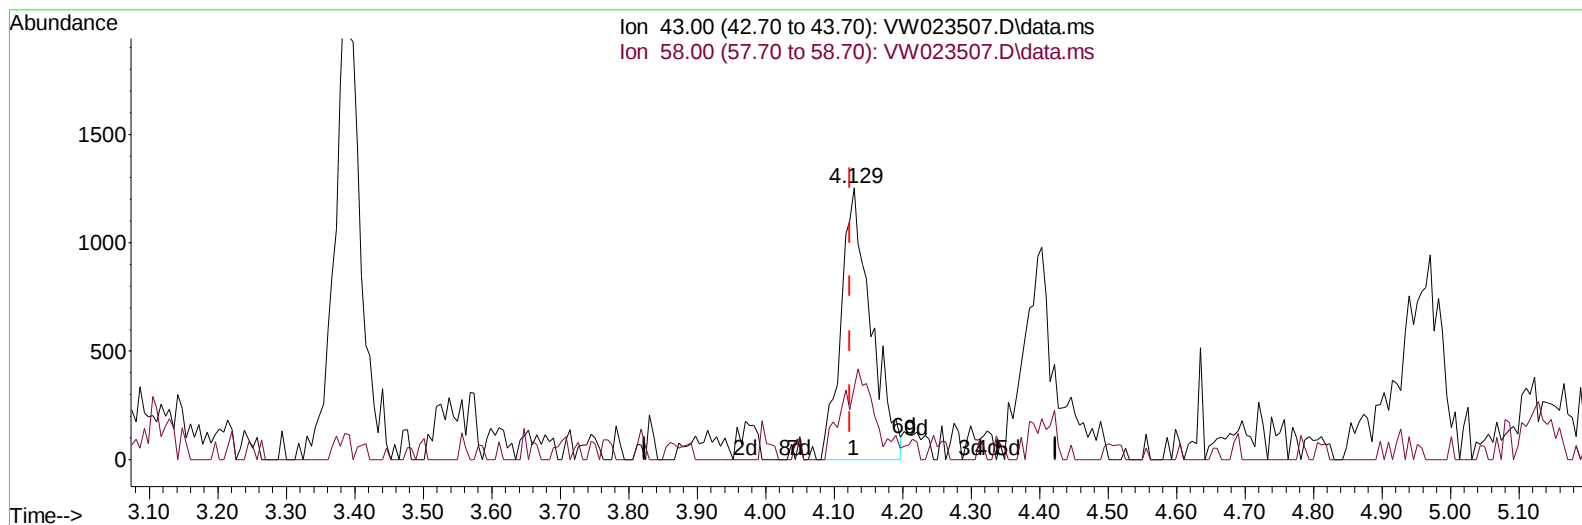

TIC: VW023507.D\data.ms

(13) Acetone (T)




4.129min (+ 0.006) 4.49 ug/L m

response 3842

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	20.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
 Data File : VW023507.D
 Acq On : 22 Jun 2022 13:38
 Operator : SY/VA
 Sample : VW0622SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:22:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 23 01:21:32 2022
 Response via : Initial Calibration

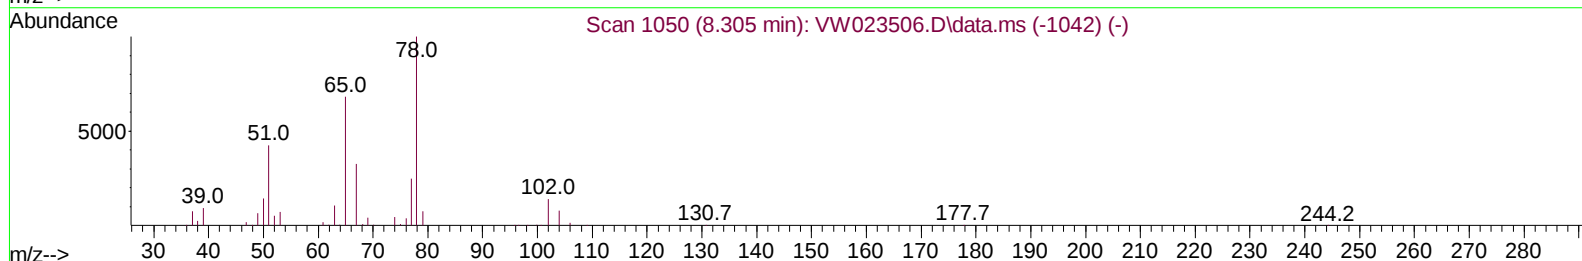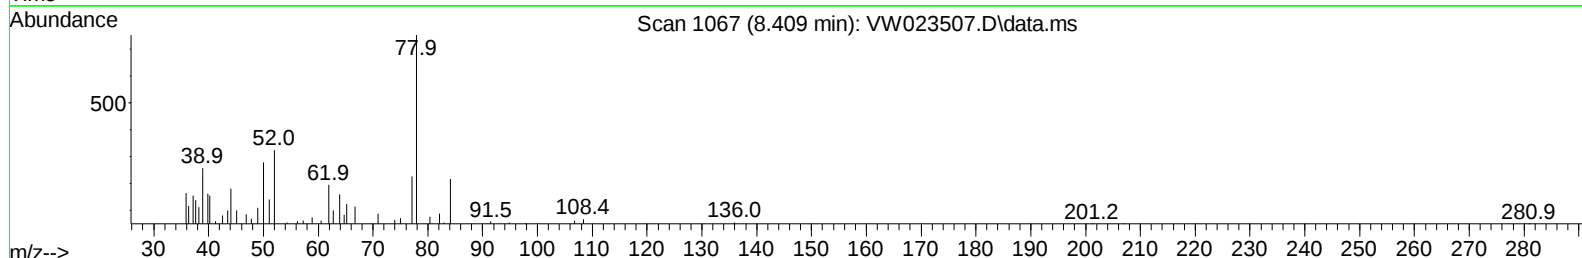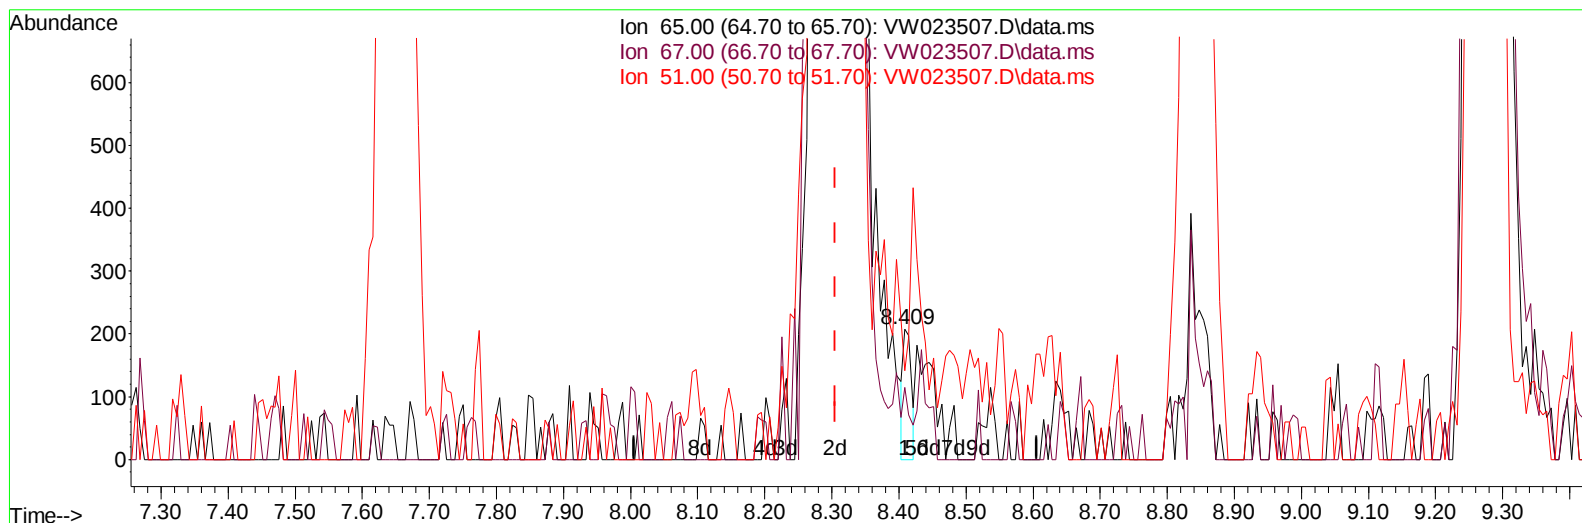




TIC: VW023507.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.409min (+ 0.103) 0.03 ug/L****response 178**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	60.11
51.00	92.30	98.88
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
 Data File : VW023507.D
 Acq On : 22 Jun 2022 13:38
 Operator : SY/VA
 Sample : VW0622SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:22:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 23 01:21:32 2022
 Response via : Initial Calibration

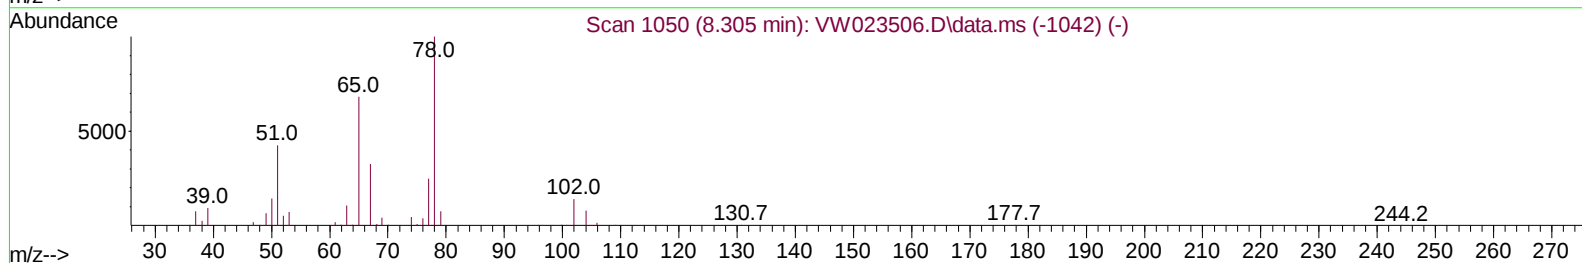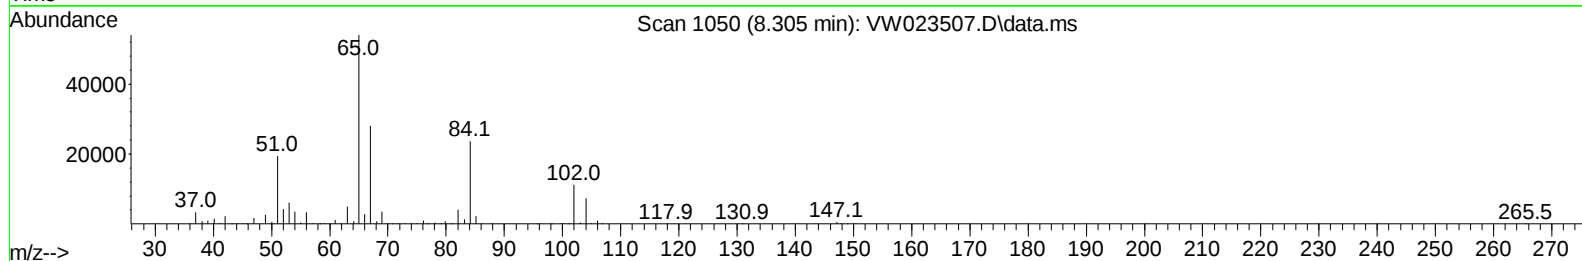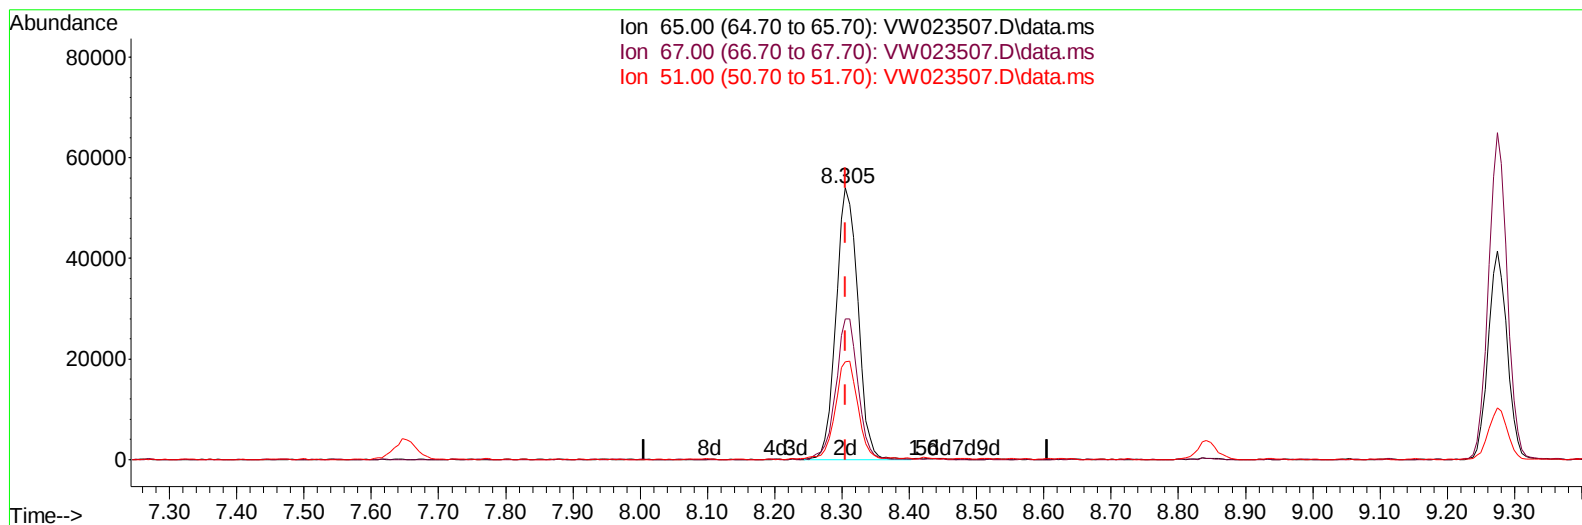

TIC: VW023507.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.305min (-0.000) 22.46 ug/L m****response 121822**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.09#
51.00	92.30	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
 Data File : VW023507.D
 Acq On : 22 Jun 2022 13:38
 Operator : SY/VA
 Sample : VW0622SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:22:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 23 01:21:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	365785	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	346494	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	160116	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	105426	18.142	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.560%		
7) Chloroethane-d5	2.885	69	74624	17.469	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.880%		
11) 1,1-Dichloroethene-d2	4.019	63	120204	14.819	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.280%		
21) 2-Butanone-d5	7.074	46	63016	53.111	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.220%		
24) Chloroform-d	7.653	84	220580	21.906	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.640%		
26) 1,2-Dichloroethane-d4	8.305	65	121822m	22.464	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.840%		
32) Benzene-d6	8.275	84	401169	21.836	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.360%		
36) 1,2-Dichloropropane-d6	9.274	67	125847	23.250	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.000%		
41) Toluene-d8	10.323	98	379791	21.164	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.640%		
43) trans-1,3-Dichloroprop...	10.579	79	53212	21.539	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.160%		
47) 2-Hexanone-d5	10.927	63	48063	55.570	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.140%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	118327	23.406	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152	135285	23.405	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	93.640%		
Target Compounds						
13) Acetone	4.129	43	3842m	4.494	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
Data File : VW023507.D
Acq On : 22 Jun 2022 13:38
Operator : SY/VA
Sample : VW0622SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:22:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 23 01:21:32 2022
Response via : Initial Calibration

