

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
 Data File : VW023508.D
 Acq On : 22 Jun 2022 14:18
 Operator : SY/VA
 Sample : N3425-09
 Misc : 4.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF1

Quant Time: Jun 23 01:22:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 23 01:21:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	398940	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	379922	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	180710	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	97055	15.313	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.240%
7) Chloroethane-d5	2.885	69	78433	16.835	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.320%
11) 1,1-Dichloroethene-d2	4.013	63	116891	13.213	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.840%
21) 2-Butanone-d5	7.074	46	77349	59.773	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.540%
24) Chloroform-d	7.647	84	224520	20.445	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.760%
26) 1,2-Dichloroethane-d4	8.305	65	131088	22.164	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.640%
32) Benzene-d6	8.275	84	404874	20.098	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.400%
36) 1,2-Dichloropropane-d6	9.275	67	127976	21.563	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.240%
41) Toluene-d8	10.323	98	372184	18.916	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.680%
43) trans-1,3-Dichloroprop...	10.579	79	54198	20.008	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.040%
47) 2-Hexanone-d5	10.921	63	59841	63.100	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.200%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	139286	25.128	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	141909	21.753	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.000%
Target Compounds						
13) Acetone	4.129	43	5095m	5.465	ug/L	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
Data File : VW023508.D
Acq On : 22 Jun 2022 14:18
Operator : SY/VA
Sample : N3425-09
Misc : 4.80g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF1

Quant Time: Jun 23 01:22:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 23 01:21:32 2022
Response via : Initial Calibration

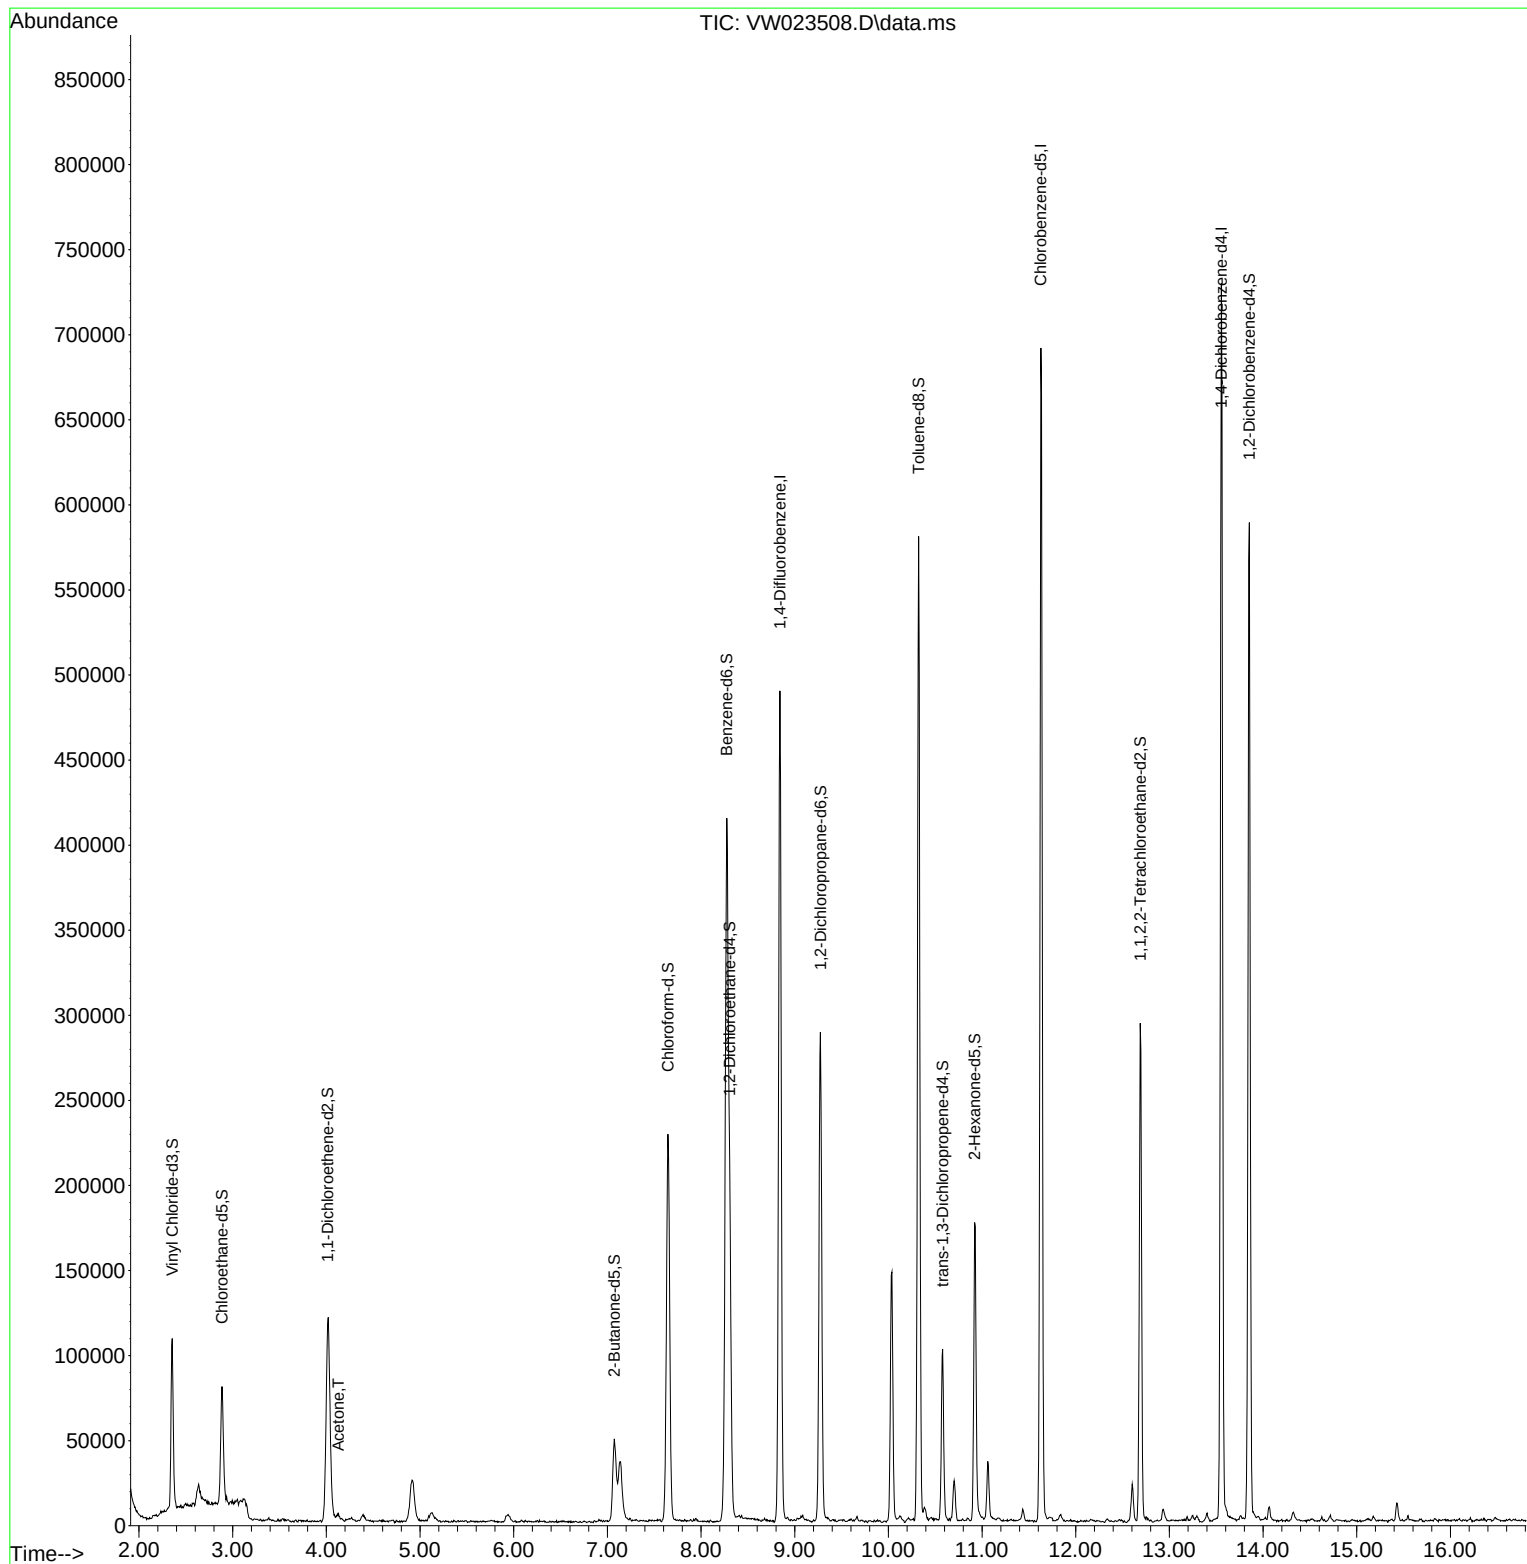

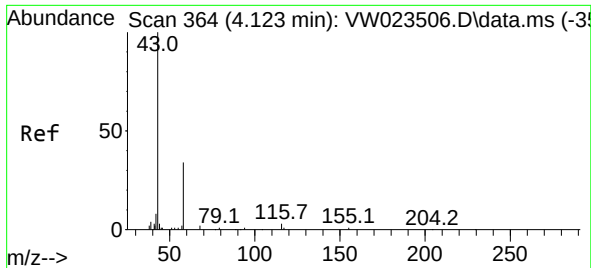

#13
 Acetone
 Concen: 5.465 ug/L m
 RT: 4.129 min Scan# 3
 Delta R.T. 0.006 min
 Lab File: VW023508.D
 Acq: 22 Jun 2022 14:18

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF1

Tgt Ion: 43 Resp: 5095
 Ion Ratio Lower Upper
 43 100
 58 20.6 0.0 64.0

