

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
 Data File : VW023510.D
 Acq On : 22 Jun 2022 15:21
 Operator : SY/VA
 Sample : VIBLK499
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK499

Quant Time: Jun 23 01:22:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 23 01:21:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	353884	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	338476	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155862	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	104552	18.597	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.400%
7) Chloroethane-d5	2.879	69	70885	17.152	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.600%
11) 1,1-Dichloroethene-d2	4.013	63	114352	14.572	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.280%
21) 2-Butanone-d5	7.080	46	56805	49.486	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.980%
24) Chloroform-d	7.647	84	209794	21.536	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.160%
26) 1,2-Dichloroethane-d4	8.305	65	114053	21.739	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.960%
32) Benzene-d6	8.274	84	382050	21.288	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.160%
36) 1,2-Dichloropropane-d6	9.274	67	118075	22.331	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.320%
41) Toluene-d8	10.323	98	354035	20.196	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	10.579	79	49701	20.594	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.360%
47) 2-Hexanone-d5	10.920	63	43371	51.333	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.660%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111751	22.629	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.520%
66) 1,2-Dichlorobenzene-d4	13.847	152	126895	22.553	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.200%
Target Compounds						
13) Acetone	4.135	43	3669	4.436	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062222\
Data File : VW023510.D
Acq On : 22 Jun 2022 15:21
Operator : SY/VA
Sample : VIBLK499
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK499

Quant Time: Jun 23 01:22:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 23 01:21:32 2022
Response via : Initial Calibration

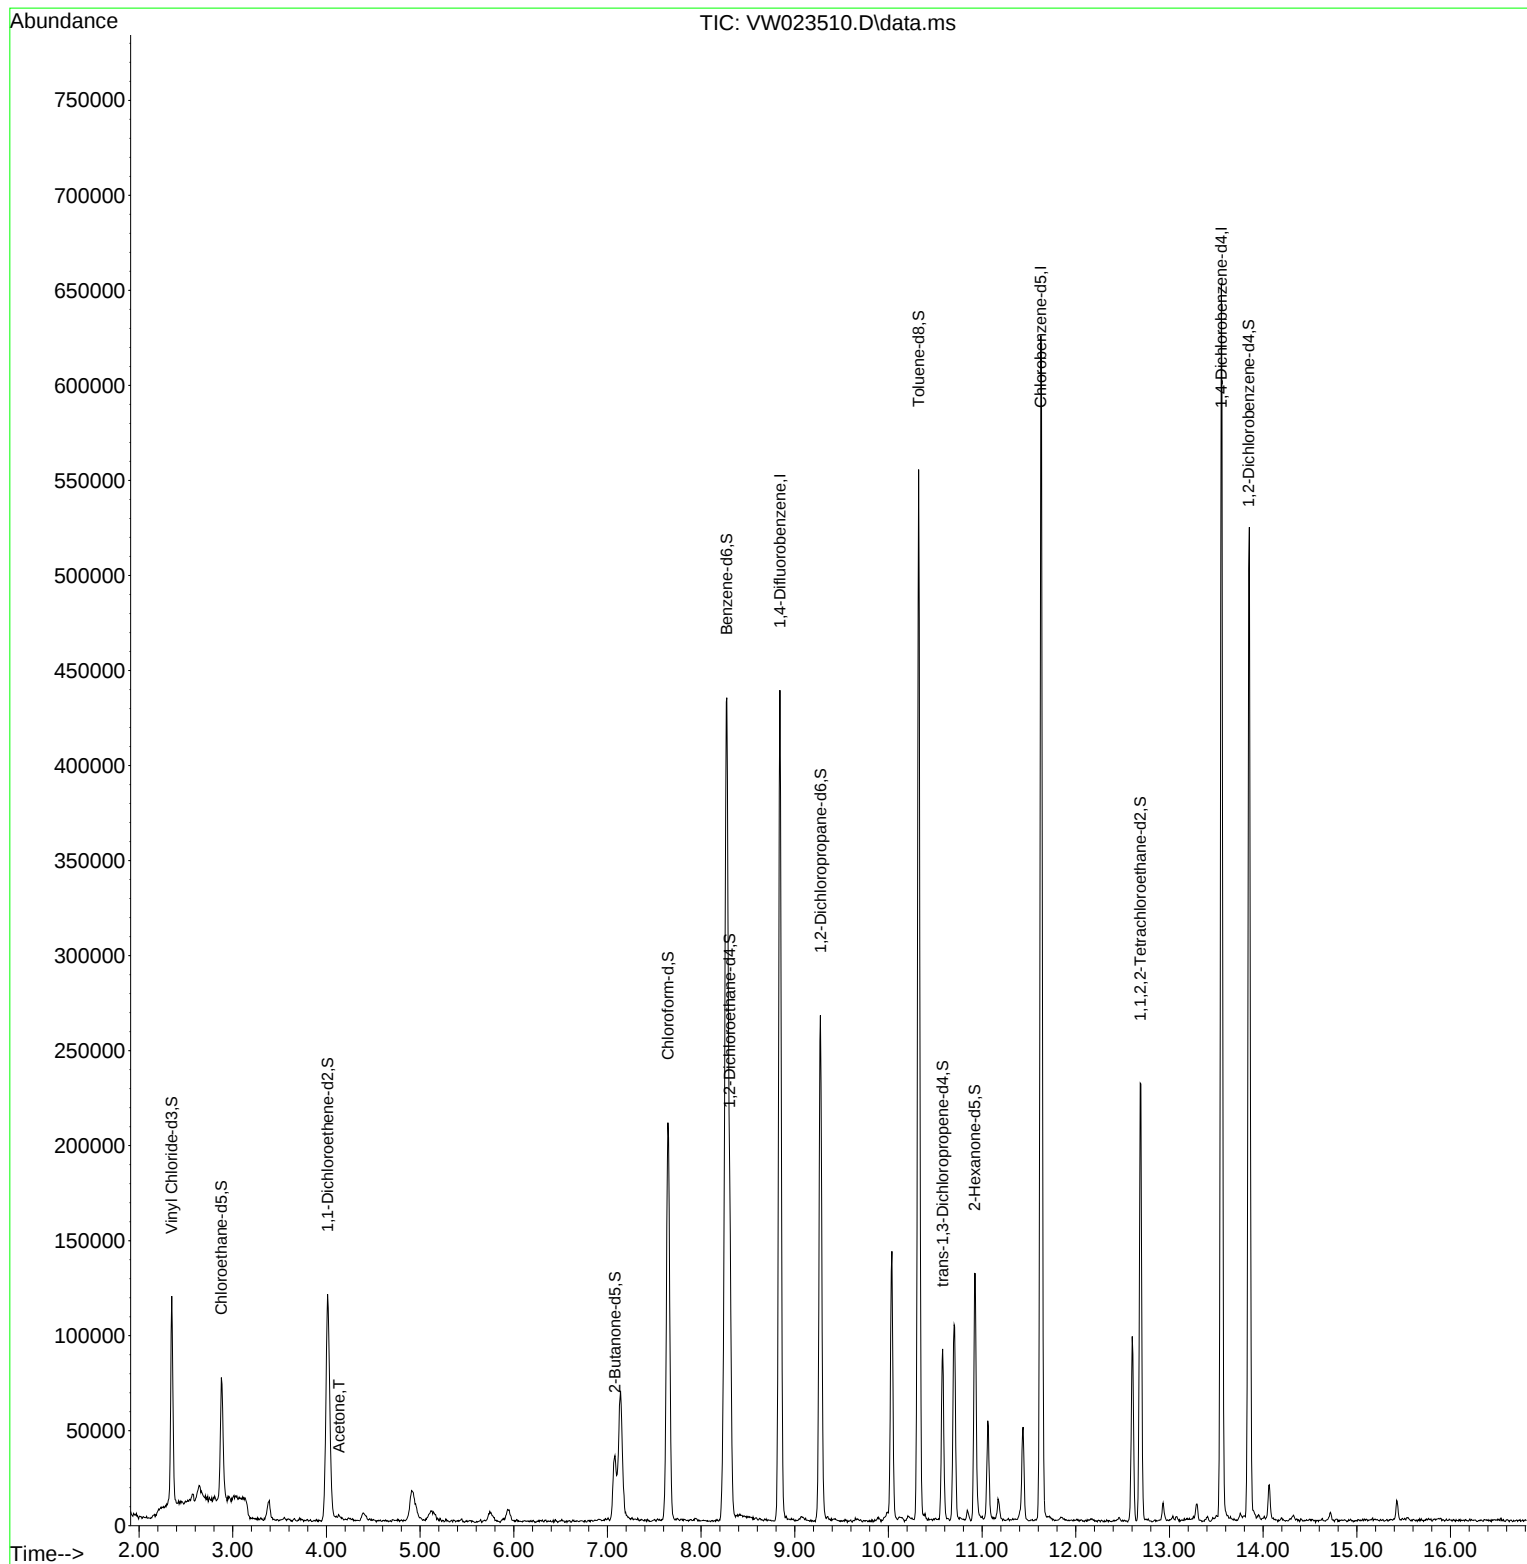

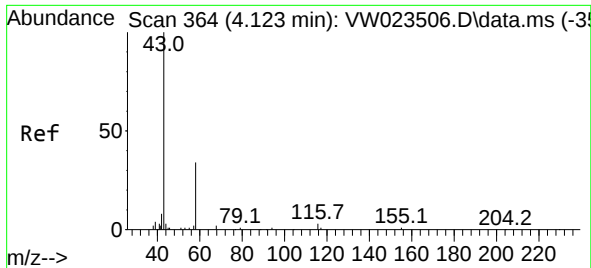

#13
 Acetone
 Concen: 4.436 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023510.D
 Acq: 22 Jun 2022 15:21

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK499

Tgt Ion: 43 Resp: 3669
 Ion Ratio Lower Upper
 43 100
 58 27.1 0.0 64.0

