


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062418\
 Data File : VW003527.D
 Acq On : 24 Jun 2018 23:42
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
 Title : SW846 8260
 Last Update : Sat Jun 16 05:18:54 2018

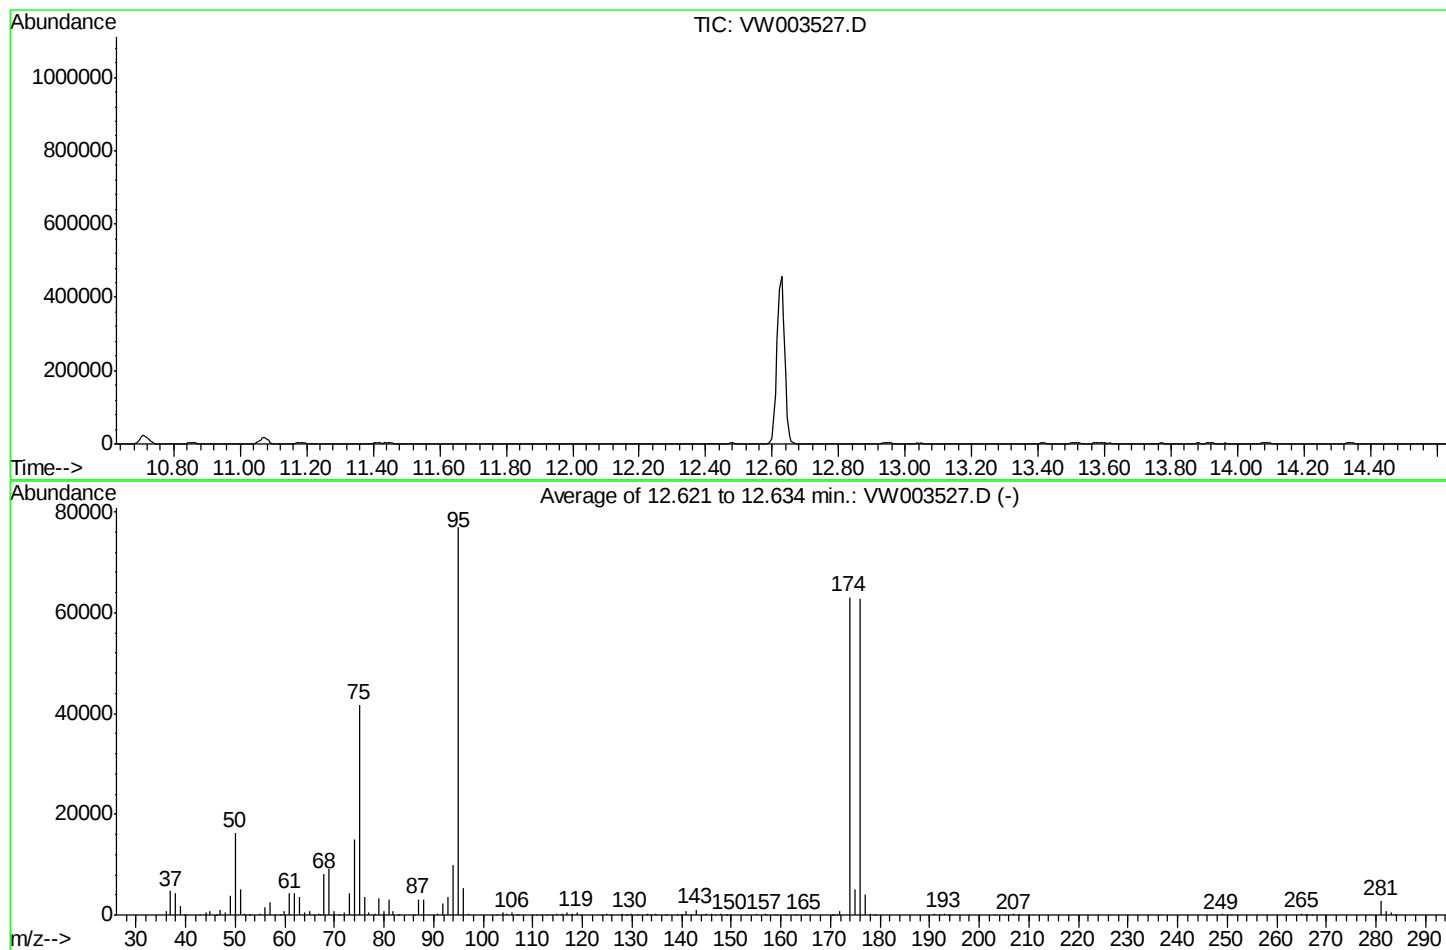

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	16324	PASS
75	95	30	60	54.2	41714	PASS
95	95	100	100	100.0	76944	PASS
96	95	5	9	6.8	5218	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.0	63085	PASS
175	174	5	9	7.9	5009	PASS
176	174	95	101	99.7	62874	PASS
177	176	5	9	6.6	4131	PASS