




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062422\
 Data File : VW023514.D
 Acq On : 24 Jun 2022 11:19
 Operator : SY/VA
 Sample : VW0624SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK532

Manual IntegrationsAPPROVED

Quant Time: Jun 24 23:30:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 24 23:29:48 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/25/2022
 Supervised By :Mahesh Dadoda 06/30/2022

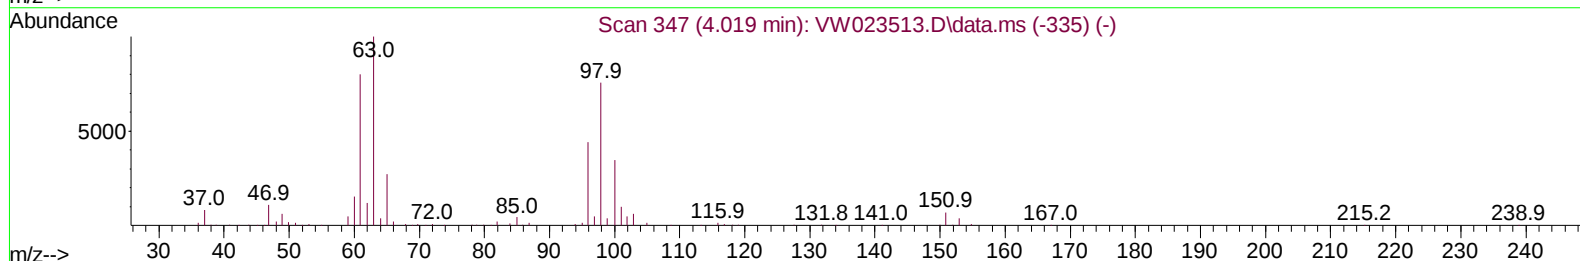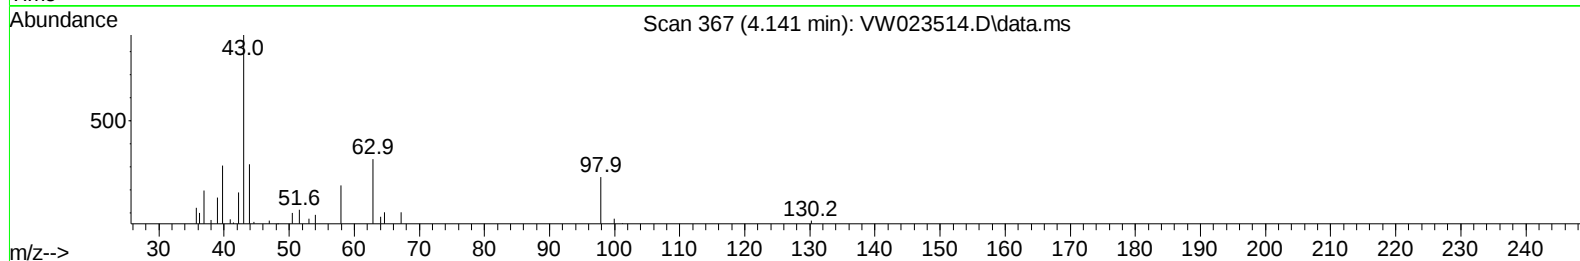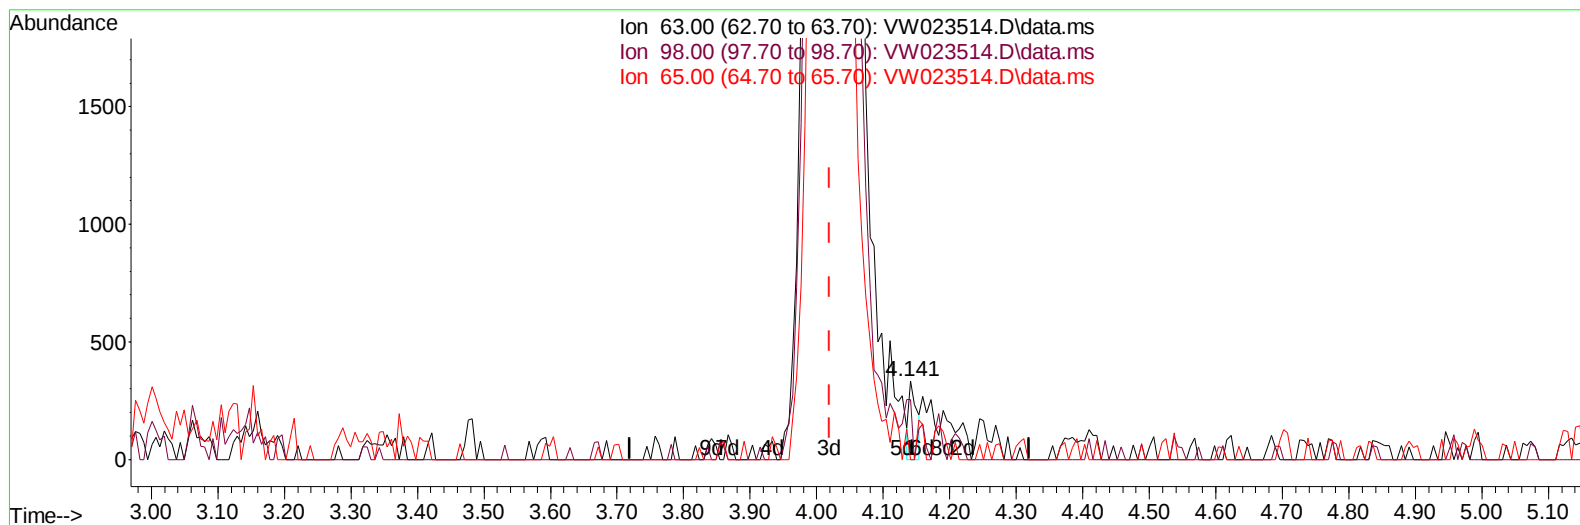

TIC: VW023514.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.141min (+ 0.122) 0.03 ug/L

response 277

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	87.36
65.00	23.30	17.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062422\
 Data File : VW023514.D
 Acq On : 24 Jun 2022 11:19
 Operator : SY/VA
 Sample : VW0624SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK532

Manual IntegrationsAPPROVED

Quant Time: Jun 24 23:30:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 24 23:29:48 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/25/2022
 Supervised By :Mahesh Dadoda 06/30/2022

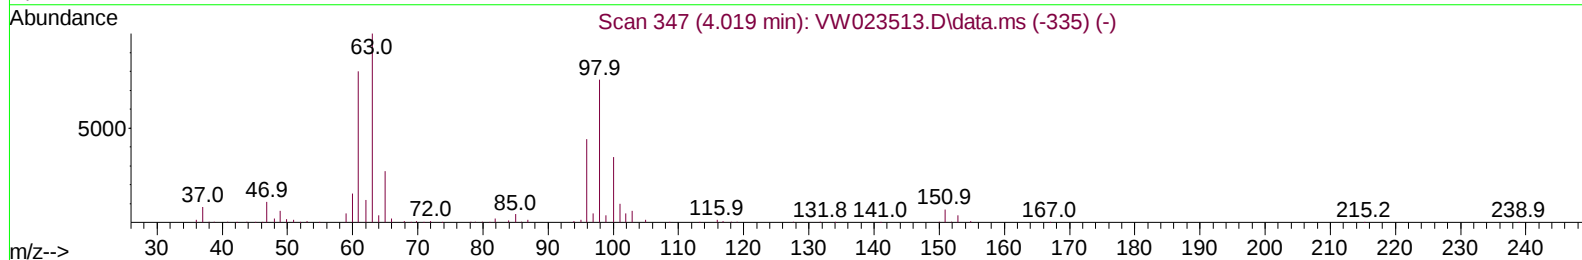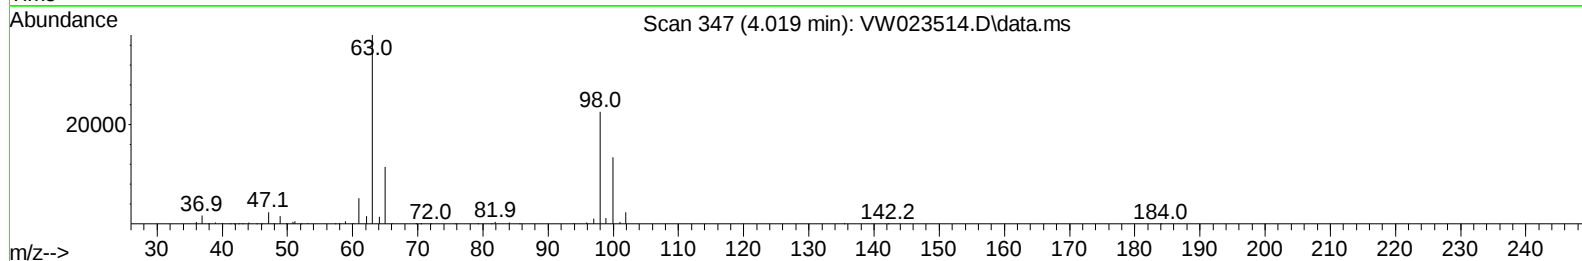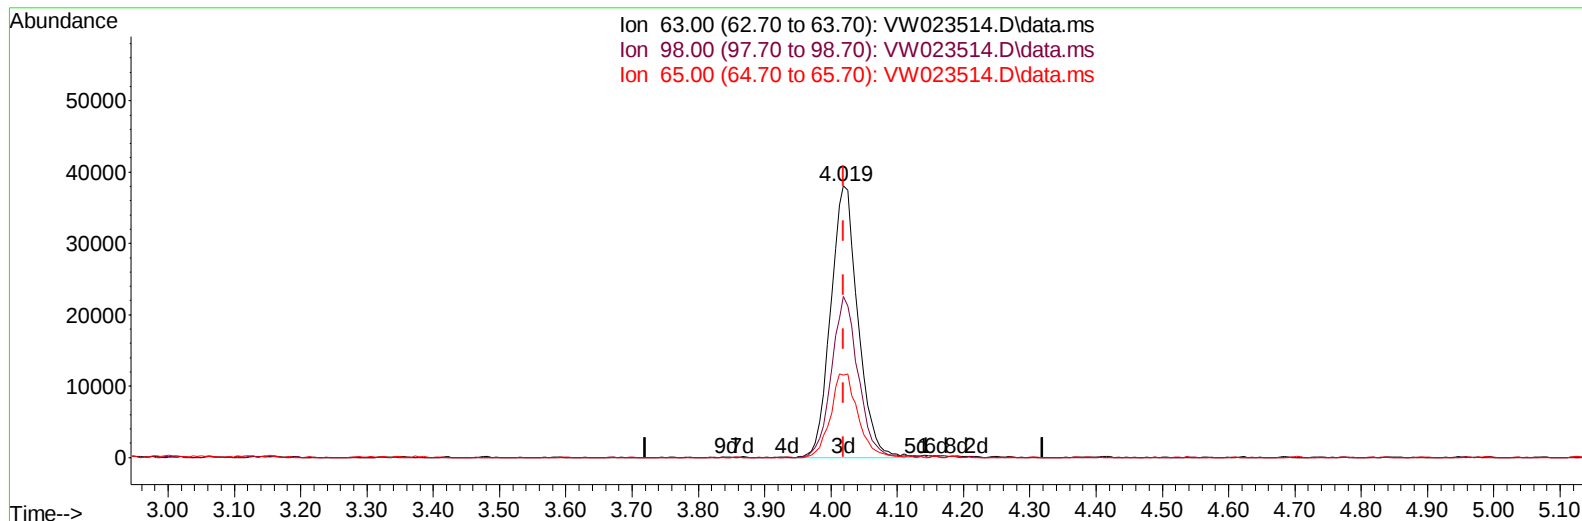

TIC: VW023514.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 13.49 ug/L m

response 109128

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.22#
65.00	23.30	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062422\
 Data File : VW023514.D
 Acq On : 24 Jun 2022 11:19
 Operator : SY/VA
 Sample : VW0624SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK532

Manual IntegrationsAPPROVED

Quant Time: Jun 24 23:30:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 24 23:29:48 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/25/2022
 Supervised By :Mahesh Dadoda 06/30/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	364770	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	340057	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	160517	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	95474	16.475	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.920%	
7) Chloroethane-d5	2.885	69	71899	16.878	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.520%	
11) 1,1-Dichloroethene-d2	4.019	63	109128m	13.491	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.960%	
21) 2-Butanone-d5	7.073	46	53007	44.799	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.600%	
24) Chloroform-d	7.653	84	210129	20.927	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	83.720%	
26) 1,2-Dichloroethane-d4	8.305	65	111073	20.539	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	82.160%	
32) Benzene-d6	8.274	84	377910	20.959	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.840%	
36) 1,2-Dichloropropane-d6	9.274	67	116300	21.893	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.560%	
41) Toluene-d8	10.323	98	349284	19.833	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.320%	
43) trans-1,3-Dichloroprop...	10.579	79	48190	19.875	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.520%	
47) 2-Hexanone-d5	10.926	63	40886	48.167	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.340%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	105379	21.240	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	129659	22.376	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.520%	
Target Compounds						
13) Acetone	4.129	43	2738	3.212	ug/L	Qvalue 62

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062422\
Data File : VW023514.D
Acq On : 24 Jun 2022 11:19
Operator : SY/VA
Sample : VW0624SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK532

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/25/2022
Supervised By :Mahesh Dadoda 06/30/2022

Quant Time: Jun 24 23:30:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 24 23:29:48 2022
Response via : Initial Calibration

