

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062422\
 Data File : VW023514.D
 Acq On : 24 Jun 2022 11:19
 Operator : SY/VA
 Sample : VW0624SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK532

Manual Integrations
 APPROVED

Reviewed By : Semsettin
 Yesilyurt

Quant Time: Jun 24 23:30:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 24 23:29:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	364770	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	340057	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	160517	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	95474	16.475	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	65.920%		
7) Chloroethane-d5	2.885	69	71899	16.878	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	67.520%		
11) 1,1-Dichloroethene-d2	4.019	63	109128m	13.491	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	53.960%		
21) 2-Butanone-d5	7.073	46	53007	44.799	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	89.600%		
24) Chloroform-d	7.653	84	210129	20.927	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	83.720%		
26) 1,2-Dichloroethane-d4	8.305	65	111073	20.539	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	82.160%		
32) Benzene-d6	8.274	84	377910	20.959	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	83.840%		
36) 1,2-Dichloropropane-d6	9.274	67	116300	21.893	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	87.560%		
41) Toluene-d8	10.323	98	349284	19.833	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	79.320%		
43) trans-1,3-Dichloroprop...	10.579	79	48190	19.875	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	79.520%		
47) 2-Hexanone-d5	10.926	63	40886	48.167	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	96.340%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	105379	21.240	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	84.960%		
66) 1,2-Dichlorobenzene-d4	13.853	152	129659	22.376	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	89.520%		
Target Compounds						
13) Acetone	4.129	43	2738	3.212	ug/L	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062422\
Data File : VW023514.D
Acq On : 24 Jun 2022 11:19
Operator : SY/VA
Sample : VW0624SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VBLK532

Quant Time: Jun 24 23:30:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 24 23:29:48 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin
Yesilyurt

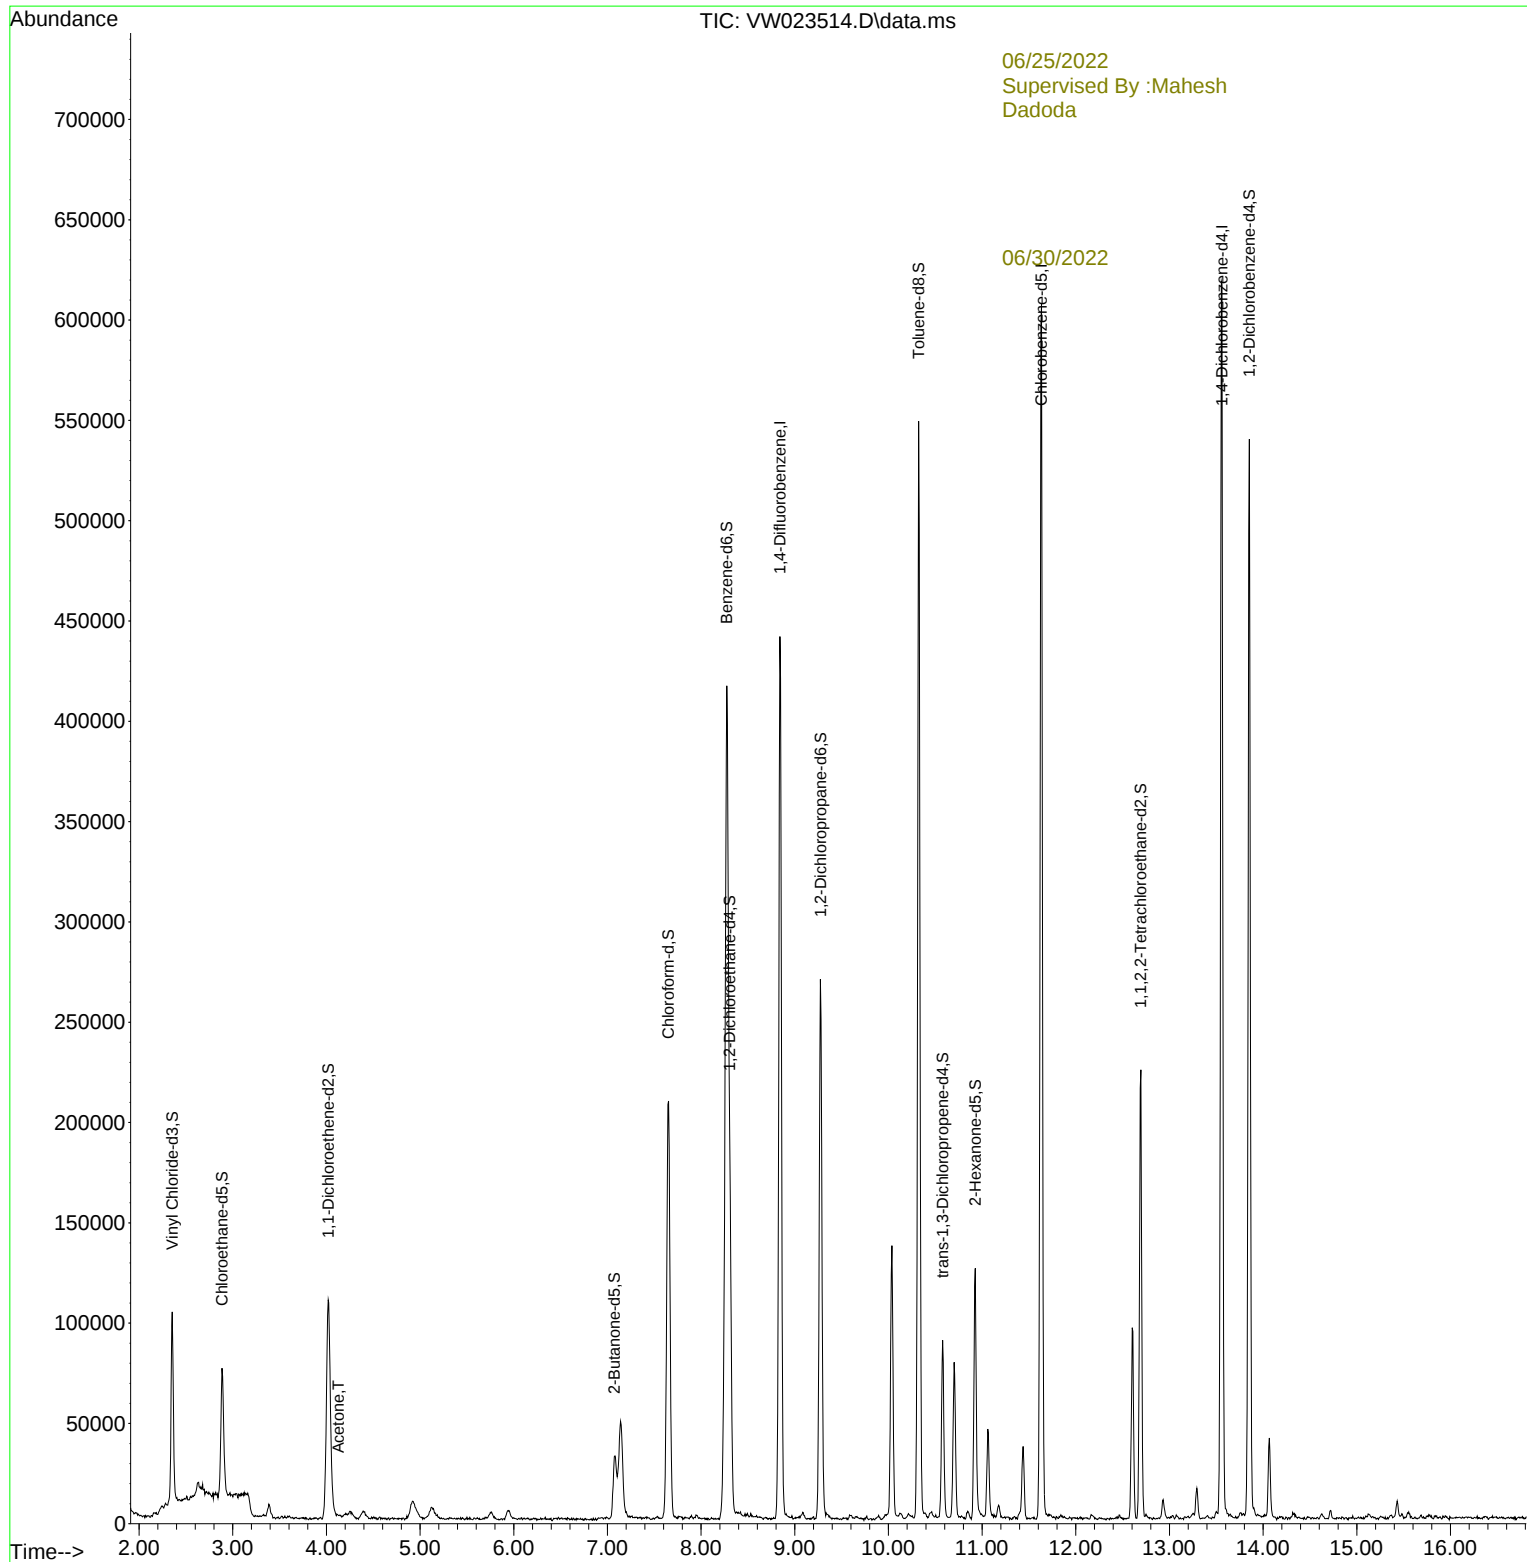

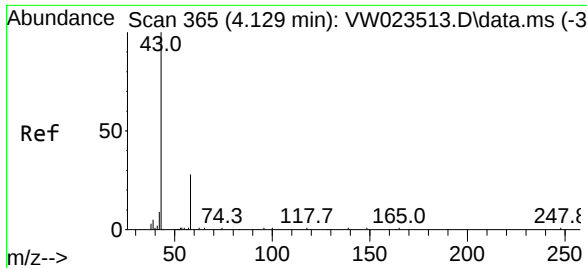

#13
 Acetone
 Concen: 3.212 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW023514.D
 Acq: 24 Jun 2022 11:19



Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK532

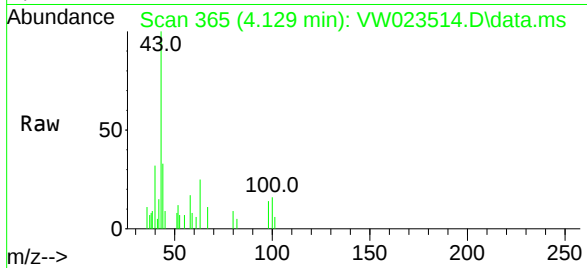

Tgt Ion: 43 Resp: 2738
 Ion Ratio Lower Upper
 43 100
 58 10.6 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin
 Yesilyurt

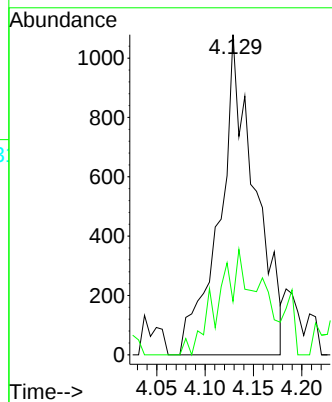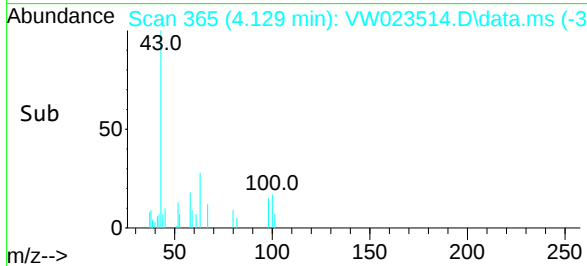

06/25/2022
 Supervised By :Mahesh
 Dadoda

06/30/2022