

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062424\
 Data File : VW029334.D
 Acq On : 24 Jun 2024 17:58
 Operator : SY/MD
 Sample : P2982-26
 Misc : 5.15g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 25 01:42:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 25 01:37:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	467267	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	419285	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	181058	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	124270	19.214	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.840%
7) Chloroethane-d5	2.899	69	113969	20.867	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.480%
11) 1,1-Dichloroethene-d2	4.027	65	61622	19.734	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.920%
21) 2-Butanone-d5	7.075	46	88288	45.628	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.260%
24) Chloroform-d	7.648	84	319654	22.933	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.720%
26) 1,2-Dichloroethane-d4	8.307	65	186290	23.278	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.120%
32) Benzene-d6	8.276	84	605845	23.789	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.160%
36) 1,2-Dichloropropane-d6	9.276	67	203946	25.192	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.760%
41) Toluene-d8	10.325	98	511769	22.713	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.840%
43) trans-1,3-Dichloroprop...	10.575	79	66096	20.260	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.040%
47) 2-Hexanone-d5	10.922	63	54354	42.830	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	156704	24.321	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	171497	27.288	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.160%
Target Compounds			Qvalue			
39) cis-1,3-Dichloropropene	10.032	75	4952	0.495	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062424\
Data File : VW029334.D
Acq On : 24 Jun 2024 17:58
Operator : SY/MD
Sample : P2982-26
Misc : 5.15g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 25 01:42:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 25 01:37:56 2024
Response via : Initial Calibration

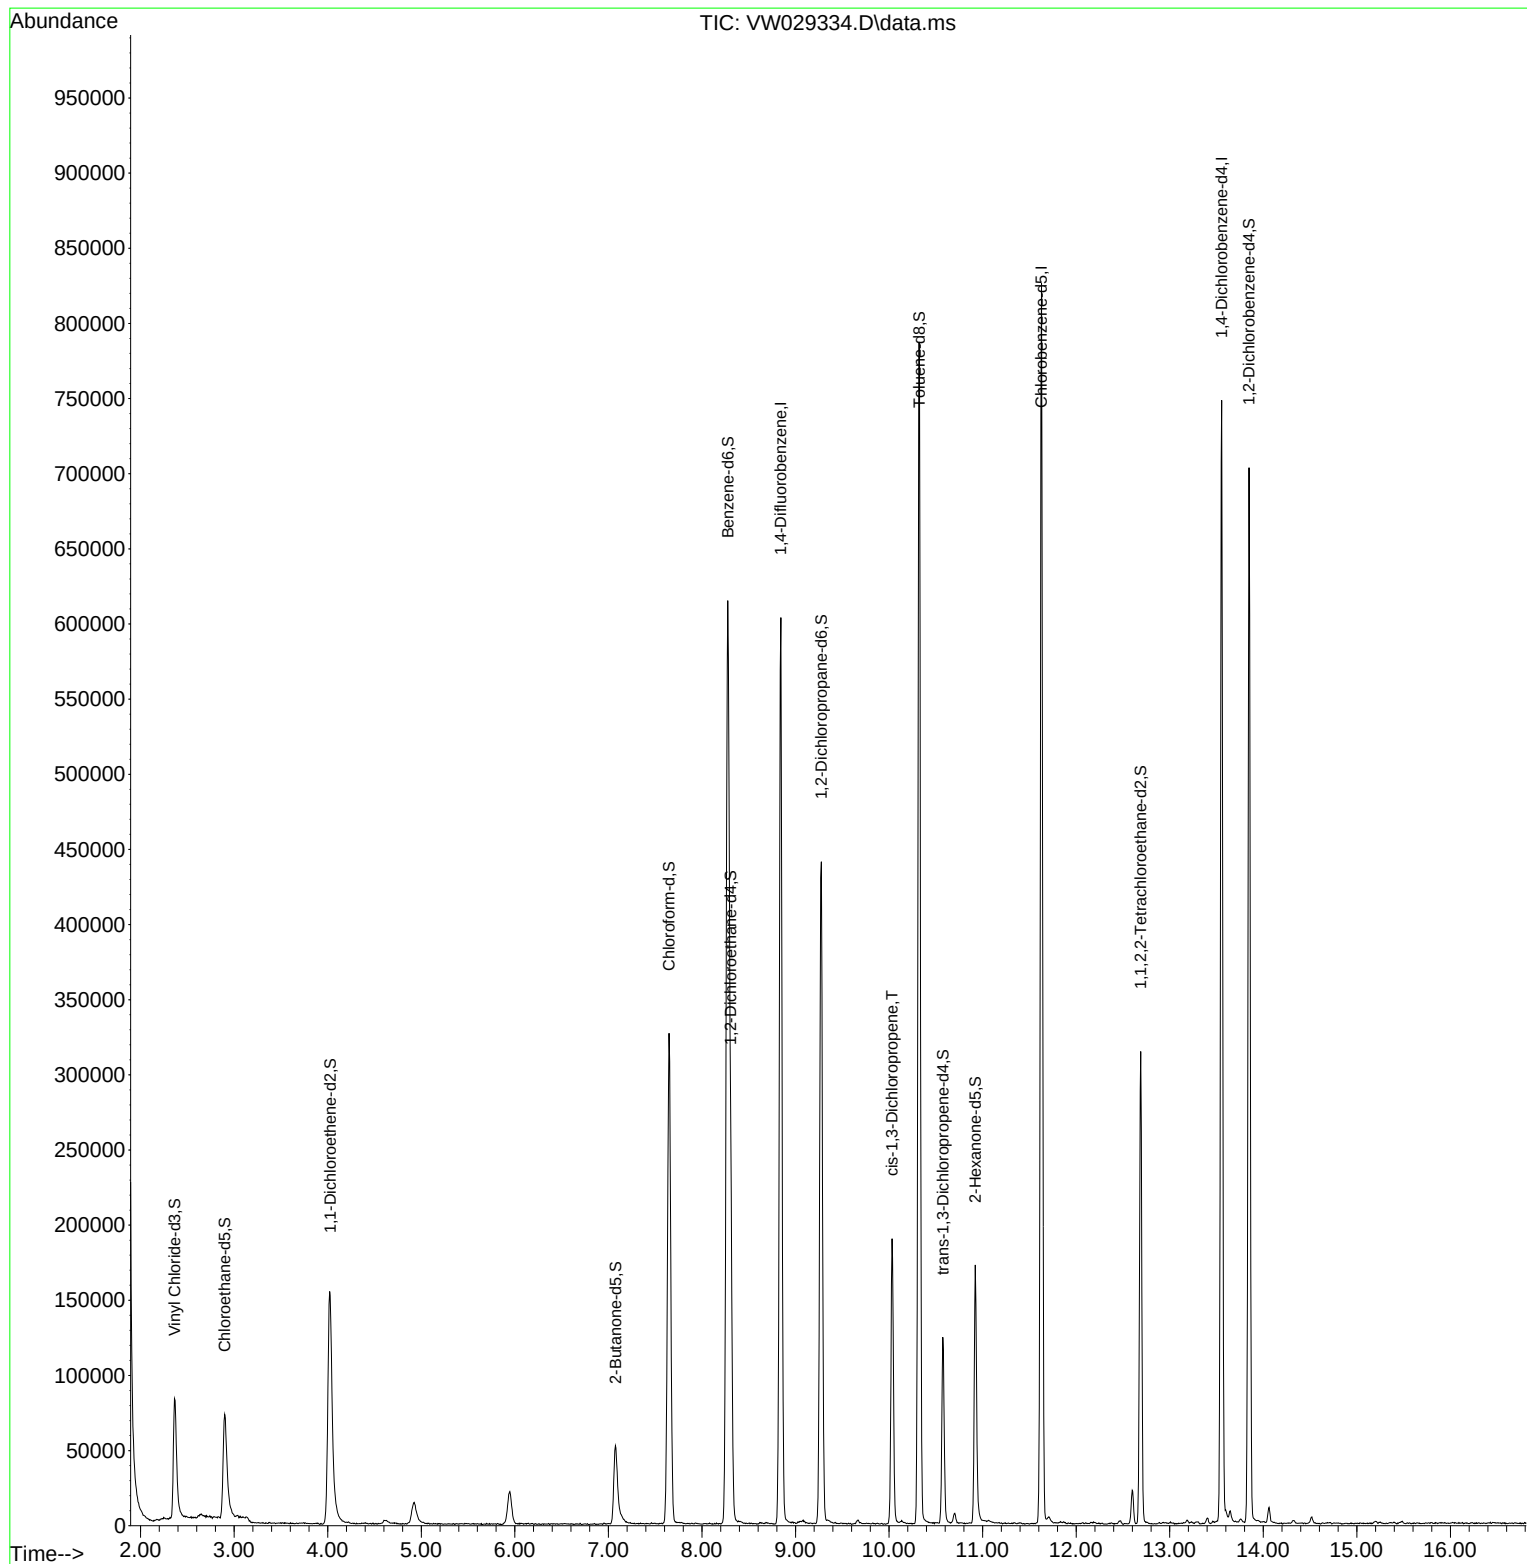

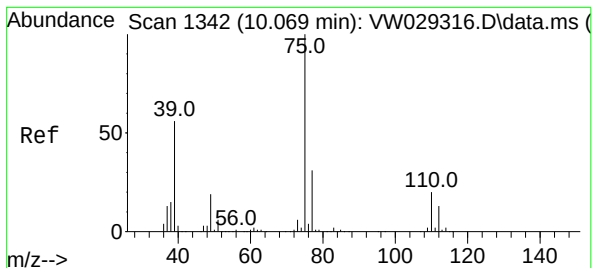

#39
cis-1,3-Dichloropropene
Concen: 0.495 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.037 min
Lab File: VW029334.D
Acq: 24 Jun 2024 17:58

Instrument :
MSVOA_W
ClientSampleId :

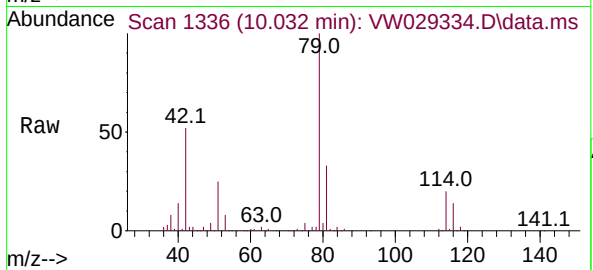

Tgt Ion: 75 Resp: 4952
Ion Ratio Lower Upper
75 100
77 50.0 22.7 42.1#

