

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062524\
 Data File : VW029340.D
 Acq On : 25 Jun 2024 10:33
 Operator : SY/MD
 Sample : P2963-20
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 26 02:26:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 26 02:25:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	269325	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	252083	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	112821	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	93658	25.124	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.480%
7) Chloroethane-d5	2.899	69	74343	23.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.480%
11) 1,1-Dichloroethene-d2	4.021	65	44312	24.619	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.480%
21) 2-Butanone-d5	7.075	46	52870	47.405	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.800%
24) Chloroform-d	7.648	84	192132	23.915	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.640%
26) 1,2-Dichloroethane-d4	8.307	65	113190	24.538	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.160%
32) Benzene-d6	8.276	84	381610	24.923	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.680%
36) 1,2-Dichloropropane-d6	9.270	67	121586	24.981	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.920%
41) Toluene-d8	10.325	98	339104	25.032	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.120%
43) trans-1,3-Dichloroprop...	10.575	79	45070	22.979	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.920%
47) 2-Hexanone-d5	10.922	63	35724	46.821	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91951	23.737	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.960%
66) 1,2-Dichlorobenzene-d4	13.849	152	107825	27.534	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.120%
Target Compounds						
39) cis-1,3-Dichloropropene	10.026	75	3665	0.609	ug/L	Qvalue # 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062524\
Data File : VW029340.D
Acq On : 25 Jun 2024 10:33
Operator : SY/MD
Sample : P2963-20
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 26 02:26:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 26 02:25:08 2024
Response via : Initial Calibration

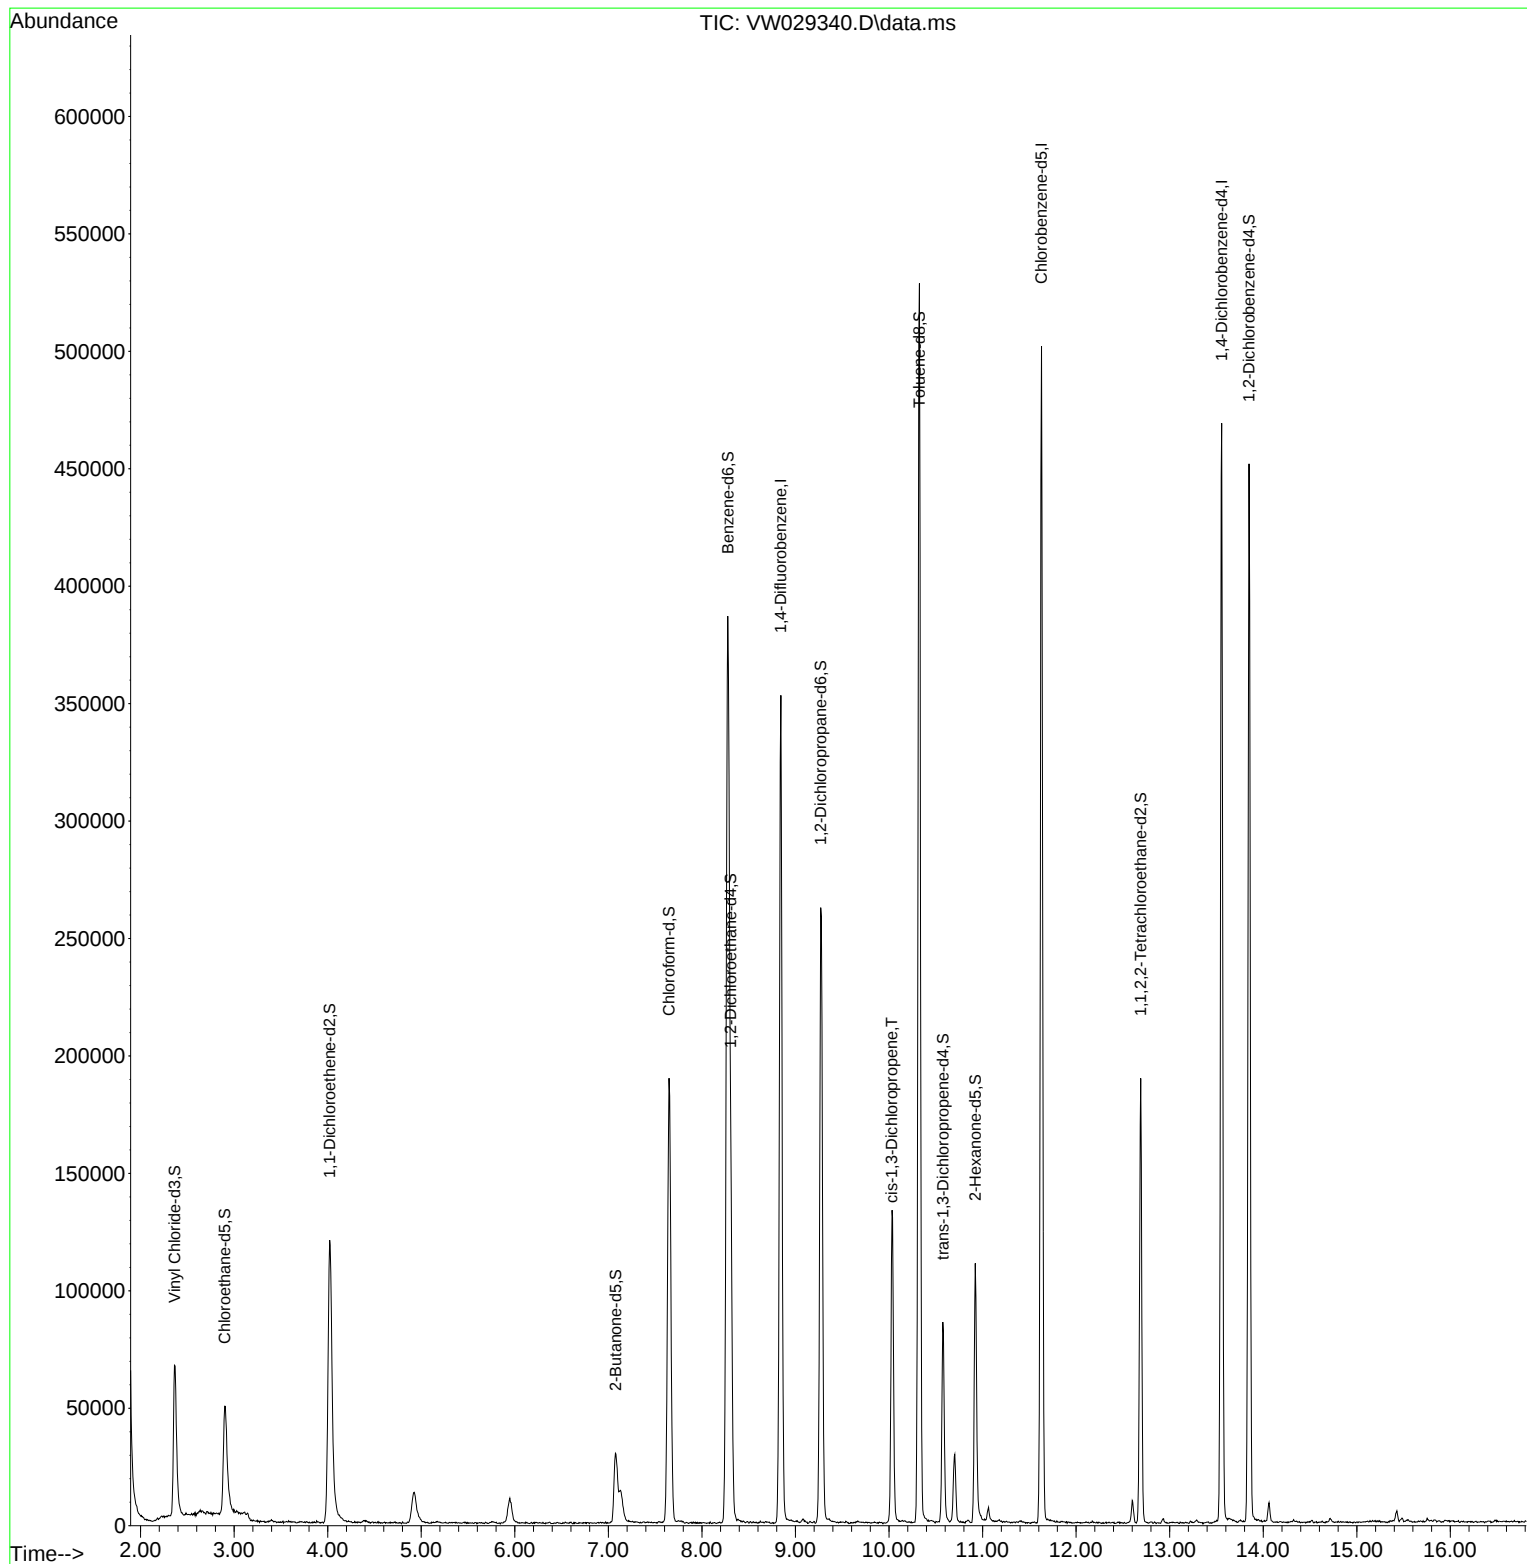

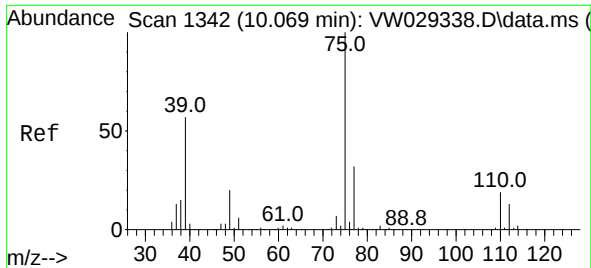

#39
cis-1,3-Dichloropropene
Concen: 0.609 ug/L
RT: 10.026 min Scan# 14
Delta R.T. -0.043 min
Lab File: VW029340.D
Acq: 25 Jun 2024 10:33

Instrument :
MSVOA_W
ClientSampleId :

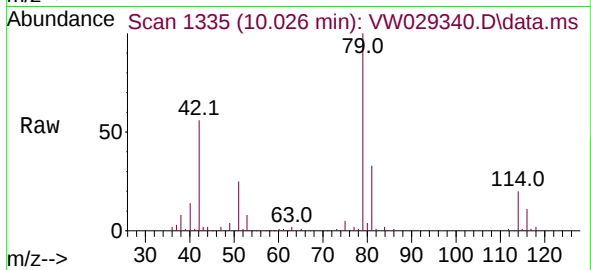

Tgt Ion: 75 Resp: 3665
Ion Ratio Lower Upper
75 100
77 47.4 22.7 42.1#

