

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062524\
 Data File : VW029342.D
 Acq On : 25 Jun 2024 11:20
 Operator : SY/MD
 Sample : P2982-05
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 26 02:26:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 26 02:25:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	280334	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	262204	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	112720	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	88322	22.762	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.040%
7) Chloroethane-d5	2.899	69	71411	21.794	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.160%
11) 1,1-Dichloroethene-d2	4.021	65	42354	22.608	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.440%
21) 2-Butanone-d5	7.075	46	45377	39.089	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.180%
24) Chloroform-d	7.648	84	187224	22.389	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.560%
26) 1,2-Dichloroethane-d4	8.307	65	106403	22.161	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.640%
32) Benzene-d6	8.276	84	376397	23.634	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.520%
36) 1,2-Dichloropropane-d6	9.270	67	120032	23.709	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.840%
41) Toluene-d8	10.325	98	338160	23.999	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.000%
43) trans-1,3-Dichloroprop...	10.575	79	44399	21.763	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.040%
47) 2-Hexanone-d5	10.922	63	30517	38.453	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	82764	20.541	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.160%
66) 1,2-Dichlorobenzene-d4	13.849	152	103434	26.436	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3384	0.541	ug/L	# 52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062524\
Data File : VW029342.D
Acq On : 25 Jun 2024 11:20
Operator : SY/MD
Sample : P2982-05
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 26 02:26:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 26 02:25:08 2024
Response via : Initial Calibration

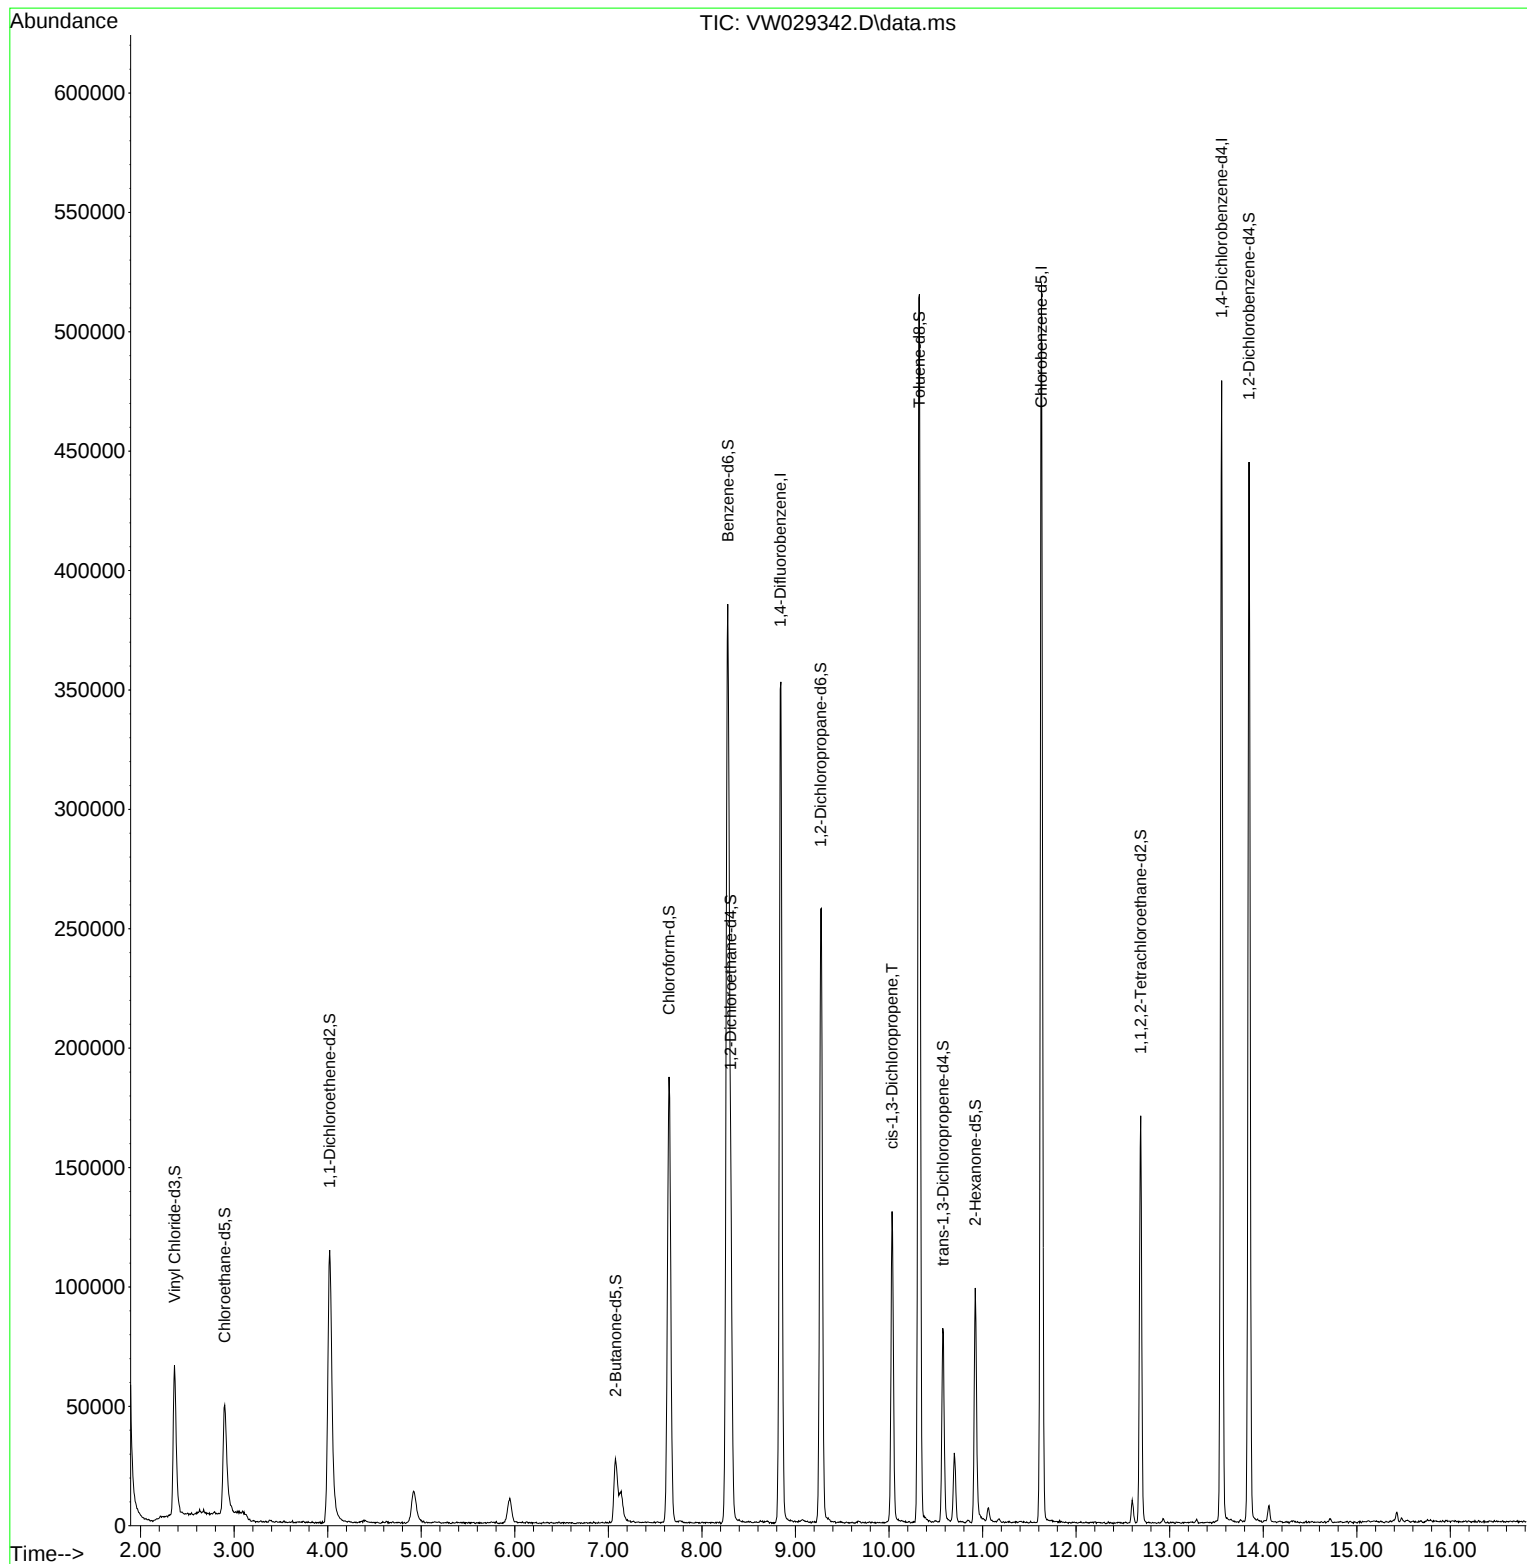

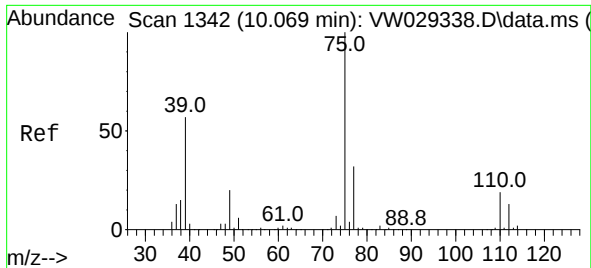

#39
 cis-1,3-Dichloropropene
 Concen: 0.541 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029342.D
 Acq: 25 Jun 2024 11:20

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3384
 Ion Ratio Lower Upper
 75 100
 77 59.3 22.7 42.1#

