

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062524\
 Data File : VW029339.D
 Acq On : 25 Jun 2024 10:09
 Operator : SY/MD
 Sample : VW0625SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK512

Quant Time: Jun 26 02:25:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 26 02:25:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	288483	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	271898	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	121039	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	97513	24.421	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.680%		
7) Chloroethane-d5	2.899	69	75379	22.355	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.400%		
11) 1,1-Dichloroethene-d2	4.027	65	45283	23.488	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	93.960%		
21) 2-Butanone-d5	7.075	46	51623	43.213	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.420%		
24) Chloroform-d	7.648	84	191150	22.212	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.840%		
26) 1,2-Dichloroethane-d4	8.307	65	110331	22.330	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.320%		
32) Benzene-d6	8.276	84	383783	23.238	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.960%		
36) 1,2-Dichloropropane-d6	9.270	67	121377	23.120	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.480%		
41) Toluene-d8	10.325	98	342103	23.413	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.640%		
43) trans-1,3-Dichloroprop...	10.575	79	45937	21.714	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.840%		
47) 2-Hexanone-d5	10.922	63	34593	42.034	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	84.060%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	88755	21.242	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	84.960%		
66) 1,2-Dichlorobenzene-d4	13.848	152	108339	25.787	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.160%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	12115	2.388	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062524\
Data File : VW029339.D
Acq On : 25 Jun 2024 10:09
Operator : SY/MD
Sample : VW0625SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK512


Quant Time: Jun 26 02:25:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 26 02:25:08 2024
Response via : Initial Calibration

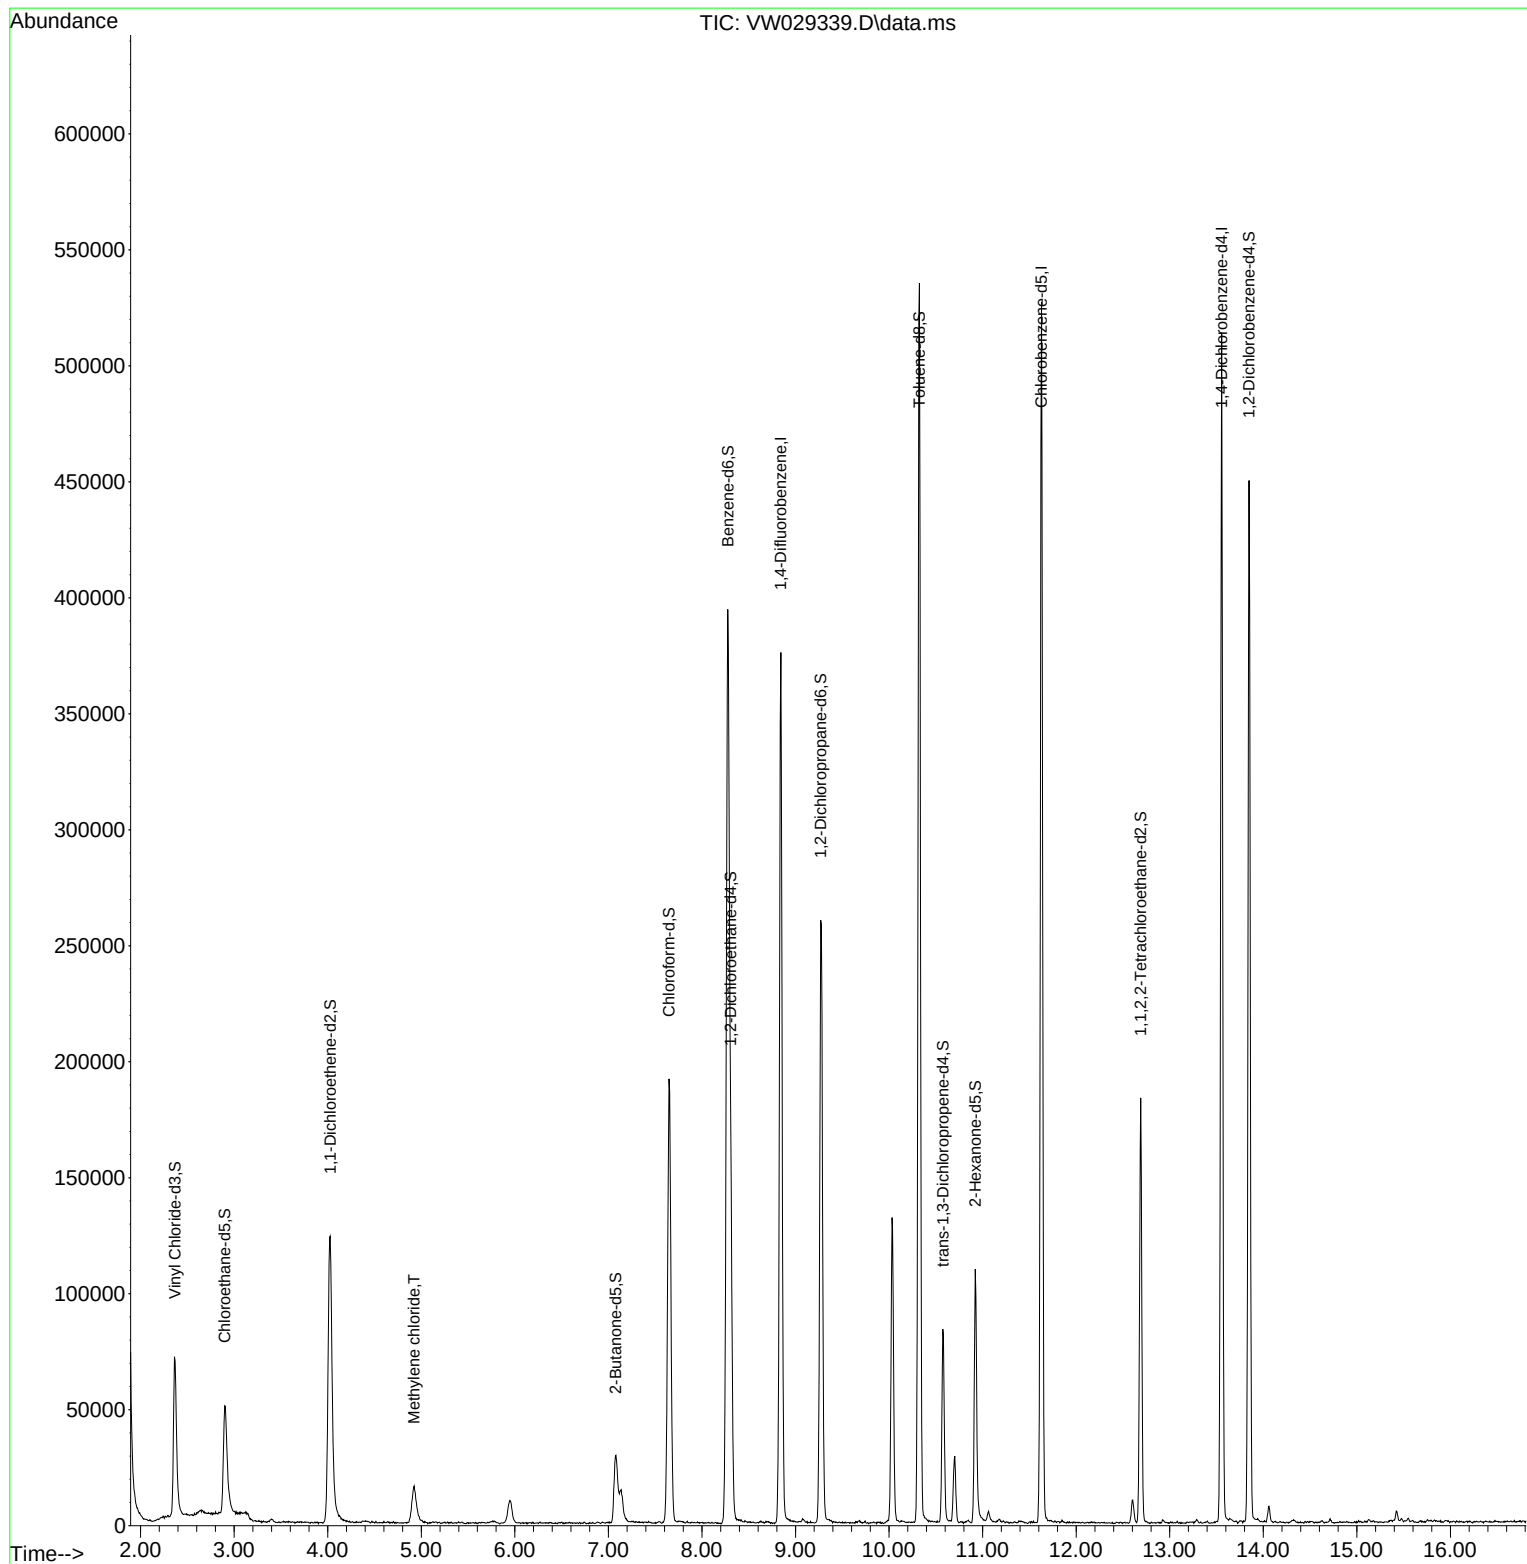

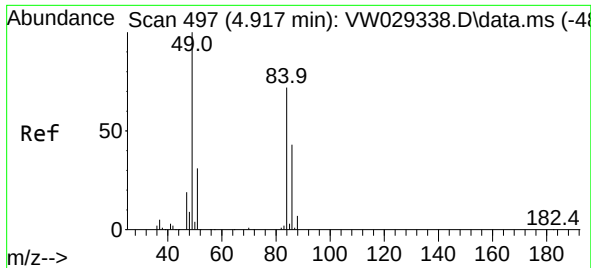

#16
Methylene chloride
Concen: 2.388 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW029339.D
Acq: 25 Jun 2024 10:09

Instrument :
MSVOA_W
ClientSampleId :
VBLK512

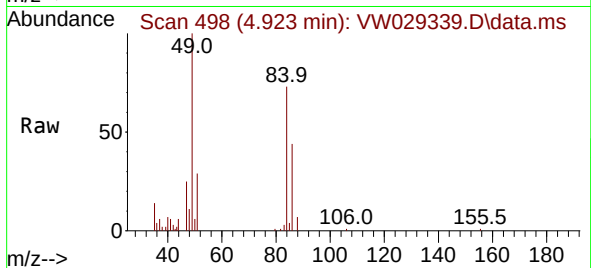

Tgt Ion: 84 Resp: 12115

Ion	Ratio	Lower	Upper
84	100		
86	60.6	41.4	77.0
49	137.0	95.7	177.7

