




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062623\
 Data File : VW026335.D
 Acq On : 26 Jun 2023 14:59
 Operator : SY/MD
 Sample : VW0626SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK525

Manual IntegrationsAPPROVED

Quant Time: Jun 27 01:52:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 27 01:51:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/27/2023
 Supervised By :Mahesh Dadoda 06/27/2023

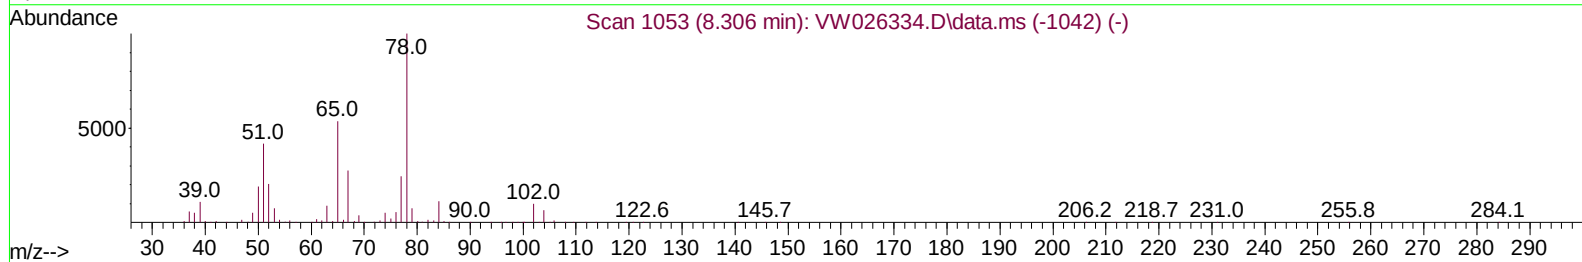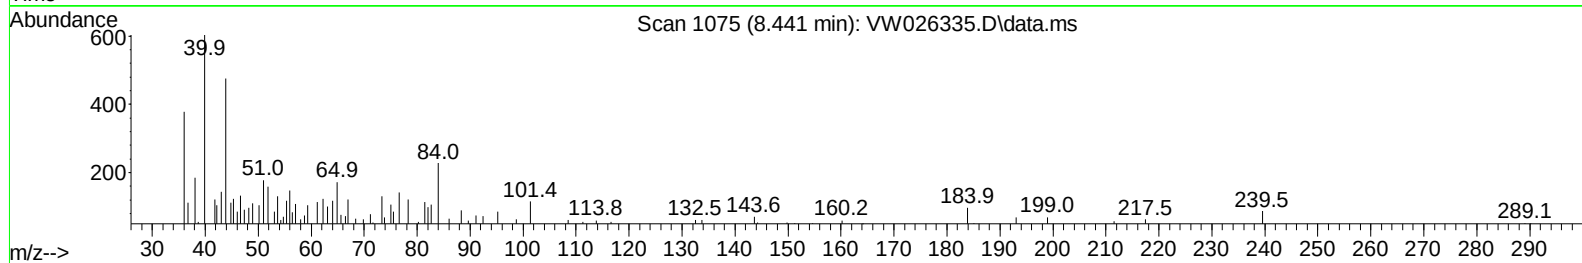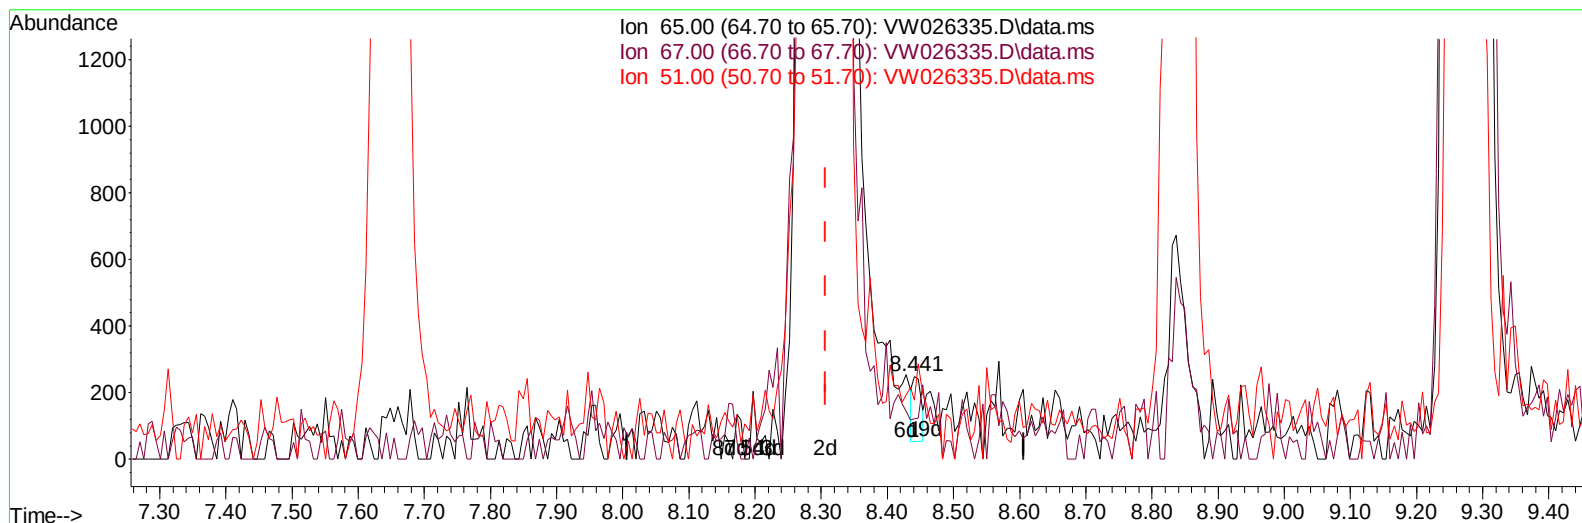

TIC: VW026335.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.441min (+ 0.134) 0.02 ug/L

response 175

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.20	41.71
51.00	117.60	114.86
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062623\
 Data File : VW026335.D
 Acq On : 26 Jun 2023 14:59
 Operator : SY/MD
 Sample : VW0626SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK525

Manual IntegrationsAPPROVED

Quant Time: Jun 27 01:52:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 27 01:51:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/27/2023
 Supervised By :Mahesh Dadoda 06/27/2023

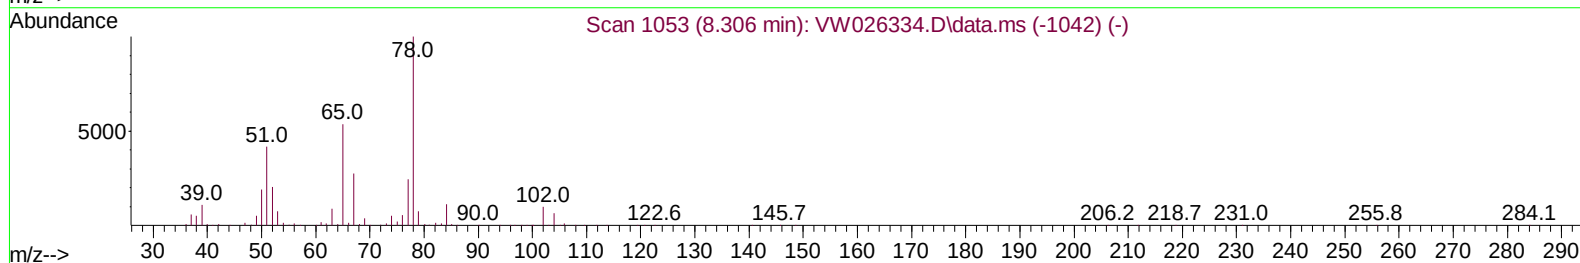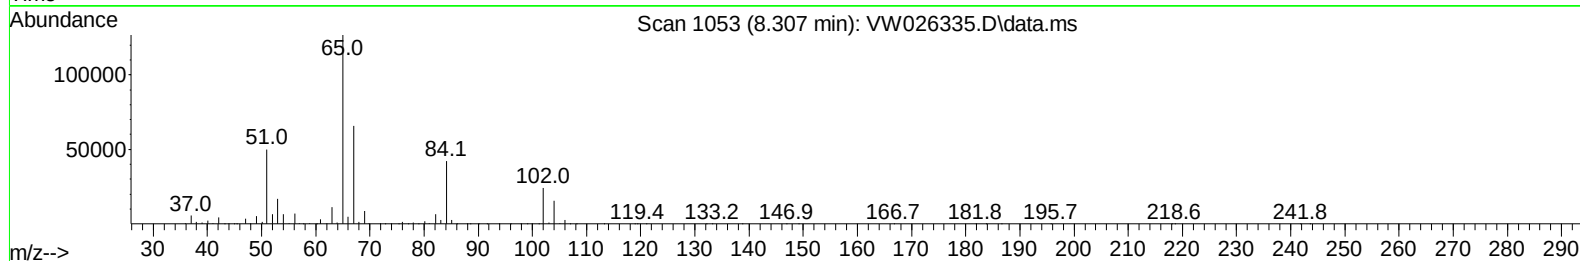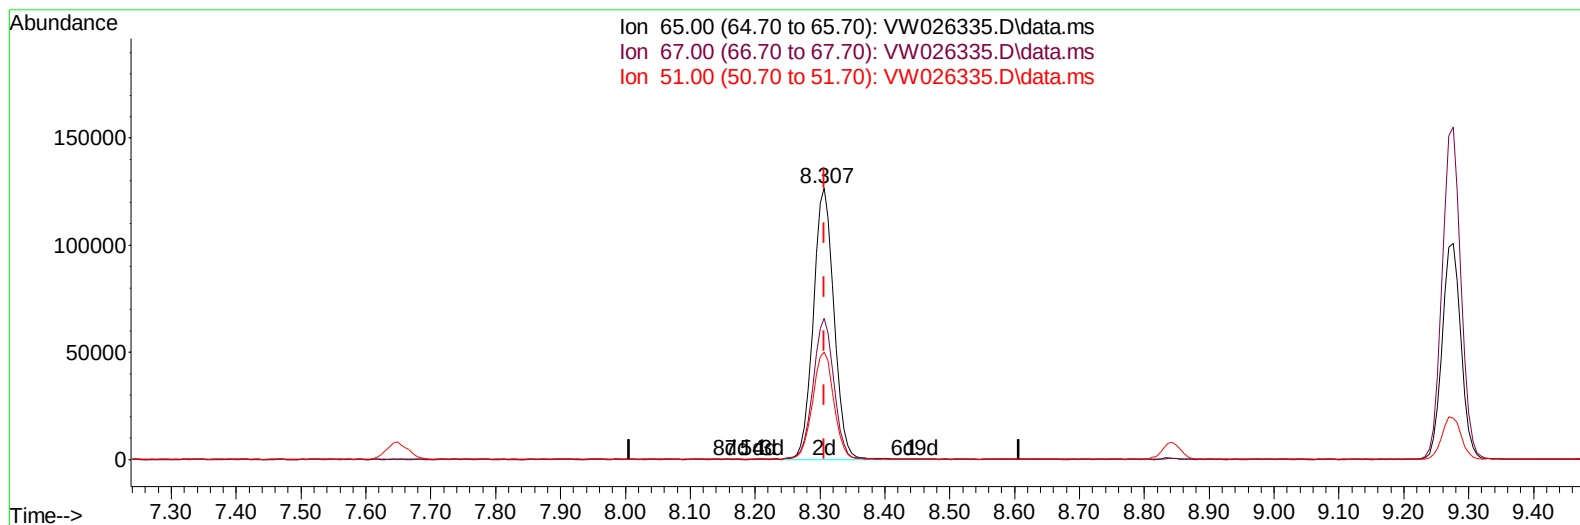

TIC: VW026335.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.65 ug/L m

response 280299

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.20	0.03#
51.00	117.60	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062623\
 Data File : VW0626335.D
 Acq On : 26 Jun 2023 14:59
 Operator : SY/MD
 Sample : VW0626SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK525

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/27/2023
 Supervised By :Mahesh Dadoda 06/27/2023

Quant Time: Jun 27 01:52:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 27 01:51:47 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		686251	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		622042	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		273371	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		252415	25.318	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	101.280%	
7) Chloroethane-d5	2.893	69		178929	25.247	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	101.000%	
11) 1,1-Dichloroethene-d2	4.027	65		115152	25.512	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	102.040%	
21) 2-Butanone-d5	7.075	46		147818	47.177	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	94.360%	
24) Chloroform-d	7.648	84		471923	24.268	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	97.080%	
26) 1,2-Dichloroethane-d4	8.307	65		280299m	25.653	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	102.600%	
32) Benzene-d6	8.276	84		960841	24.955	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	99.800%	
36) 1,2-Dichloropropane-d6	9.276	67		310854	24.846	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	99.400%	
41) Toluene-d8	10.325	98		838820	24.890	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	99.560%	
43) trans-1,3-Dichloroprop...	10.575	79		119814	23.852	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	95.400%	
47) 2-Hexanone-d5	10.922	63		90208	46.948	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	93.900%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		239072	24.271	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.080%	
66) 1,2-Dichlorobenzene-d4	13.848	152		252046	26.480	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	105.920%	
Target Compounds							
16) Methylene chloride	4.923	84		28568	2.460	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062623\
Data File : VW062635.D
Acq On : 26 Jun 2023 14:59
Operator : SY/MD
Sample : VW0626SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK525

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/27/2023
Supervised By :Mahesh Dadoda 06/27/2023

Quant Time: Jun 27 01:52:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 27 01:51:47 2023
Response via : Initial Calibration

