

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062624\
 Data File : VW029350.D
 Acq On : 26 Jun 2024 10:09
 Operator : SY/MD
 Sample : VW0626SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 27 05:36:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 27 05:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	269929	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	256479	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	113449	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	84175	22.530	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.120%		
7) Chloroethane-d5	2.899	69	66842	21.186	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.760%		
11) 1,1-Dichloroethene-d2	4.027	65	39503	21.899	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	87.600%		
21) 2-Butanone-d5	7.081	46	49616	44.388	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.780%		
24) Chloroform-d	7.648	84	172546	21.429	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.720%		
26) 1,2-Dichloroethane-d4	8.307	65	101501	21.955	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.840%		
32) Benzene-d6	8.276	84	340396	21.850	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.400%		
36) 1,2-Dichloropropane-d6	9.276	67	109904	22.193	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.760%		
41) Toluene-d8	10.325	98	298895	21.686	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.760%		
43) trans-1,3-Dichloroprop...	10.575	79	40889	20.490	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.960%		
47) 2-Hexanone-d5	10.922	63	32366	41.693	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	83.380%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	84660	21.480	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.920%		
66) 1,2-Dichlorobenzene-d4	13.849	152	97644	24.796	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.200%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	13498	2.844	ug/L	94
39) cis-1,3-Dichloropropene	10.038	75	3143	0.513	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062624\
Data File : VW029350.D
Acq On : 26 Jun 2024 10:09
Operator : SY/MD
Sample : VW0626SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 27 05:36:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 27 05:32:27 2024
Response via : Initial Calibration

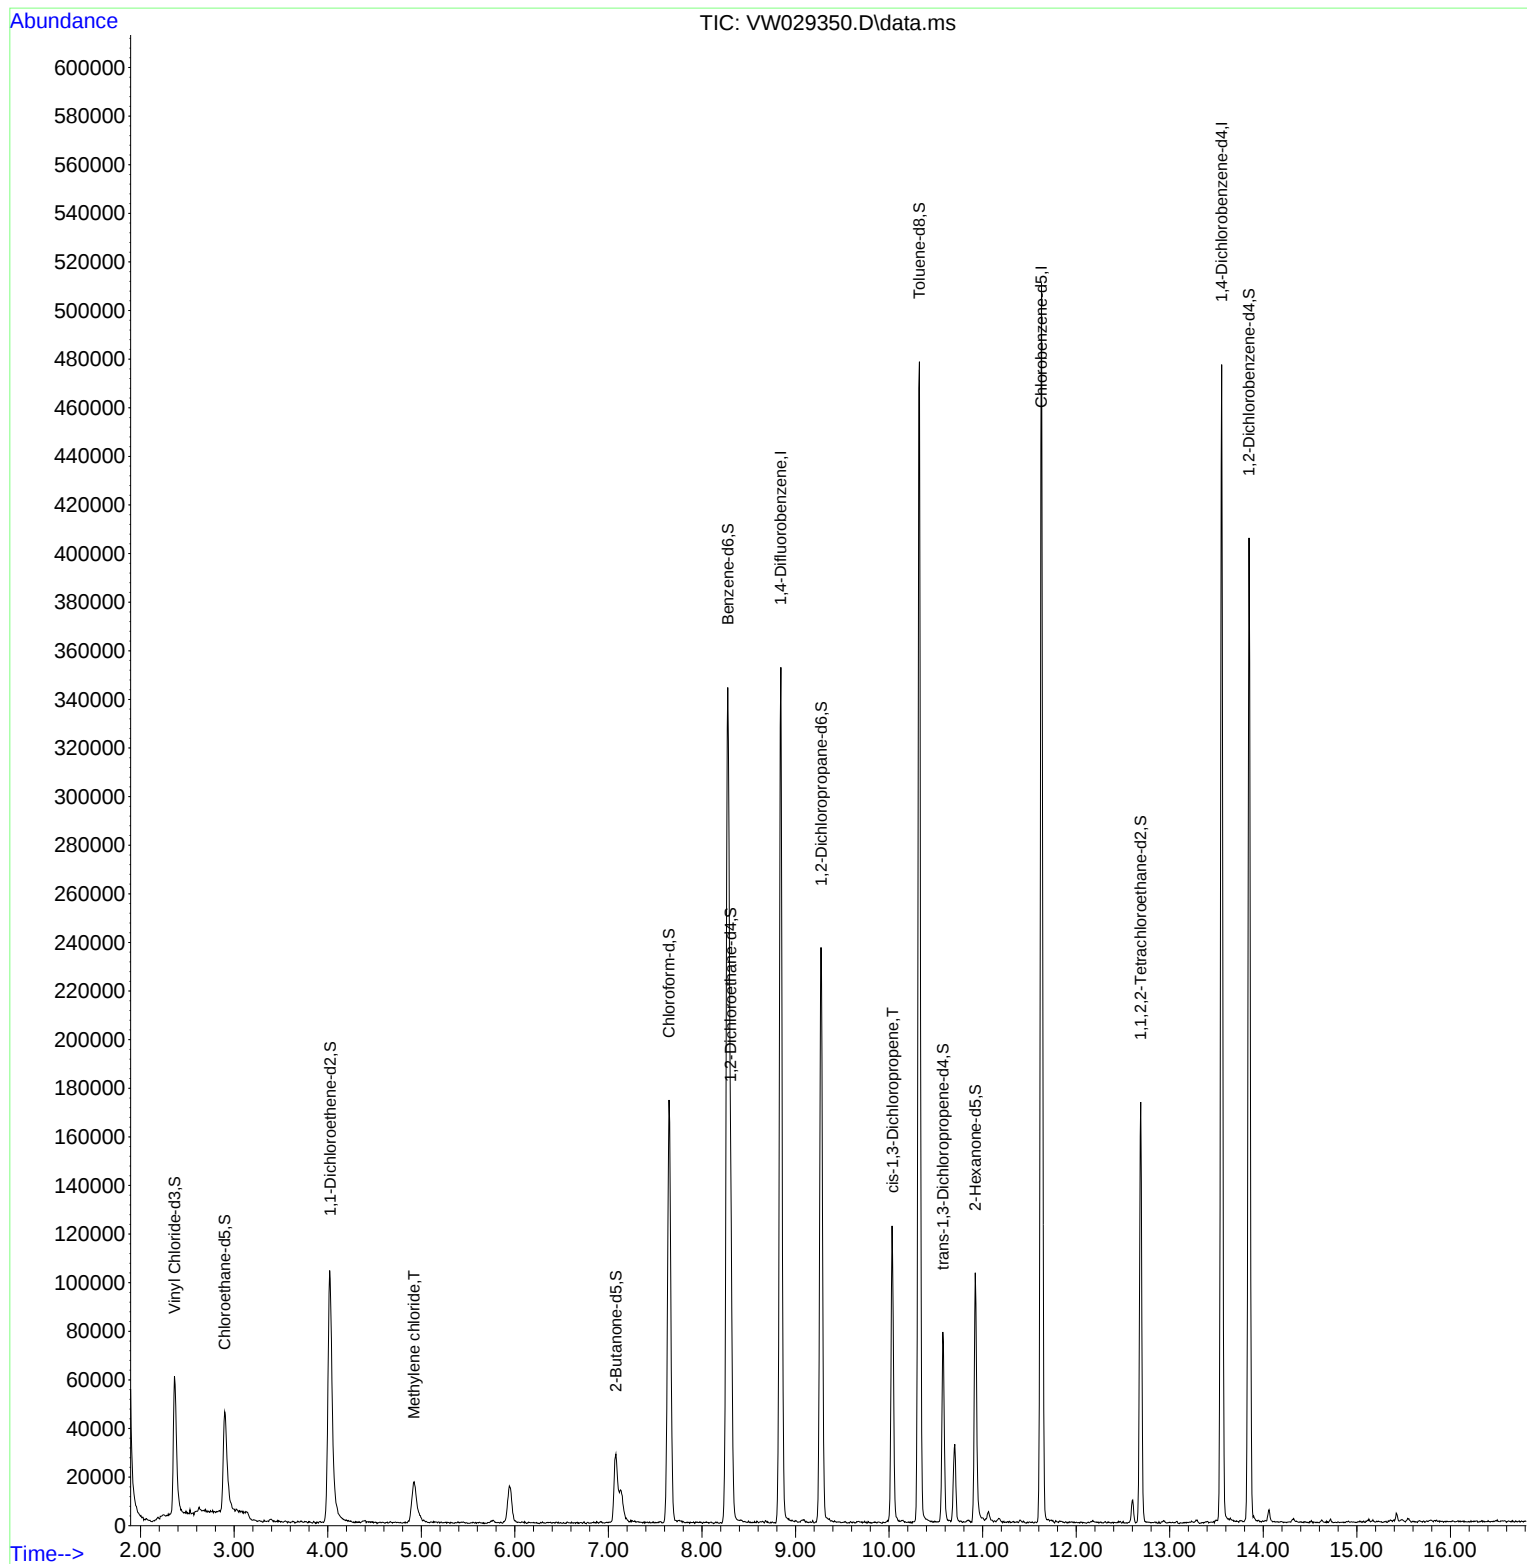



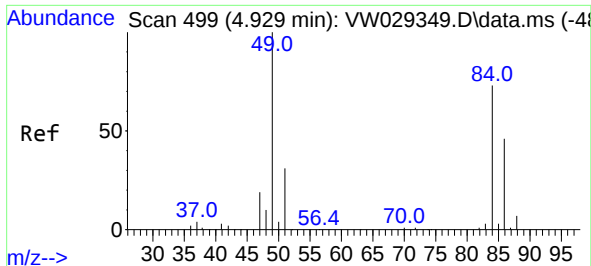


#16
Methylene chloride
Concen: 2.844 ug/L
RT: 4.923 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW029350.D
Acq: 26 Jun 2024 10:09

Instrument :
MSVOA_W
ClientSampleId :

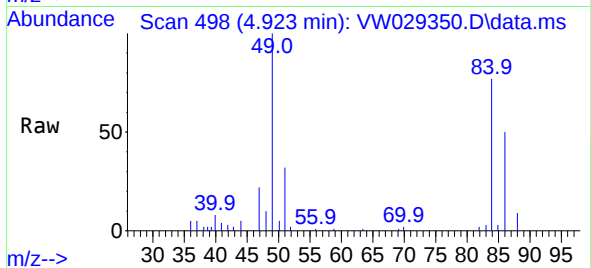

Tgt Ion: 84 Resp: 13498
Ion Ratio Lower Upper
84 100
86 65.9 41.4 77.0
49 130.6 95.7 177.7

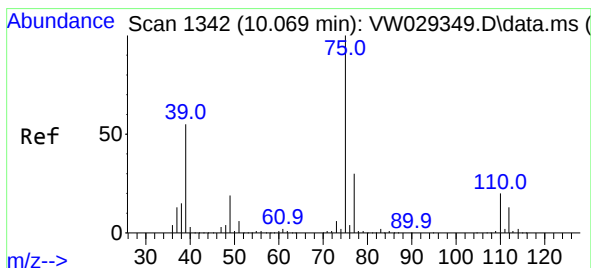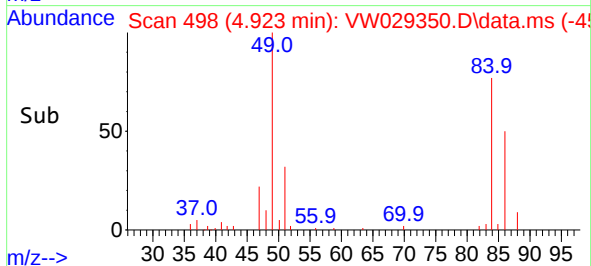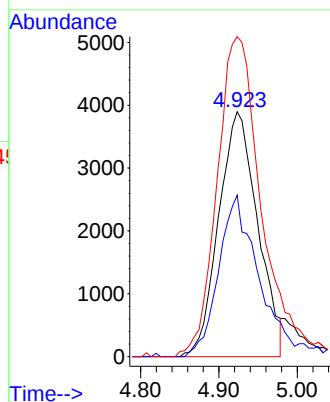

#39
cis-1,3-Dichloropropene
Concen: 0.513 ug/L
RT: 10.038 min Scan# 1337
Delta R.T. -0.030 min
Lab File: VW029350.D
Acq: 26 Jun 2024 10:09

Tgt Ion: 75 Resp: 3143
Ion Ratio Lower Upper
75 100
77 50.7 22.7 42.1#

