

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062624\
 Data File : VW029351.D
 Acq On : 26 Jun 2024 10:33
 Operator : SY/MD
 Sample : P3026-07
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 27 05:36:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 27 05:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	262277	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	250543	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	111184	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	81957	22.576	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.320%		
7) Chloroethane-d5	2.899	69	68320	22.286	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.160%		
11) 1,1-Dichloroethene-d2	4.021	65	39699	22.649	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	90.600%		
21) 2-Butanone-d5	7.081	46	50673	46.656	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.320%		
24) Chloroform-d	7.648	84	180345	23.051	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.200%		
26) 1,2-Dichloroethane-d4	8.307	65	106517	23.712	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	94.840%		
32) Benzene-d6	8.276	84	361802	23.775	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.080%		
36) 1,2-Dichloropropane-d6	9.270	67	115579	23.892	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.560%		
41) Toluene-d8	10.325	98	317270	23.565	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	94.240%		
43) trans-1,3-Dichloroprop...	10.581	79	43143	22.132	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.520%		
47) 2-Hexanone-d5	10.922	63	33283	43.890	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.780%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	89591	23.270	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.080%		
66) 1,2-Dichlorobenzene-d4	13.849	152	104948	27.194	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	108.760%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3394	0.568	ug/L	# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062624\
Data File : VW029351.D
Acq On : 26 Jun 2024 10:33
Operator : SY/MD
Sample : P3026-07
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 27 05:36:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 27 05:32:27 2024
Response via : Initial Calibration

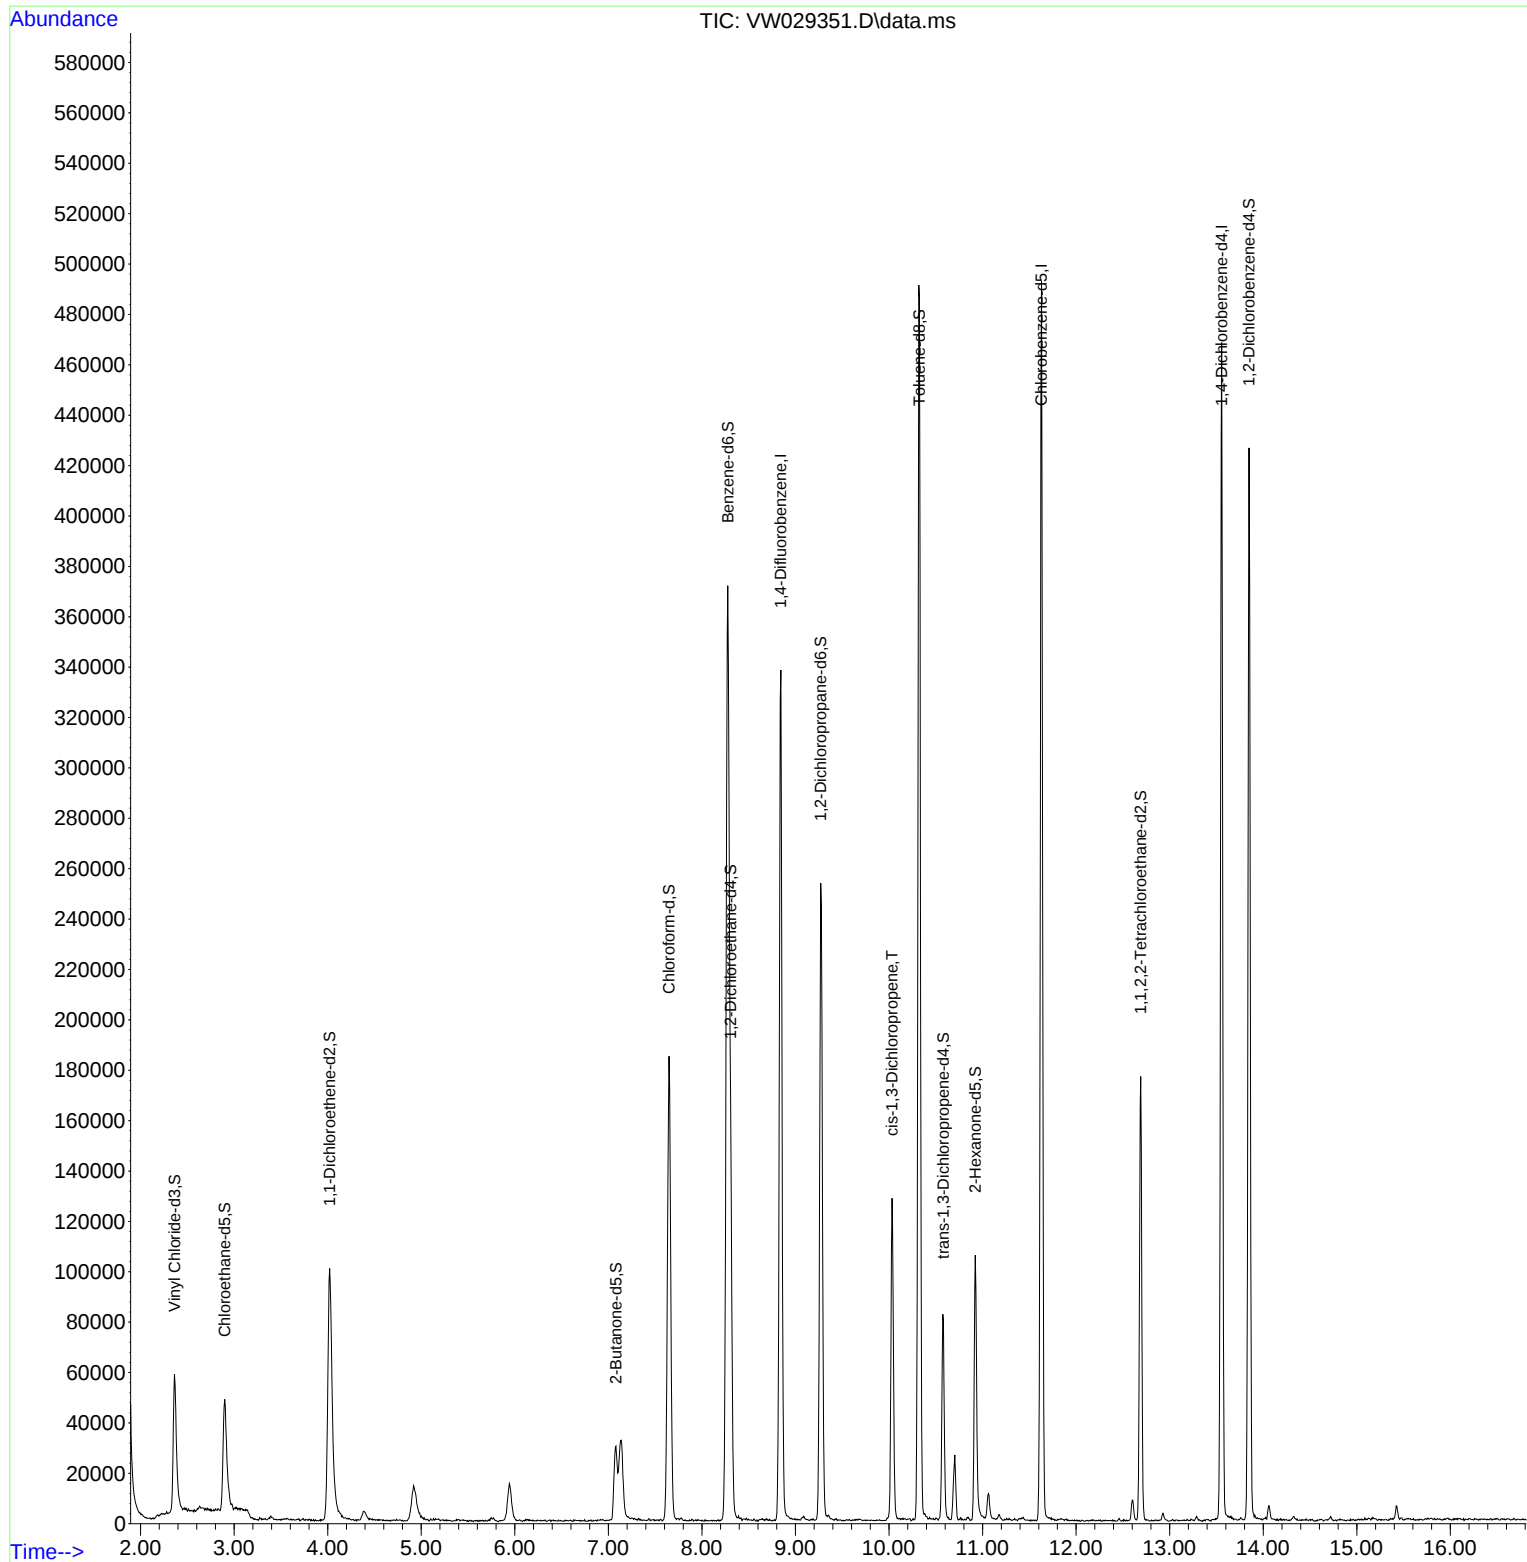

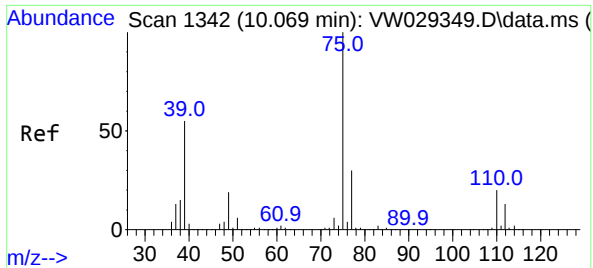

#39
cis-1,3-Dichloropropene
Concen: 0.568 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.036 min
Lab File: VW029351.D
Acq: 26 Jun 2024 10:33

Instrument :
MSVOA_W
ClientSampleId :

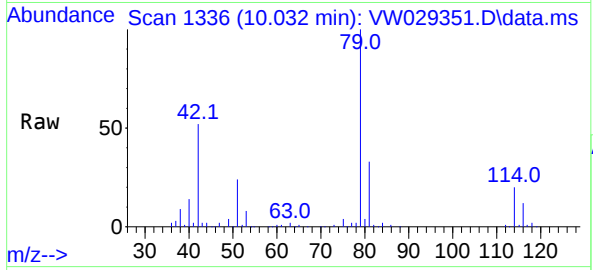

Tgt Ion: 75 Resp: 3394

Ion	Ratio	Lower	Upper
75	100		
77	46.5	22.7	42.1#

