

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026378.D
 Acq On : 28 Jun 2023 01:37
 Operator : SY/MD
 Sample : 03420-17
 Misc : 4.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46G8

Quant Time: Jun 28 05:56:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 05:31:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1222001	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1085577	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	520928	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	287876	16.216	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.880%
7) Chloroethane-d5	2.893	69	241877	19.166	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.680%
11) 1,1-Dichloroethene-d2	4.021	65	145813	18.142	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.560%
21) 2-Butanone-d5	7.075	46	195437	35.028	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.060%
24) Chloroform-d	7.648	84	629041	18.166	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.680%
26) 1,2-Dichloroethane-d4	8.106	65	117	0.006	ug/L	-0.20
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.270	84	1255184	18.680	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.720%
36) 1,2-Dichloropropane-d6	9.270	67	404693	18.535	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.120%
41) Toluene-d8	10.325	98	1130245	19.217	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.880%
43) trans-1,3-Dichloroprop...	10.575	79	159615	18.207	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.840%
47) 2-Hexanone-d5	10.922	63	127214	37.937	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.880%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	303443	17.652	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.600%
66) 1,2-Dichlorobenzene-d4	13.849	152	341156	18.809	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.240%
Target Compounds					Qvalue	
13) Acetone	4.125	43	12913	2.892	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026378.D
Acq On : 28 Jun 2023 01:37
Operator : SY/MD
Sample : 03420-17
Misc : 4.24g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46G8

Quant Time: Jun 28 05:56:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 05:31:59 2023
Response via : Initial Calibration

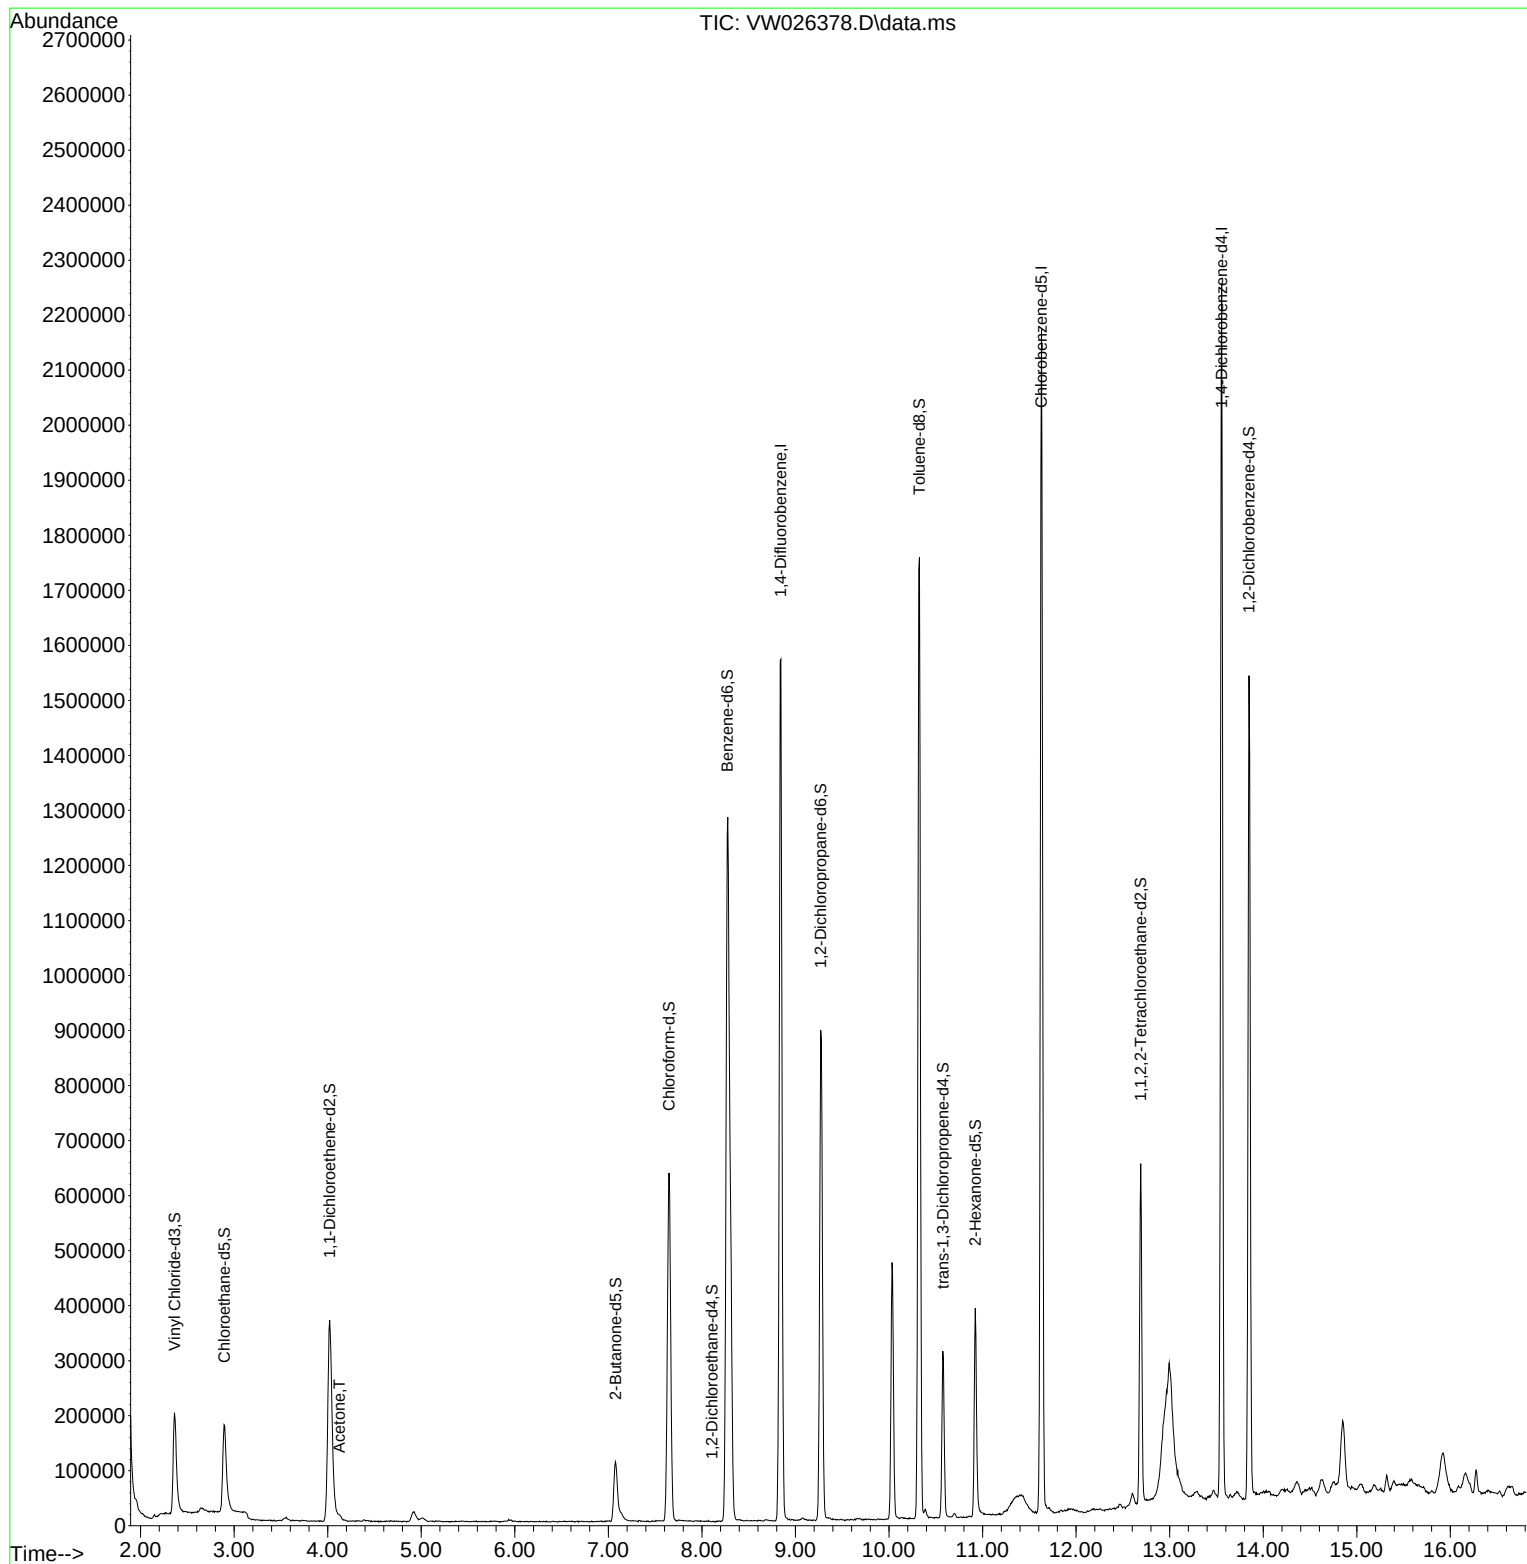

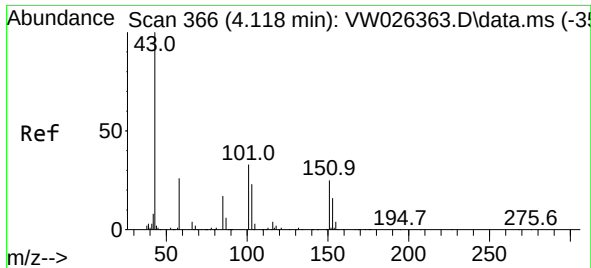

#13

Acetone

Concen: 2.892 ug/L

RT: 4.125 min Scan# 30

Delta R.T. 0.007 min

Lab File: VW026378.D

Acq: 28 Jun 2023 01:37

Instrument :

MSVOA_W

ClientSampleId :

A46G8

Tgt Ion: 43 Resp: 12913

Ion Ratio Lower Upper

43 100

58 23.4 0.0 55.8

