

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026379.D
 Acq On : 28 Jun 2023 02:01
 Operator : SY/MD
 Sample : 03420-18
 Misc : 4.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46G9

Quant Time: Jun 28 05:56:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 05:31:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1122541	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	984332	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	454773	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	293272	17.983	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.920%
7) Chloroethane-d5	2.899	69	257940	22.250	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	4.021	65	149312	20.223	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.880%
21) 2-Butanone-d5	7.081	46	183351	35.774	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.540%
24) Chloroform-d	7.648	84	645872	20.305	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.200%
26) 1,2-Dichloroethane-d4	8.307	65	391762	21.919	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.680%
32) Benzene-d6	8.276	84	1286377	21.113	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.440%
36) 1,2-Dichloropropane-d6	9.276	67	414708	20.947	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.800%
41) Toluene-d8	10.325	98	1166098	21.866	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.480%
43) trans-1,3-Dichloroprop...	10.575	79	159685	20.089	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.360%
47) 2-Hexanone-d5	10.922	63	118688	39.035	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.080%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	298603	19.157	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	349887	22.097	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.400%
Target Compounds						
					Qvalue	
48) 2-Hexanone	10.922	43	16561	1.957	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026379.D
Acq On : 28 Jun 2023 02:01
Operator : SY/MD
Sample : 03420-18
Misc : 4.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46G9


Quant Time: Jun 28 05:56:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 05:31:59 2023
Response via : Initial Calibration

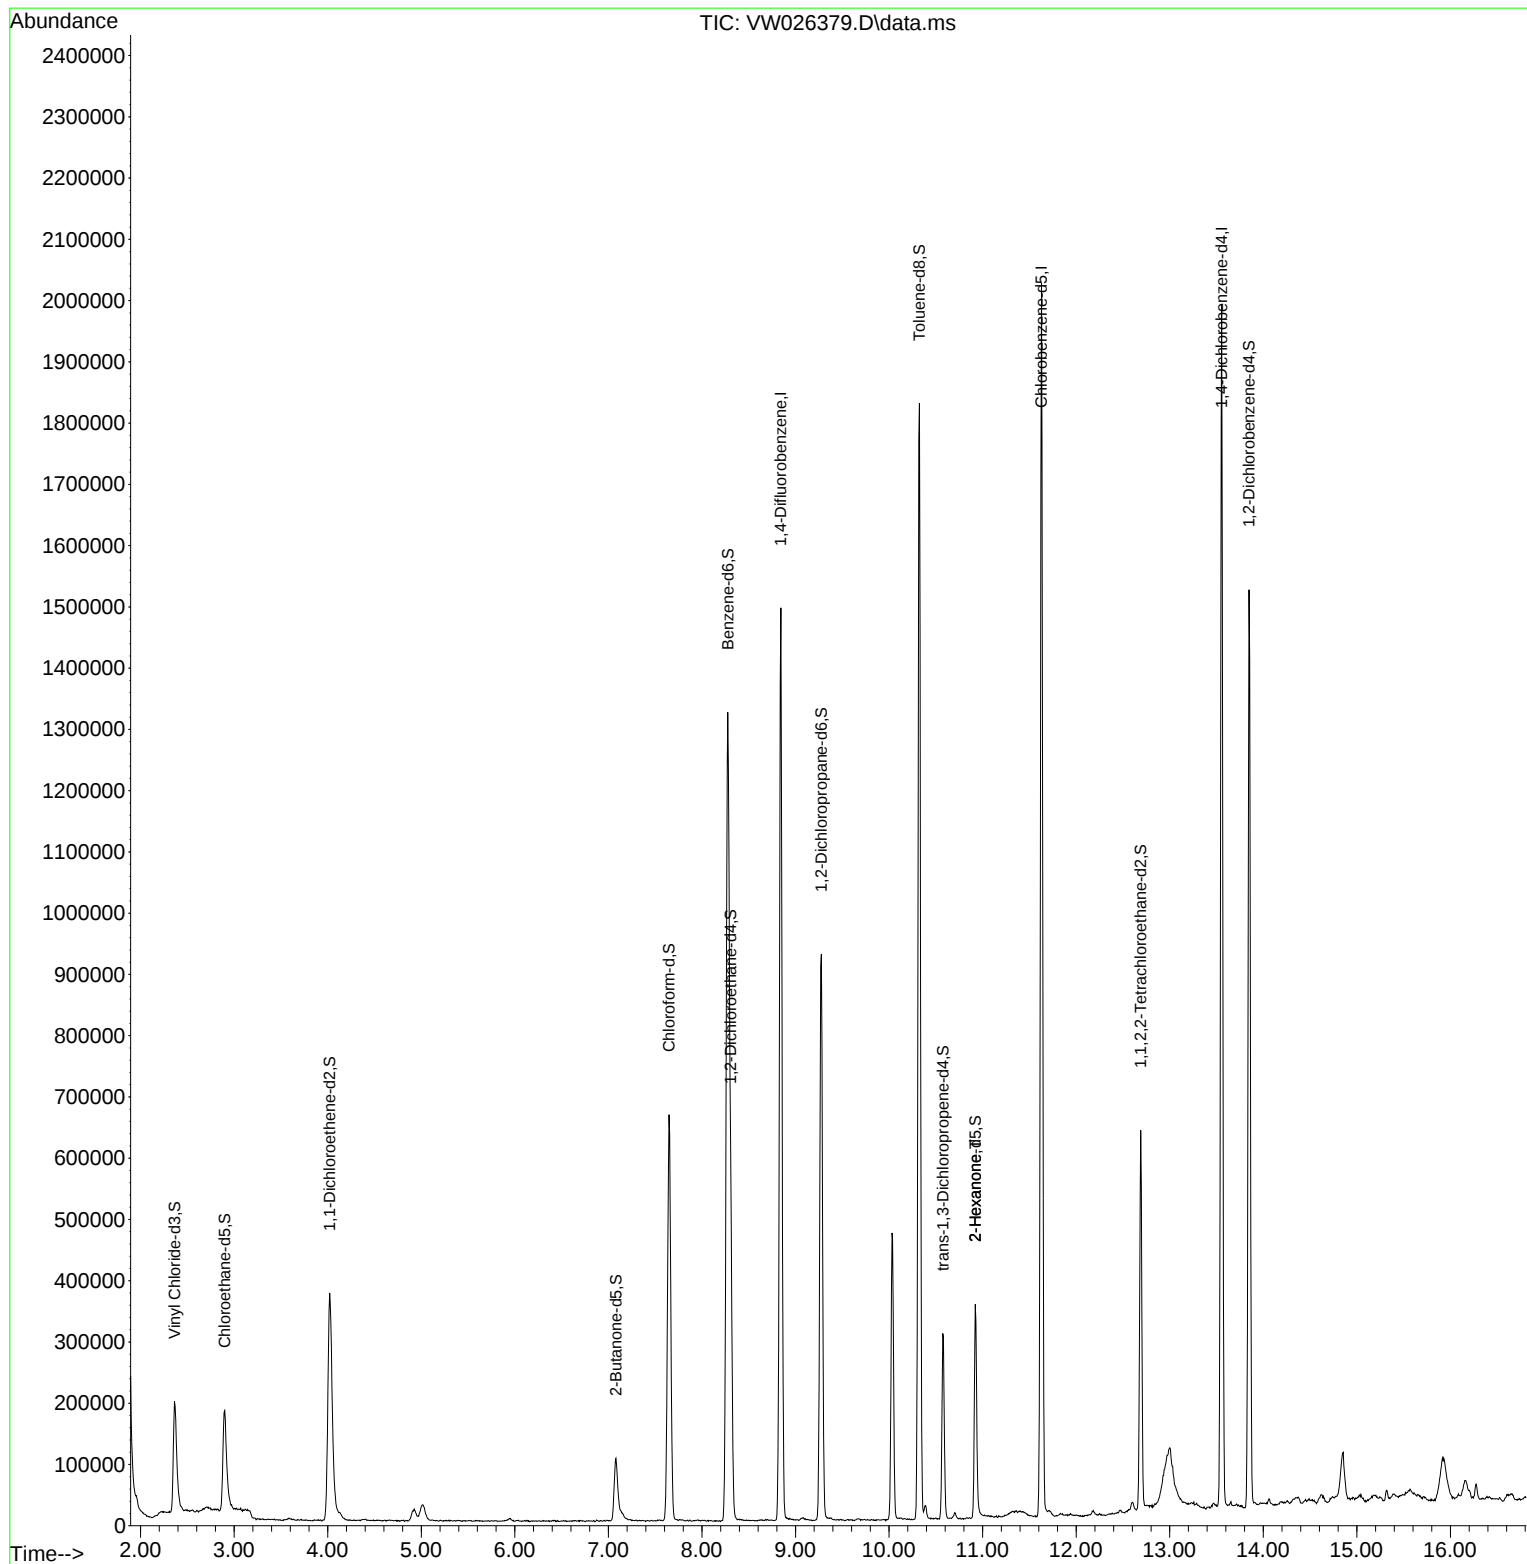

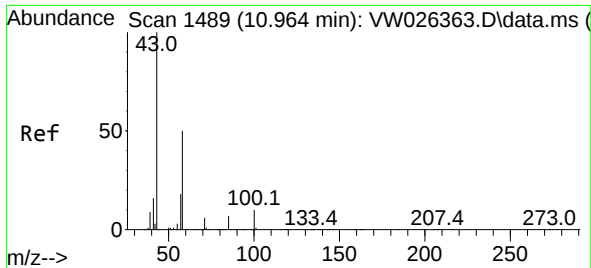

#48
 2-Hexanone
 Concen: 1.957 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.042 min
 Lab File: VW026379.D
 Acq: 28 Jun 2023 02:01

Instrument :
 MSVOA_W
 ClientSampleId :
 A46G9

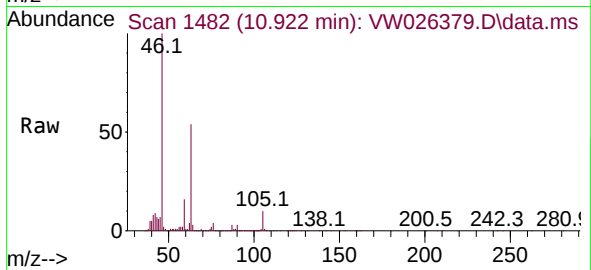

Tgt Ion: 43 Resp: 16561
 Ion Ratio Lower Upper
 43 100
 58 22.0 40.1 60.1#
 57 23.5 13.4 20.0#
 100 1.8 8.2 12.2#

