




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026341.D
 Acq On : 27 Jun 2023 09:47
 Operator : SY/MD
 Sample : VW0627SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK526

Manual IntegrationsAPPROVED

Quant Time: Jun 28 01:19:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 01:18:48 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/28/2023
 Supervised By :Mahesh Dadoda 06/29/2023

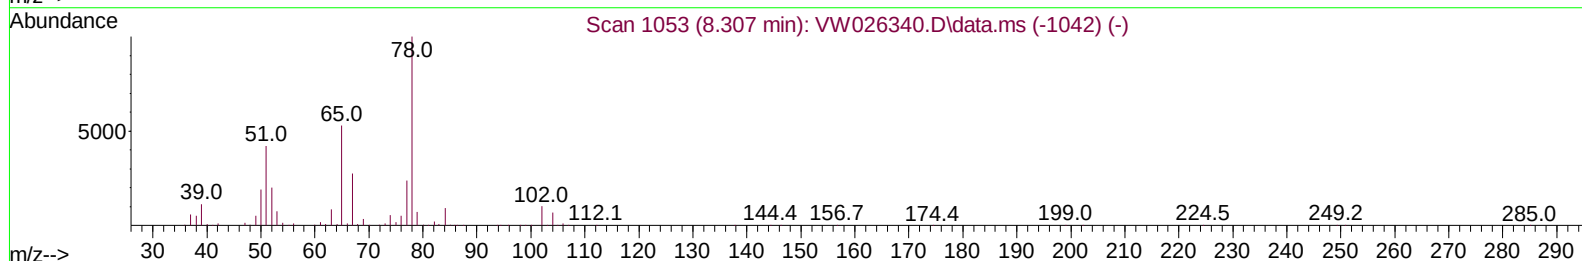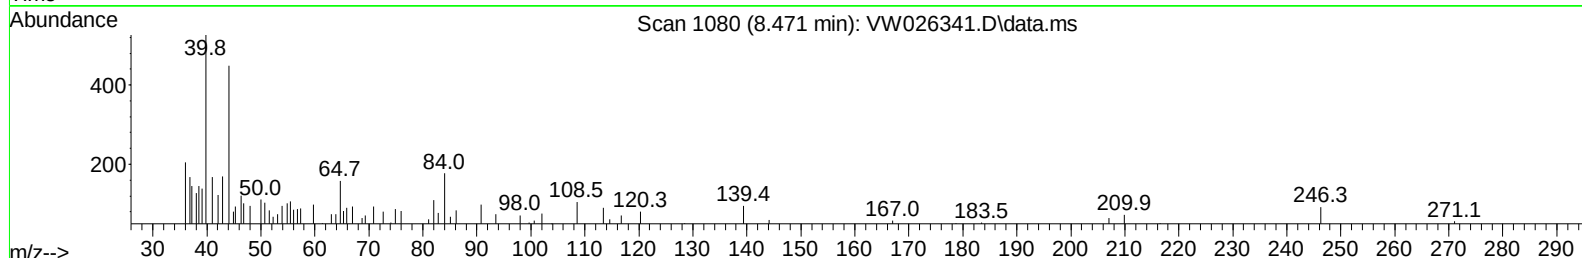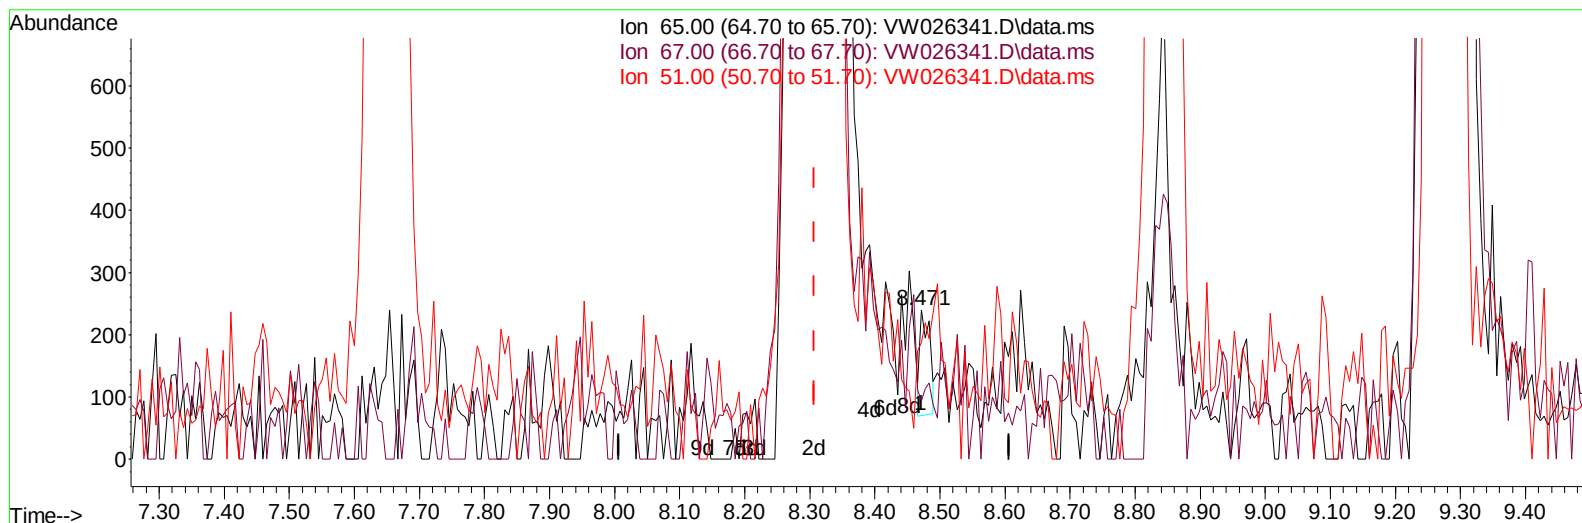

TIC: VW026341.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.471min (+ 0.165) 0.02 ug/L

response 182

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.20	37.91
51.00	117.60	115.38
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026341.D
 Acq On : 27 Jun 2023 09:47
 Operator : SY/MD
 Sample : VW0627SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK526

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/28/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 01:19:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 01:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		684476	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		631939	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		270824	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		255903	25.735	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	102.920%	
7) Chloroethane-d5	2.893	69		167990	23.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.040%	
11) 1,1-Dichloroethene-d2	4.027	65		111319	24.727	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	98.920%	
21) 2-Butanone-d5	7.081	46		123377	39.478	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	78.960%	
24) Chloroform-d	7.648	84		431094	22.226	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	88.920%	
26) 1,2-Dichloroethane-d4	8.307	65		253922m	23.299	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.200%	
32) Benzene-d6	8.276	84		896931	22.930	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	91.720%	
36) 1,2-Dichloropropane-d6	9.276	67		286397	22.533	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	90.120%	
41) Toluene-d8	10.325	98		765866	22.369	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	89.480%	
43) trans-1,3-Dichloroprop...	10.581	79		108294	21.221	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	84.880%	
47) 2-Hexanone-d5	10.922	63		75089	38.467	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	76.940%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		212830	21.268	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	85.080%	
66) 1,2-Dichlorobenzene-d4	13.849	152		228357	24.217	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	96.880%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026341.D
Acq On : 27 Jun 2023 09:47
Operator : SY/MD
Sample : VW0627SBL01
Misc : 5.00g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK526

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/28/2023
Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 01:19:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 01:18:48 2023
Response via : Initial Calibration

