

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026356.D
 Acq On : 27 Jun 2023 15:50
 Operator : SY/MD
 Sample : 03421-13
 Misc : 6.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46H2

Quant Time: Jun 28 01:23:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 01:18:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	1156296	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1019382	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	457226	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	306651	18.255	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.000%
7) Chloroethane-d5	2.893	69	291256	24.390	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.560%
11) 1,1-Dichloroethene-d2	4.021	65	158097	20.788	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.160%
21) 2-Butanone-d5	7.075	46	228993	43.375	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.740%
24) Chloroform-d	7.648	84	659280	20.121	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.480%
26) 1,2-Dichloroethane-d4	8.306	65	415261	22.555	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.240%
32) Benzene-d6	8.276	84	1351058	21.412	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.640%
36) 1,2-Dichloropropane-d6	9.276	67	430861	21.015	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.040%
41) Toluene-d8	10.324	98	1197913	21.690	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.760%
43) trans-1,3-Dichloroprop...	10.574	79	176567	21.449	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.800%
47) 2-Hexanone-d5	10.922	63	153056	48.608	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.220%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	345664	21.414	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	354209	22.249	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.000%
Target Compounds					Qvalue	
13) Acetone	4.124	43	29961	7.090	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026356.D
Acq On : 27 Jun 2023 15:50
Operator : SY/MD
Sample : 03421-13
Misc : 6.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46H2

Quant Time: Jun 28 01:23:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 01:18:48 2023
Response via : Initial Calibration

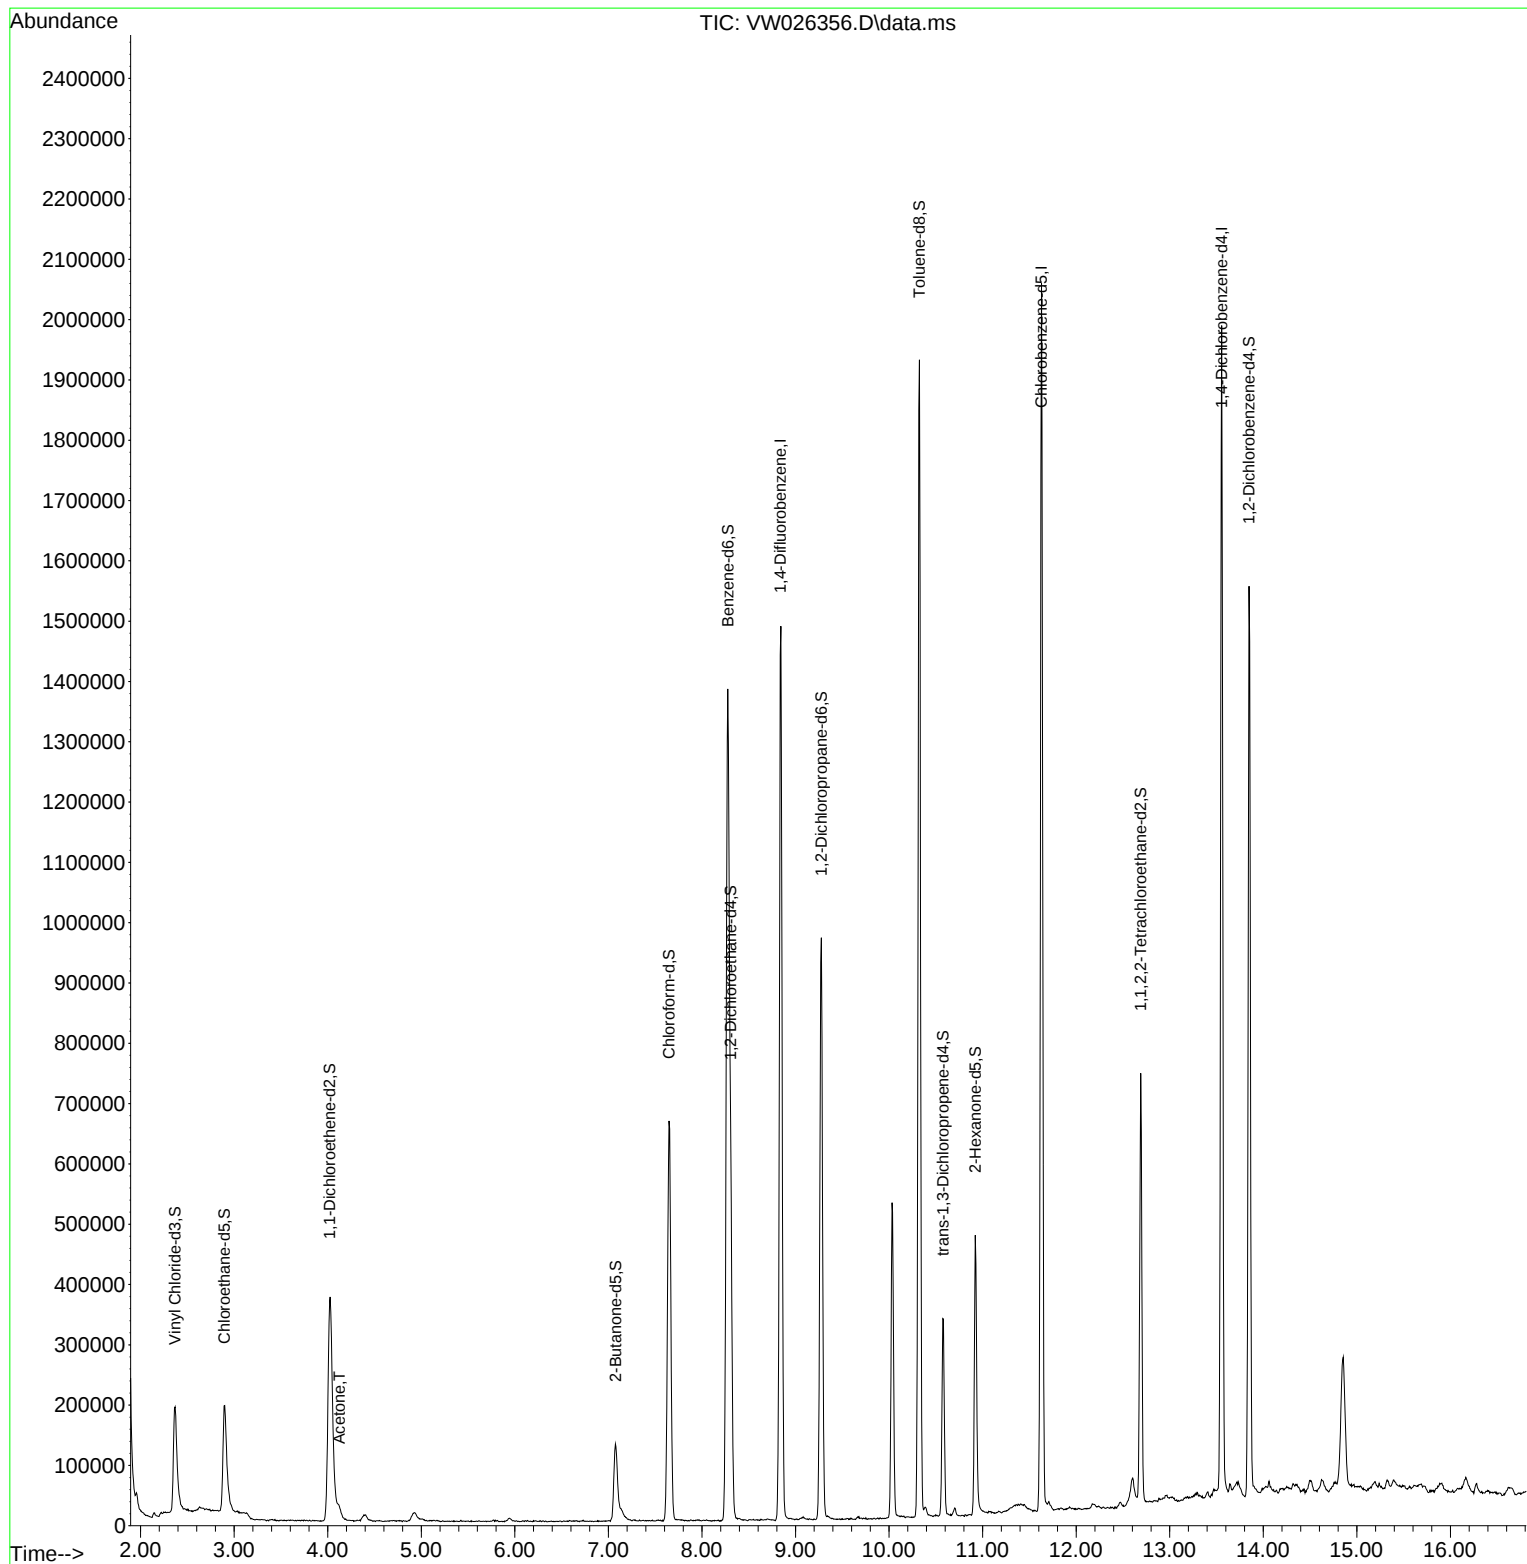

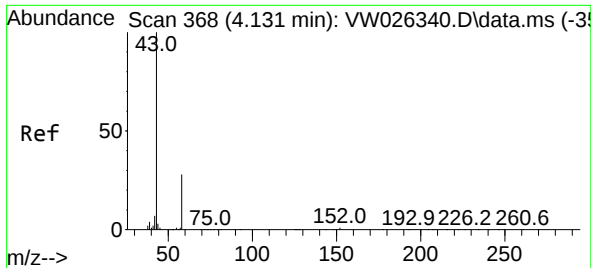

#13
 Acetone
 Concen: 7.090 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW026356.D
 Acq: 27 Jun 2023 15:50

Instrument :
 MSVOA_W
 ClientSampleId :
 A46H2

Tgt Ion: 43 Resp: 29961
 Ion Ratio Lower Upper
 43 100
 58 28.9 0.0 55.8

