

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026366.D
 Acq On : 27 Jun 2023 20:50
 Operator : SY/MD
 Sample : 03420-03
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4639

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/28/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 05:53:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 05:31:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1115634	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	996702	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	440651	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	302953	18.692	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.760%		
7) Chloroethane-d5	2.893	69	268532	23.307	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.240%		
11) 1,1-Dichloroethene-d2	4.021	65	154194	21.014	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	84.040%		
21) 2-Butanone-d5	7.075	46	191085	37.514	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	75.020%		
24) Chloroform-d	7.648	84	663849	20.999	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.000%		
26) 1,2-Dichloroethane-d4	8.307	65	404584m	22.776	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.120%		
32) Benzene-d6	8.276	84	1325328	21.482	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.920%		
36) 1,2-Dichloropropane-d6	9.270	67	425399	21.220	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.880%		
41) Toluene-d8	10.325	98	1161153	21.503	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.000%		
43) trans-1,3-Dichloroprop...	10.575	79	167271	20.782	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.120%		
47) 2-Hexanone-d5	10.922	63	125031	40.611	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.220%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	310377	19.665	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	78.680%		
66) 1,2-Dichlorobenzene-d4	13.849	152	352091	22.948	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.800%		
Target Compounds					Qvalue	
13) Acetone	4.119	43	25986	6.374	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026366.D
Acq On : 27 Jun 2023 20:50
Operator : SY/MD
Sample : 03420-03
Misc : 5.64g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4639

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/28/2023
Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 05:53:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 05:31:59 2023
Response via : Initial Calibration

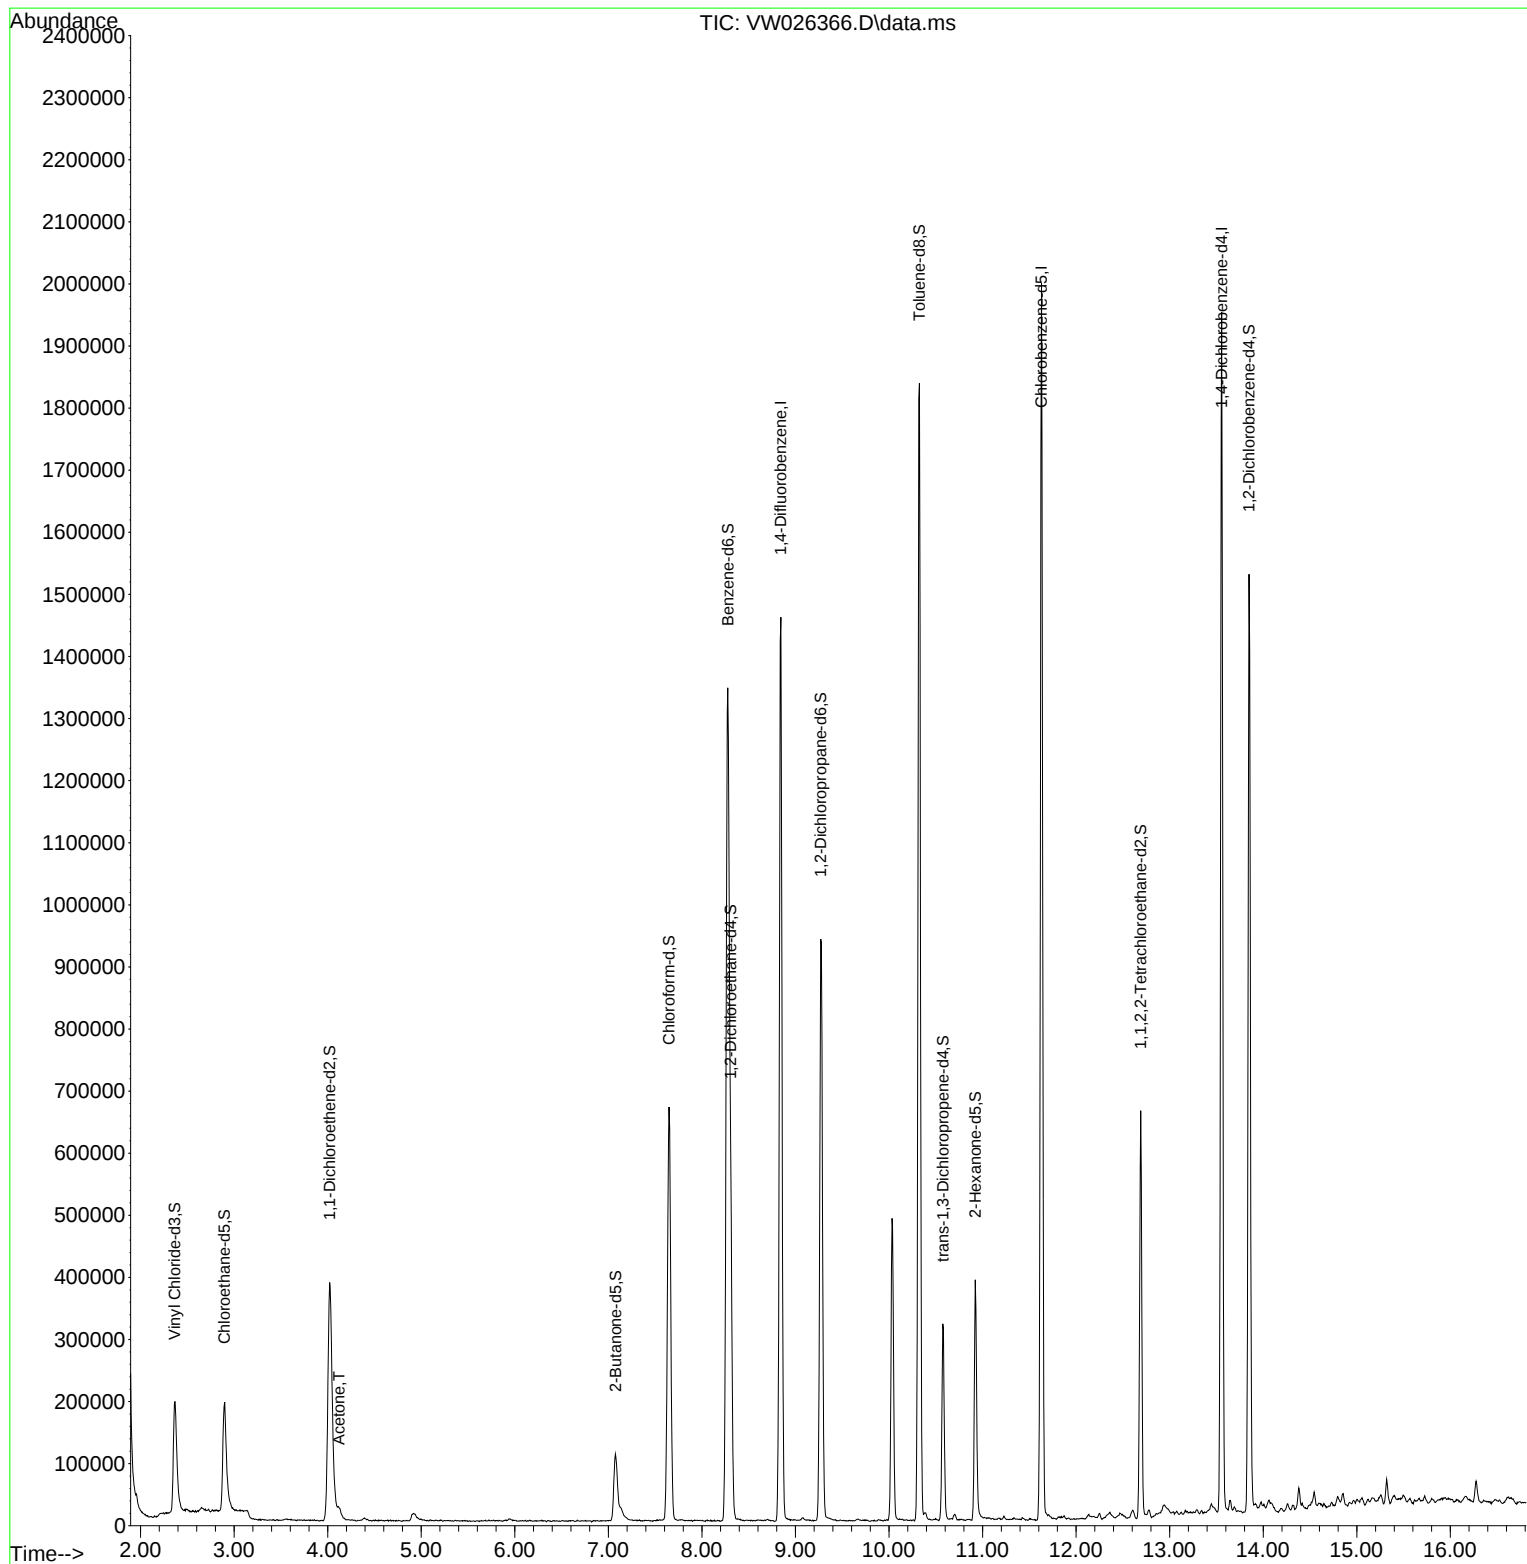

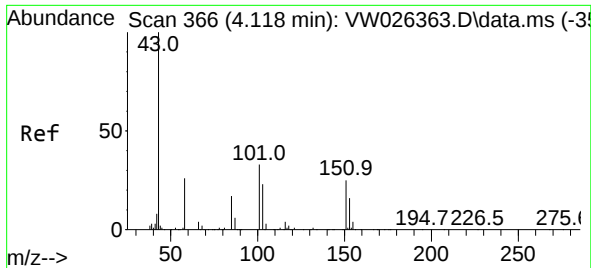

#13
 Acetone
 Concen: 6.374 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW026366.D
 Acq: 27 Jun 2023 20:50

Instrument :
 MSVOA_W
 ClientSampleId :
 A4639

Tgt Ion: 43 Resp: 2598
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 55.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/28/2023
 Supervised By :Mahesh Dadoda 06/29/2023

