

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026377.D
 Acq On : 28 Jun 2023 01:13
 Operator : SY/MD
 Sample : 03420-16
 Misc : 4.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46F1

Quant Time: Jun 28 05:56:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 05:31:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1288444	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1147727	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	535841	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	322875	17.249	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.000%
7) Chloroethane-d5	2.893	69	271386	20.395	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.600%
11) 1,1-Dichloroethene-d2	4.021	65	161574	19.066	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.280%
21) 2-Butanone-d5	7.075	46	231156	39.294	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.580%
24) Chloroform-d	7.648	84	699710	19.165	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.640%
26) 1,2-Dichloroethane-d4	8.307	65	436193	21.262	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.040%
32) Benzene-d6	8.276	84	1414663	19.913	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.640%
36) 1,2-Dichloropropane-d6	9.276	67	458722	19.871	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.480%
41) Toluene-d8	10.325	98	1295128	20.828	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.320%
43) trans-1,3-Dichloroprop...	10.581	79	185339	19.997	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.000%
47) 2-Hexanone-d5	10.922	63	161659	45.599	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	361027	19.865	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.440%
66) 1,2-Dichlorobenzene-d4	13.855	152	397850	21.324	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.280%
Target Compounds						
13) Acetone	4.125	43	18848	4.003	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026377.D
Acq On : 28 Jun 2023 01:13
Operator : SY/MD
Sample : 03420-16
Misc : 4.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46F1

Quant Time: Jun 28 05:56:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 05:31:59 2023
Response via : Initial Calibration

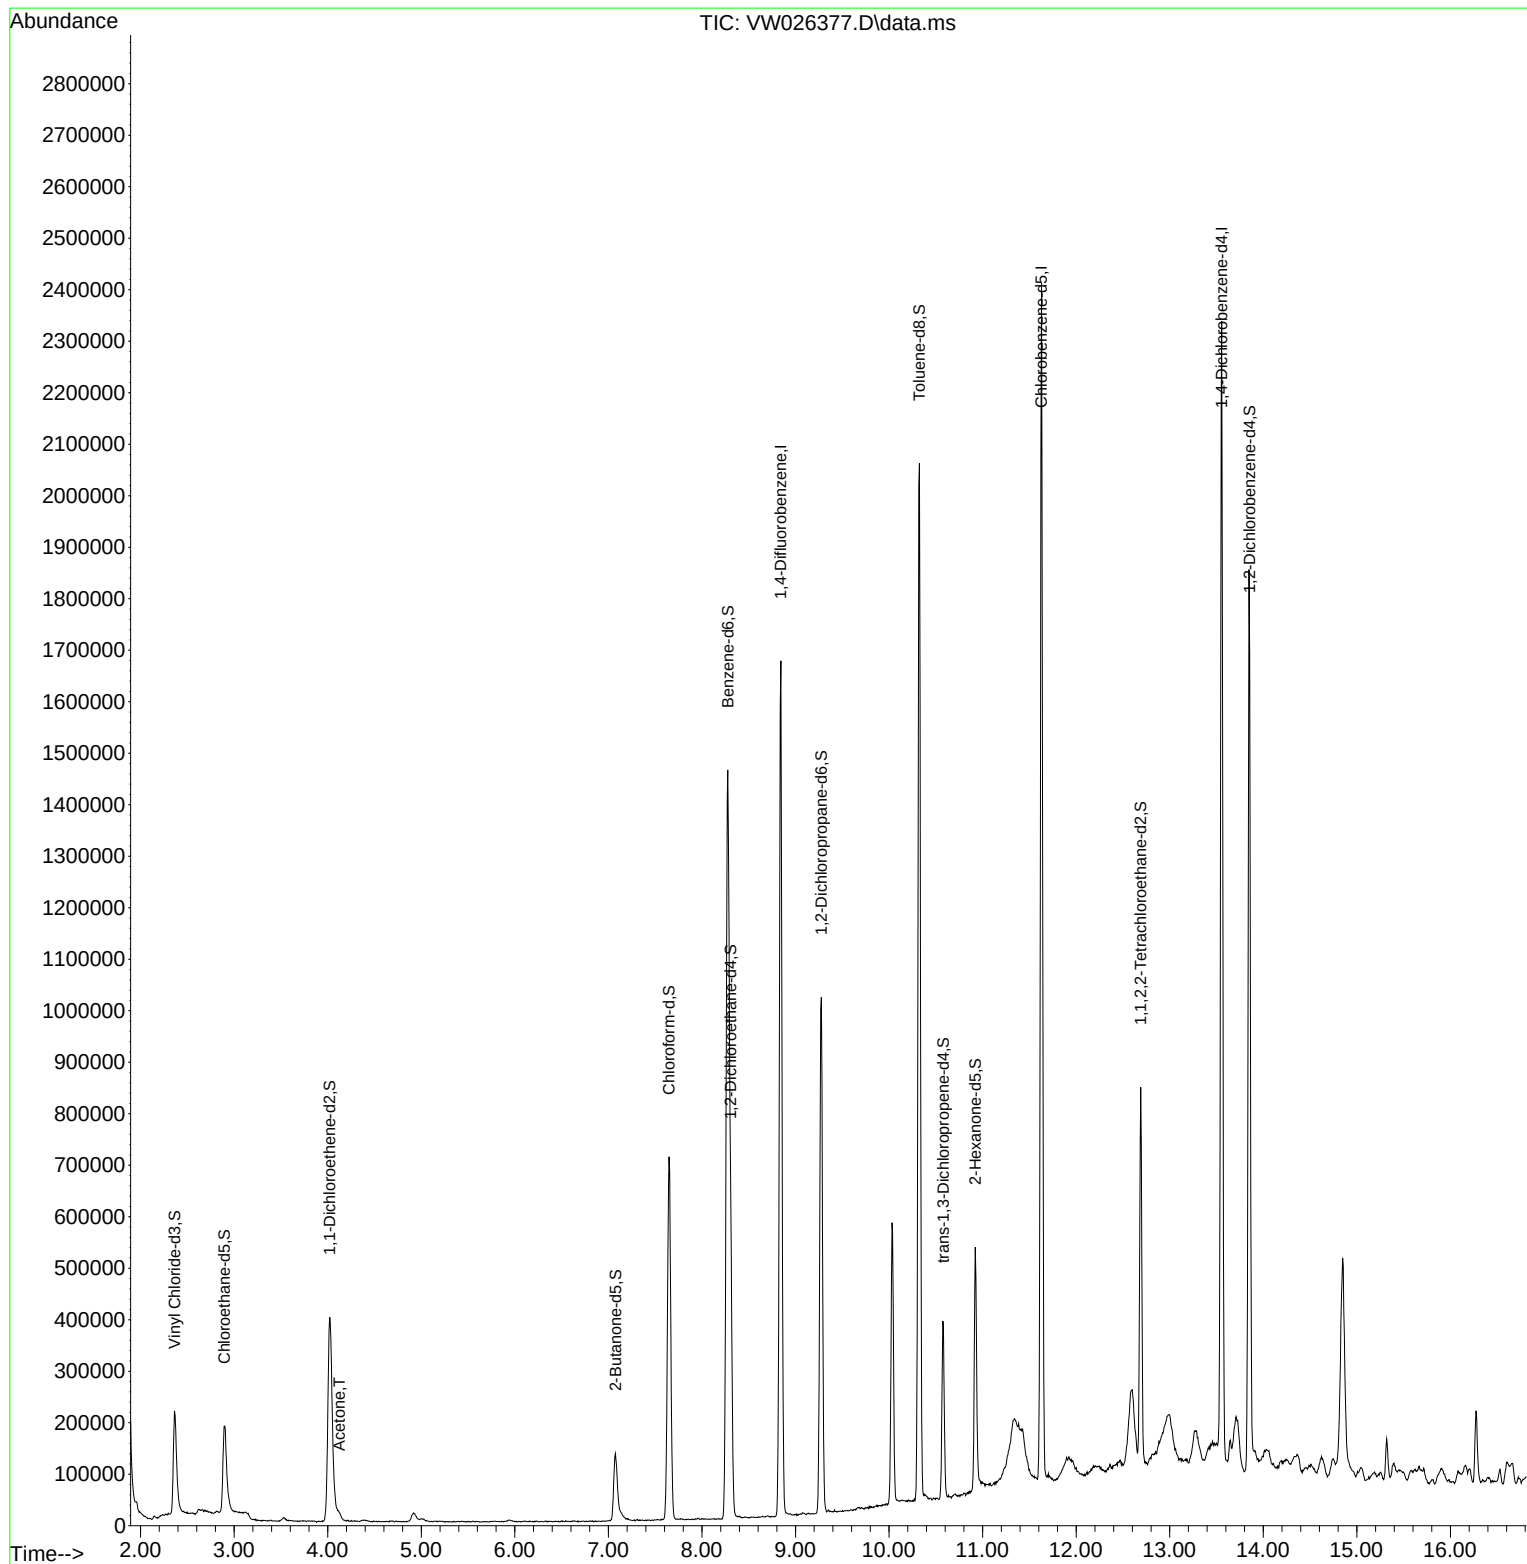

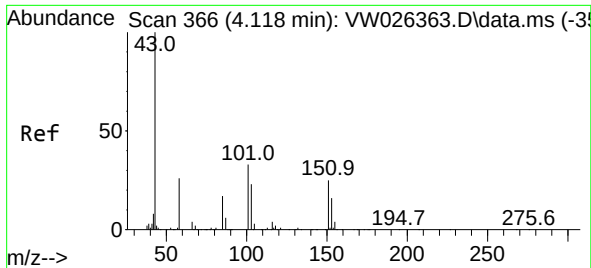

#13
 Acetone
 Concen: 4.003 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.007 min
 Lab File: VW026377.D
 Acq: 28 Jun 2023 01:13

Instrument :
 MSVOA_W
 ClientSampleId :
 A46F1

Tgt Ion: 43 Resp: 18848
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 55.8

