

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026383.D
 Acq On : 28 Jun 2023 03:37
 Operator : SY/MD
 Sample : 03420-23MSD
 Misc : 5.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46K5MSD

Quant Time: Jun 28 05:58:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 05:31:59 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin
 Yesilyurt

06/28/2023
 Supervised By : Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	864593	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	602387	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	167683	25.000	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.363	65	309821	24.666	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.680%
7) Chloroethane-d5	2.899	69	250762	28.084	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.320%
11) 1,1-Dichloroethene-d2	4.021	65	142513	25.061	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	100.240%
21) 2-Butanone-d5	7.075	46	169671	42.981	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.960%
24) Chloroform-d	7.648	84	547096	22.331	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.320%
26) 1,2-Dichloroethane-d4	8.307	65	311881	22.656	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.640%
32) Benzene-d6	8.276	84	1061618	28.472	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.880%
36) 1,2-Dichloropropane-d6	9.276	67	329661	27.209	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.840%
41) Toluene-d8	10.325	98	837185	25.652	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.600%
43) trans-1,3-Dichloroprop...	10.575	79	106113	21.813	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.240%
47) 2-Hexanone-d5	10.922	63	112931	60.692	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.380%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	210135	22.029	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.120%
66) 1,2-Dichlorobenzene-d4	13.854	152	123987	21.236	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.960%

Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.015	85	253902	24.430	ug/L	89
3) Chloromethane	2.222	50	349711	23.271	ug/L	99
5) Vinyl chloride	2.375	62	353347	22.614	ug/L	100
6) Bromomethane	2.789	94	182226	21.247	ug/L	99
8) Chloroethane	2.930	64	220260	26.289	ug/L	99
9) Trichlorofluoromethane	3.265	101	264361	23.986	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	4.076	101	215800	18.087	ug/L	98
12) 1,1-Dichloroethene	4.045	96	250582	22.415	ug/L	99
13) Acetone	4.118	43	295099	93.396	ug/L	99
14) Carbon disulfide	4.387	76	728064	18.430	ug/L	99
15) Methyl Acetate	4.667	43	145284	20.057	ug/L	98
16) Methylene chloride	4.923	84	273693	18.706	ug/L	99
17) trans-1,2-Dichloroethene	5.429	96	245330	19.966	ug/L	94
18) Methyl tert-butyl Ether	5.423	73	479181	24.934	ug/L	98
19) 1,1-Dichloroethane	6.216	63	549158	21.340	ug/L	99
20) cis-1,2-Dichloroethene	7.173	96	276119	20.794	ug/L	99
22) 2-Butanone	7.167	43	263391	54.481	ug/L	99
23) Bromochloromethane	7.514	128	113551	19.937	ug/L	95
25) Chloroform	7.679	83	504852	21.168	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
 Data File : VW026383.D
 Acq On : 28 Jun 2023 03:37
 Operator : SY/MD
 Sample : 03420-23MSD
 Misc : 5.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46K5MSD

Quant Time: Jun 28 05:58:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 05:31:59 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Semsettin
 Yesilyurt

06/28/2023
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	8.398	62	370806	21.625	ug/L	96
29) Cyclohexane	7.959	56	316345	18.186	ug/L	98
30) 1,1,1-Trichloroethane	7.874	97	397187	27.256	ug/L	100
31) Carbon tetrachloride	8.069	117	255851	19.531	ug/L	100
33) Benzene	8.325	78	1079893	26.540	ug/L	100
34) Trichloroethene	9.087	95	259669	24.925	ug/L	91
35) Methylcyclohexane	9.337	83	221746	12.412	ug/L	100
37) 1,2-Dichloropropane	9.367	63	290562	25.559	ug/L	99
38) Bromodichloromethane	9.642	83	324127	24.827	ug/L	96
39) cis-1,3-Dichloropropene	10.075	75	358904	22.035	ug/L	97
40) 4-Methyl-2-pentanone	10.209	43	424534	57.855	ug/L	99
42) Toluene	10.386	91	1002948	24.571	ug/L	97
44) trans-1,3-Dichloropropene	10.605	75	282823	20.571	ug/L	99
45) 1,1,2-Trichloroethane	10.788	97	193626	25.438	ug/L	98
46) Tetrachloroethene	10.861	164	123140	16.777	ug/L	94
48) 2-Hexanone	10.965	43	279072	53.901	ug/L	96
49) Dibromochloromethane	11.129	129	179424	23.021	ug/L	97
50) 1,2-Dibromoethane	11.233	107	171958	24.607	ug/L	100
51) Chlorobenzene	11.654	112	521475	20.028	ug/L	98
52) Ethylbenzene	11.727	91	890042	19.351	ug/L	97
53) m,p-Xylene	11.837	106	311770	18.586	ug/L	98
54) o-Xylene	12.166	106	299624	18.971	ug/L	95
55) Styrene	12.178	104	459410	16.677	ug/L	99
57) 1,1,2,2-Tetrachloroethane	12.714	83	190080	19.978	ug/L	97
59) Bromoform	12.349	173	85542	33.722	ug/L	97
60) Isopropylbenzene	12.458	105	639816	25.387	ug/L	99
61) 1,2,3-Trichloropropane	12.763	75	159665	39.171	ug/L	96
62) 1,3,5-Trimethylbenzene	12.940	105	435427	22.288	ug/L	99
63) 1,2,4-Trimethylbenzene	13.245	105	430905	22.869	ug/L	99
64) 1,3-Dichlorobenzene	13.495	146	202352	18.746	ug/L	93
65) 1,4-Dichlorobenzene	13.574	146	213187	19.735	ug/L #	82
67) 1,2-Dichlorobenzene	13.867	146	184122	19.151	ug/L #	76
68) 1,2-Dibromo-3-chloropr...	14.482	75	28862	30.722	ug/L	97
69) 1,3,5-Trichlorobenzene	14.629	180	66189	9.542	ug/L	99
70) 1,2,4-trichlorobenzene	15.129	180	56882	10.021	ug/L #	65
71) Naphthalene	15.360	128	202691	17.763	ug/L #	86
72) 1,2,3-Trichlorobenzene	15.549	180	74721m	14.099	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062723\
Data File : VW026383.D
Acq On : 28 Jun 2023 03:37
Operator : SY/MD
Sample : 03420-23MSD
Misc : 5.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD


Manual Integrations
APPROVED


Reviewed By : Semsettin
Yesilyurt

06/28/2023
Supervised By : Mahesh
Dadoda

06/29/2023


Quant Time: Jun 28 05:58:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 05:31:59 2023
Response via : Initial Calibration

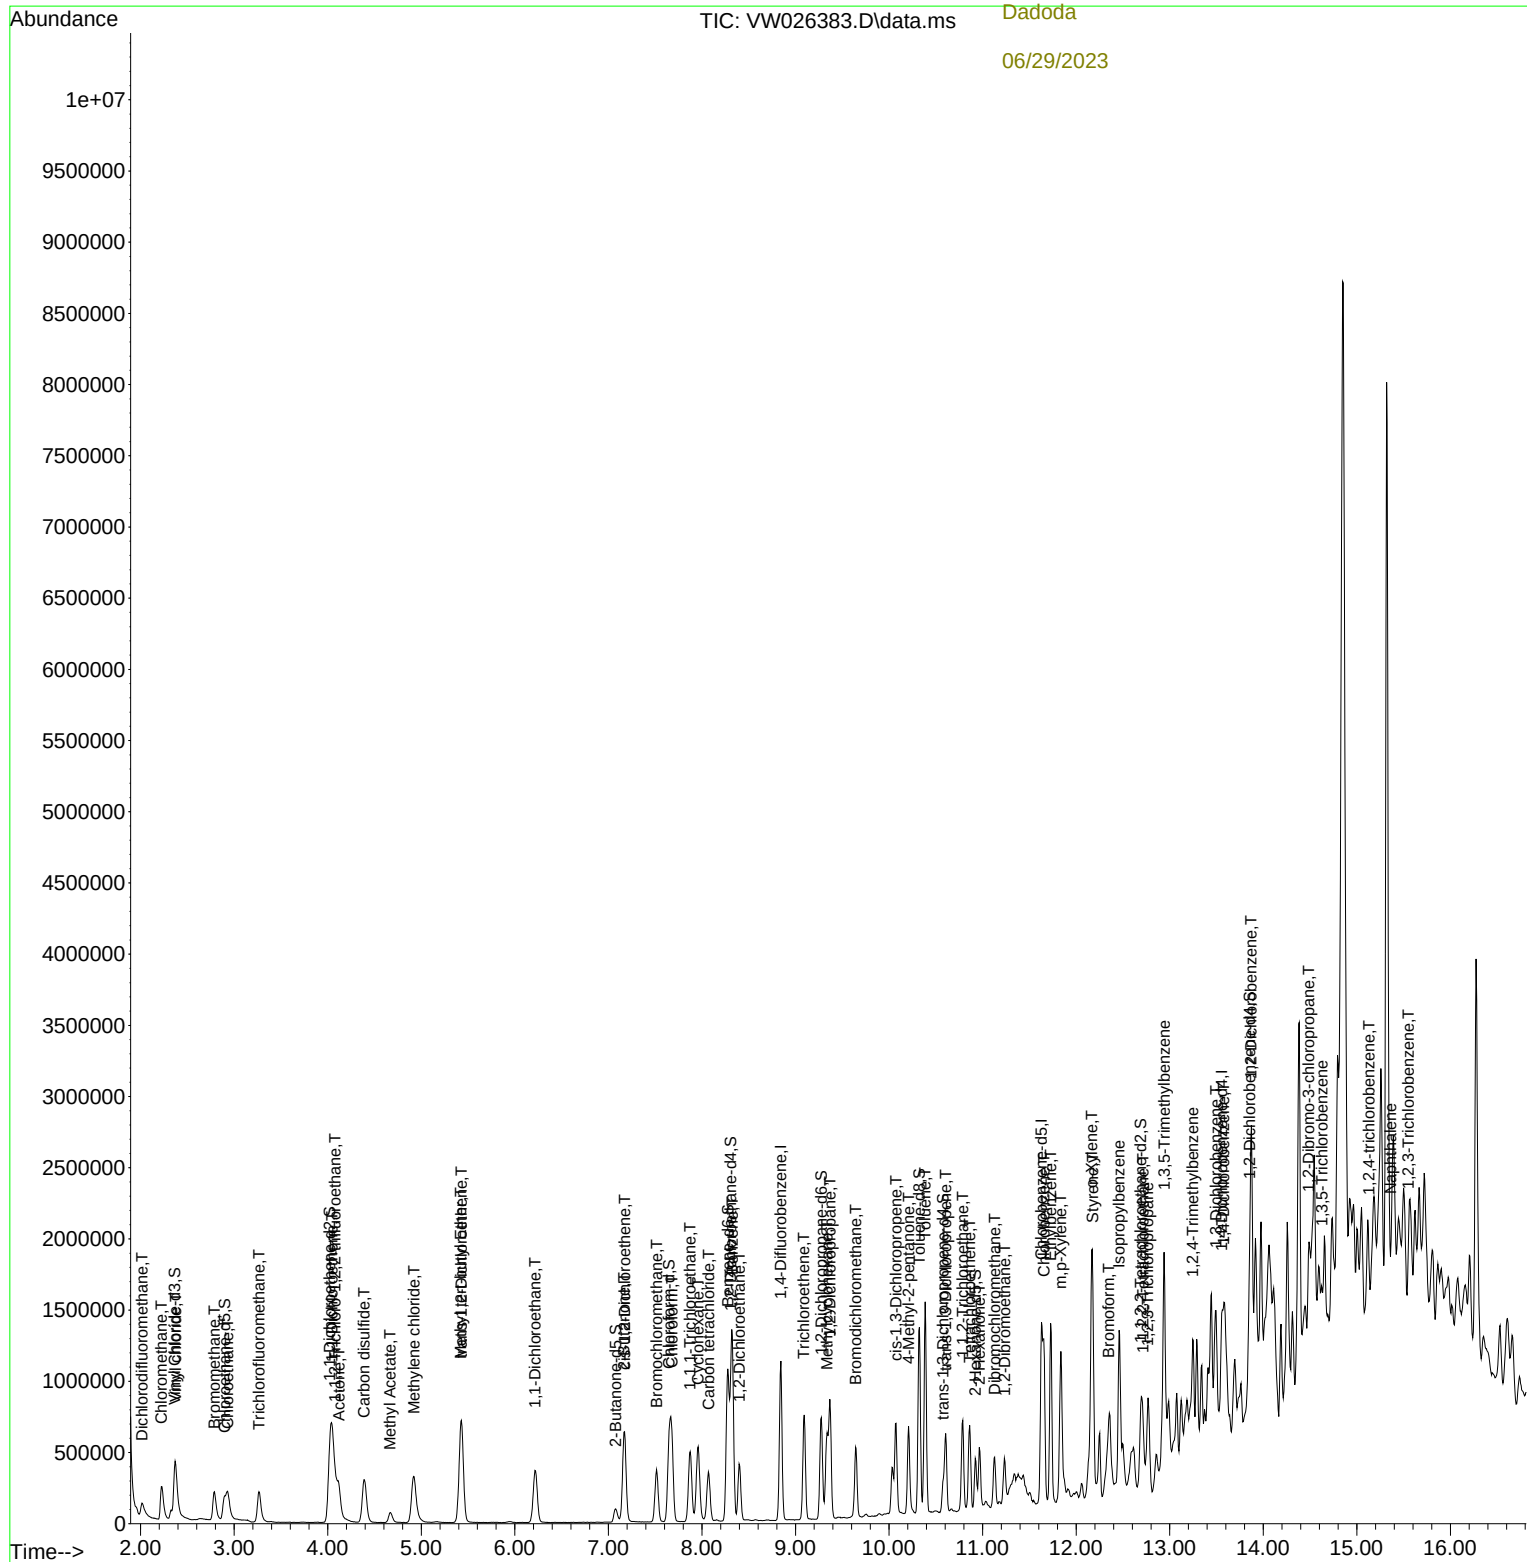



#2
Dichlorodifluoromethane
Concen: 24.430 ug/L
RT: 2.015 min Scan# 21
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 85 Resp: 25390
Ion Ratio Lower Upper
85 100
87 25.6 25.2 37.8

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#3
Chloromethane
Concen: 23.271 ug/L
RT: 2.222 min Scan# 55
Delta R.T. -0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 50 Resp: 349711
Ion Ratio Lower Upper
50 100
52 30.9 21.4 39.8

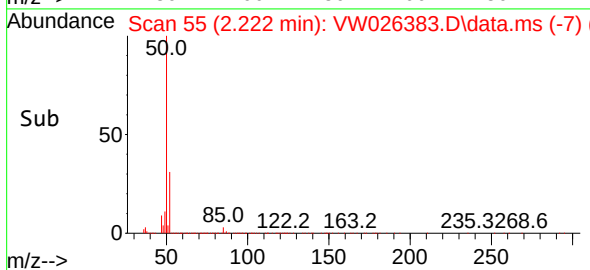



#5
 Vinyl chloride
 Concen: 22.614 ug/L
 RT: 2.375 min Scan# 80
 Delta R.T. 0.000 min
 Lab File: VW026383.D
 Acq: 28 Jun 2023 03:37

Instrument :
 MSVOA_W
 ClientSampleId :
 A46K5MSD

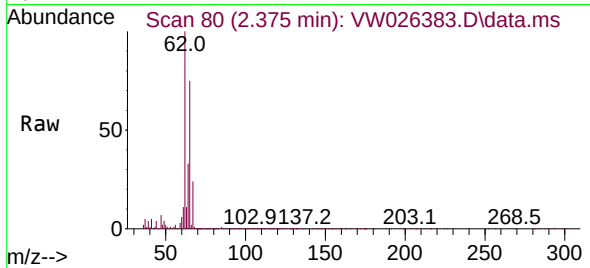




Tgt Ion: 62 Resp: 35334
 Ion Ratio Lower Upper
 62 100
 64 33.0 23.0 42.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin
 Yesilyurt




06/28/2023
 Supervised By :Mahesh
 Dadoda


06/29/2023

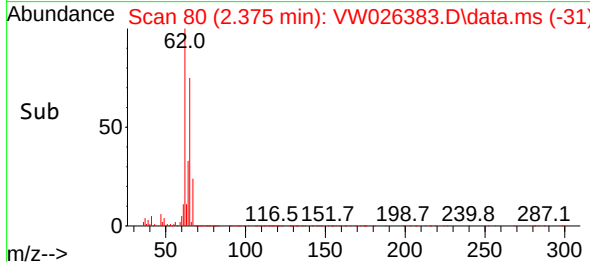

#6
 Bromomethane
 Concen: 21.247 ug/L
 RT: 2.789 min Scan# 148
 Delta R.T. 0.000 min
 Lab File: VW026383.D
 Acq: 28 Jun 2023 03:37


Tgt Ion: 94 Resp: 182226
 Ion Ratio Lower Upper
 94 100
 96 91.0 64.6 120.0

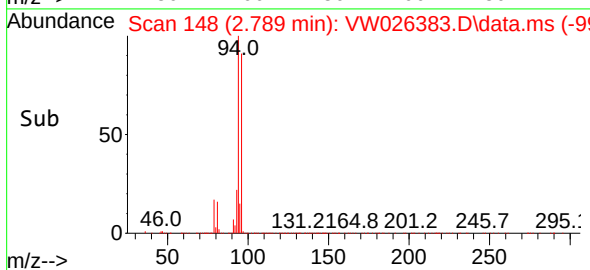



#8
Chloroethane
Concen: 26.289 ug/L
RT: 2.930 min Scan# 171
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 64 Resp: 220260
Ion Ratio Lower Upper
64 100
66 31.6 22.5 41.7

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#9
Trichlorofluoromethane
Concen: 23.986 ug/L
RT: 3.265 min Scan# 226
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:101 Resp: 264361
Ion Ratio Lower Upper
101 100
103 64.7 52.9 79.3

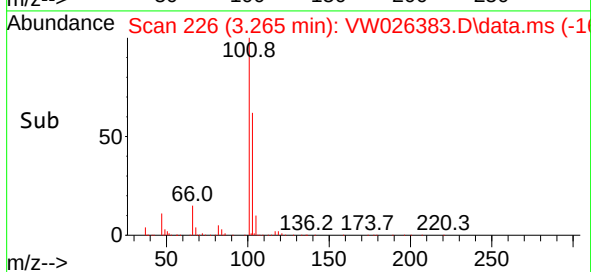

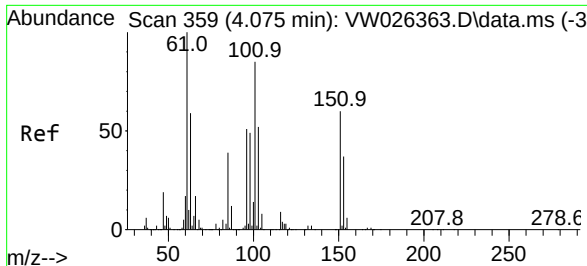

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 18.087 ug/L
 RT: 4.076 min Scan# 359
 Delta R.T. 0.000 min
 Lab File: VW026383.D
 Acq: 28 Jun 2023 03:37

Instrument :
 MSVOA_W
 ClientSampleId :
 A46K5MSD

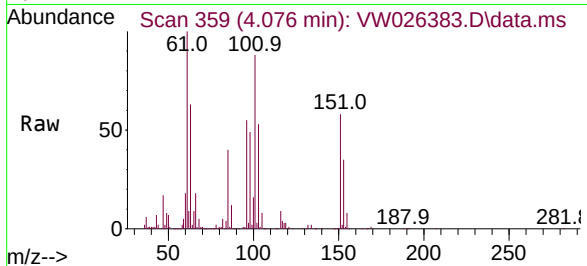




Tgt Ion:101 Resp: 215800
 Ion Ratio Lower Upper
 101 100
 85 43.2 35.4 53.0
 151 68.4 56.1 84.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin
 Yesilyurt




06/28/2023
 Supervised By :Mahesh
 Dadoda


06/29/2023

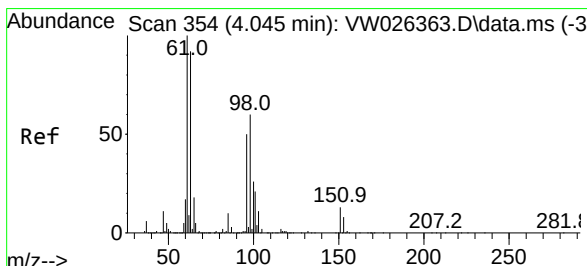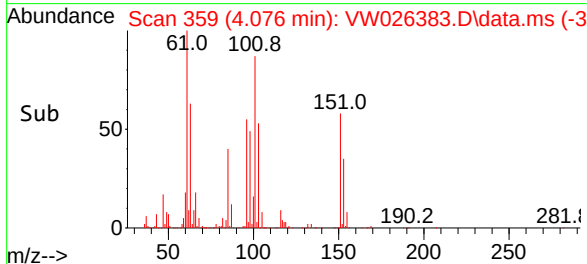

#12
 1,1-Dichloroethene
 Concen: 22.415 ug/L
 RT: 4.045 min Scan# 354
 Delta R.T. 0.000 min
 Lab File: VW026383.D
 Acq: 28 Jun 2023 03:37


Tgt Ion: 96 Resp: 250582
 Ion Ratio Lower Upper
 96 100
 61 194.7 134.3 249.3
 63 159.4 112.3 208.5

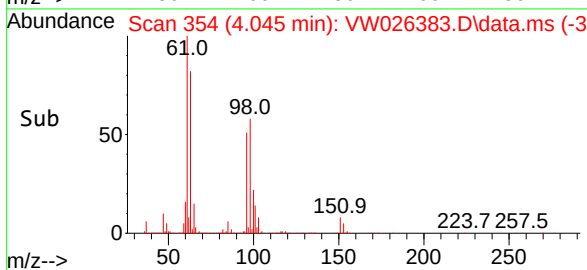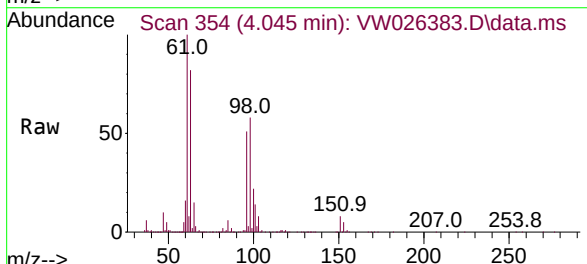



#13
Acetone
Concen: 93.396 ug/L
RT: 4.118 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 43 Resp: 295099
Ion Ratio Lower Upper
43 100
58 27.6 0.0 55.8

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

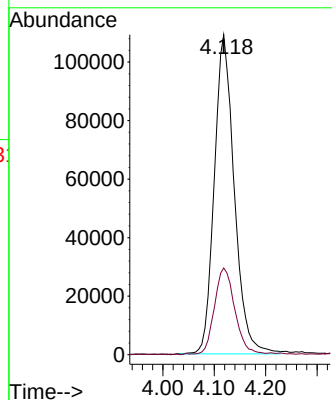

#14
Carbon disulfide
Concen: 18.430 ug/L
RT: 4.387 min Scan# 410
Delta R.T. -0.012 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 76 Resp: 728064
Ion Ratio Lower Upper
76 100
78 9.3 7.2 10.8

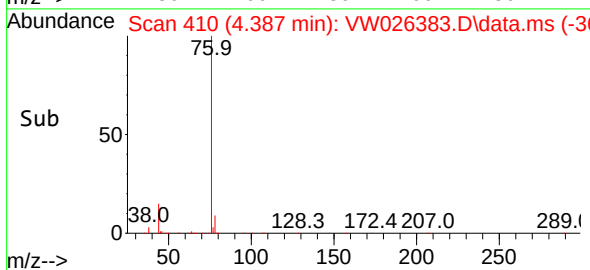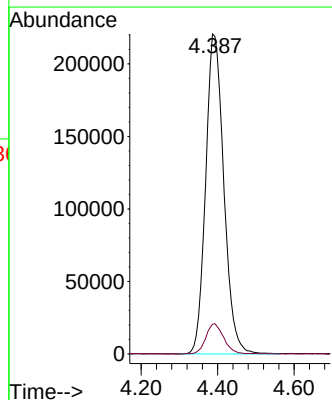

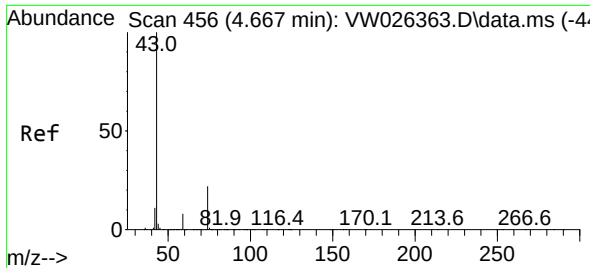

#15
Methyl Acetate
Concen: 20.057 ug/L
RT: 4.667 min Scan# 41
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD

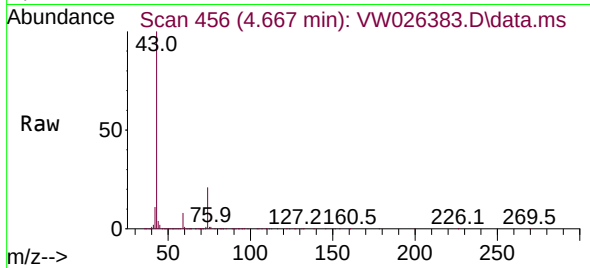




Tgt Ion: 43 Resp: 145284
Ion Ratio Lower Upper
43 100
74 21.1 16.3 24.5

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

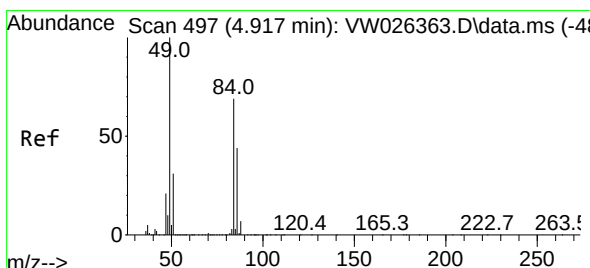

#16
Methylene chloride
Concen: 18.706 ug/L
RT: 4.923 min Scan# 498
Delta R.T. 0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 84 Resp: 273693
Ion Ratio Lower Upper
84 100
86 62.1 43.9 81.5
49 141.5 100.4 186.4

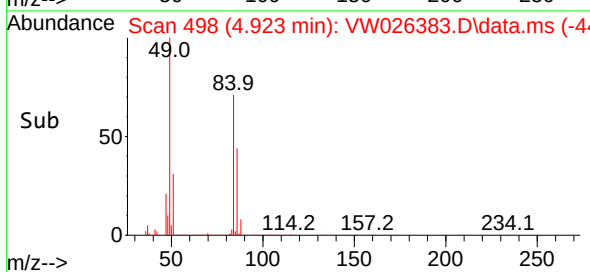



#17
trans-1,2-Dichloroethene
Concen: 19.966 ug/L
RT: 5.429 min Scan# 581
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 96 Resp: 245330
Ion Ratio Lower Upper
96 100
61 160.2 106.1 197.1
98 65.3 43.9 81.5

Manual Integrations
APPROVED


Reviewed By :Semsettin
Yesilyurt

06/28/2023
Supervised By :Mahesh
Dadoda



06/29/2023

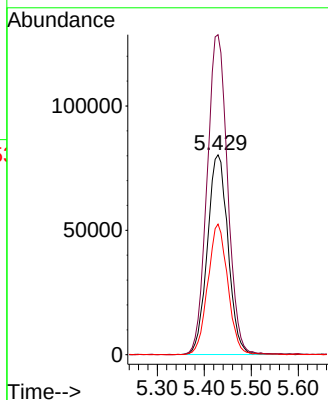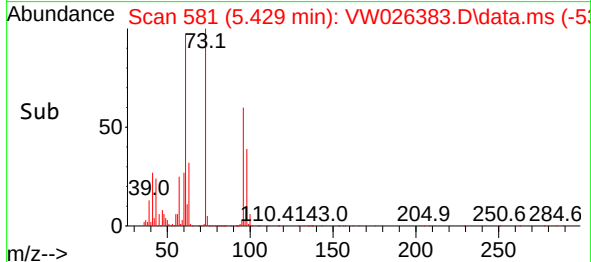


#18
Methyl tert-butyl Ether
Concen: 24.934 ug/L
RT: 5.423 min Scan# 580
Delta R.T. -0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37



Tgt Ion: 73 Resp: 479181
Ion Ratio Lower Upper
73 100
43 24.0 18.1 27.1
57 23.7 19.5 29.3

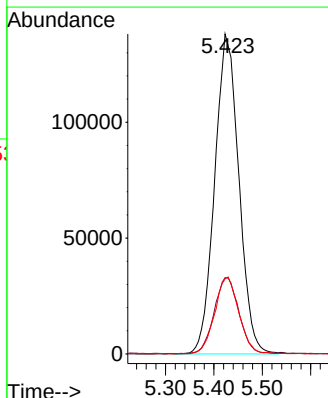



#19

1,1-Dichloroethane

Concen: 21.340 ug/L

RT: 6.216 min Scan# 711

Delta R.T. -0.006 min

Lab File: VW026383.D

Acq: 28 Jun 2023 03:37

Instrument :

MSVOA_W

ClientSampleId :

A46K5MSD

Tgt Ion: 63 Resp: 54915

Ion	Ratio	Lower	Upper
63	100		
65	32.0	22.8	42.4
83	12.5	8.7	16.1





Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt

06/28/2023

Supervised By :Mahesh
Dadoda

06/29/2023



#20

cis-1,2-Dichloroethene

Concen: 20.794 ug/L

RT: 7.173 min Scan# 867




Delta R.T. 0.000 min


Lab File: VW026383.D

Acq: 28 Jun 2023 03:37

Tgt Ion: 96 Resp: 276119


Ion	Ratio	Lower	Upper
96	100		
61	145.2	100.8	187.2
98	64.5	45.7	84.9

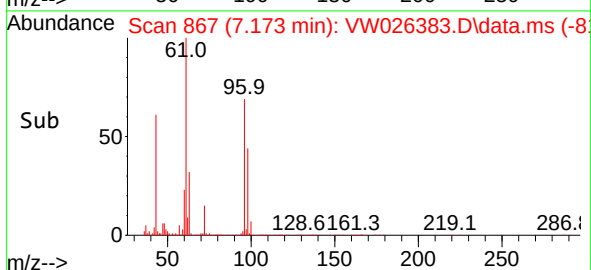



#22
2-Butanone
Concen: 54.481 ug/L
RT: 7.167 min Scan# 866
Delta R.T. -0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 43 Resp: 26339
Ion Ratio Lower Upper
43 100
72 23.9 11.8 35.3

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#23
Bromochloromethane
Concen: 19.937 ug/L
RT: 7.514 min Scan# 923
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:128 Resp: 113551
Ion Ratio Lower Upper
128 100
49 214.7 148.5 275.9
130 131.8 82.6 153.4
51 66.1 54.2 81.4

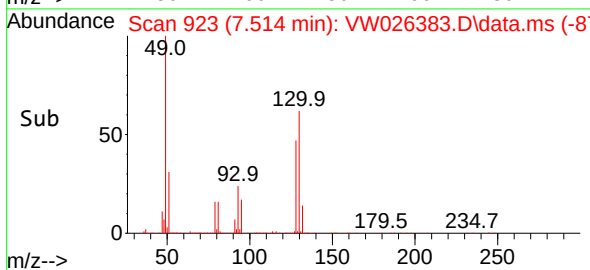



#25
Chloroform
Concen: 21.168 ug/L
RT: 7.679 min Scan# 949
Delta R.T. 0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 83 Resp: 504852
Ion Ratio Lower Upper
83 100
85 62.8 45.3 84.1

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#27
1,2-Dichloroethane
Concen: 21.625 ug/L
RT: 8.398 min Scan# 1068
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 62 Resp: 370806
Ion Ratio Lower Upper
62 100
98 7.8 7.5 11.3

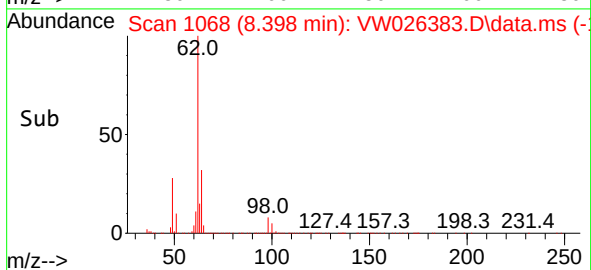



#29
Cyclohexane
Concen: 18.186 ug/L
RT: 7.959 min Scan# 996
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 56 Resp: 316345
Ion Ratio Lower Upper
56 100
69 29.1 23.0 34.4
84 77.5 63.4 95.0

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#30
1,1,1-Trichloroethane
Concen: 27.256 ug/L
RT: 7.874 min Scan# 982
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 97 Resp: 397187
Ion Ratio Lower Upper
97 100
99 64.1 50.8 76.2
61 51.7 41.4 62.2

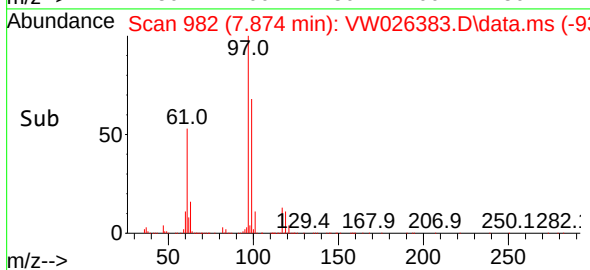

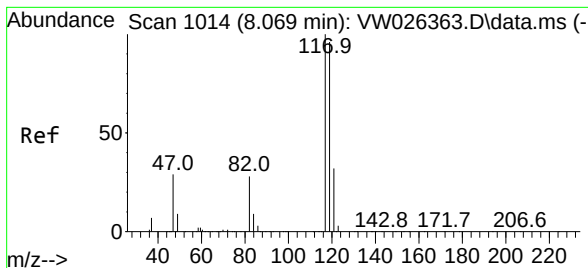

#31
Carbon tetrachloride
Concen: 19.531 ug/L
RT: 8.069 min Scan# 1014
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD

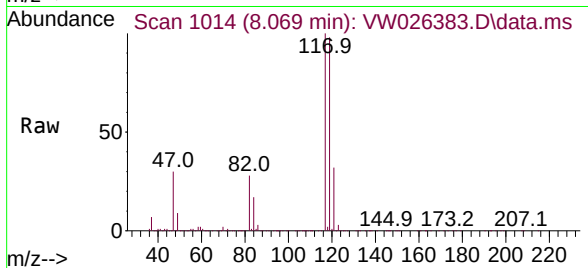



Tgt Ion:117 Resp: 25585
Ion Ratio Lower Upper
117 100
119 96.8 77.7 116.5

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

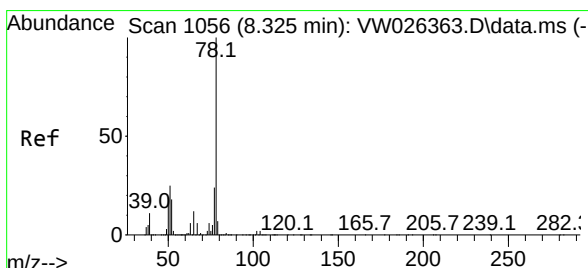

#33
Benzene
Concen: 26.540 ug/L
RT: 8.325 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Tgt Ion: 78 Resp: 1079893

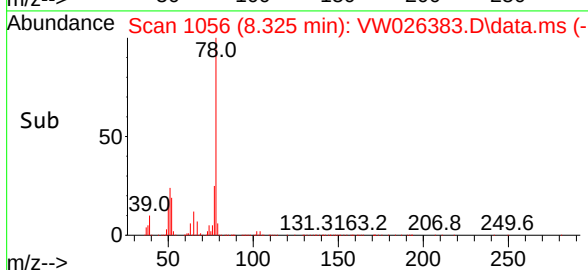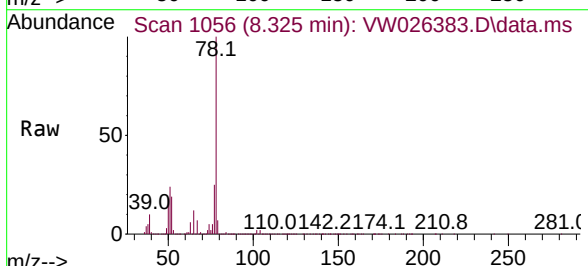

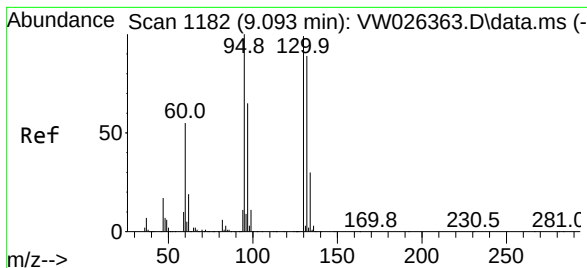

#34

Trichloroethene

Concen: 24.925 ug/L

RT: 9.087 min Scan# 1182

Delta R.T. -0.006 min

Lab File: VW026383.D


Acq: 28 Jun 2023 03:37

Instrument :

MSVOA_W

ClientSampleId :

A46K5MSD

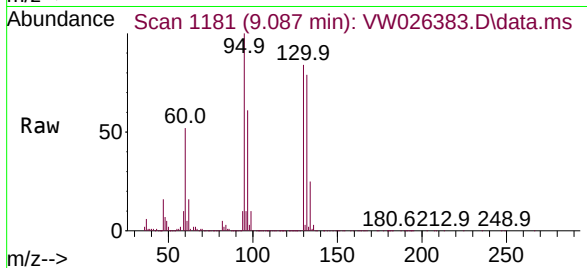

Tgt Ion: 95 Resp: 25966

Ion Ratio Lower Upper

95 100

97 61.0 44.5 82.7

132 79.0 63.3 117.5

130 83.7 64.9 120.5

Manual Integrations

APPROVED

Reviewed By :Semsettin




Yesilyurt

06/28/2023

Supervised By :Mahesh

Dadoda

06/29/2023

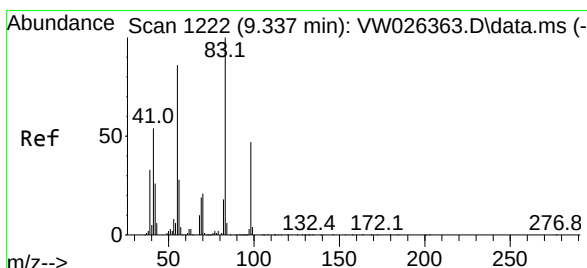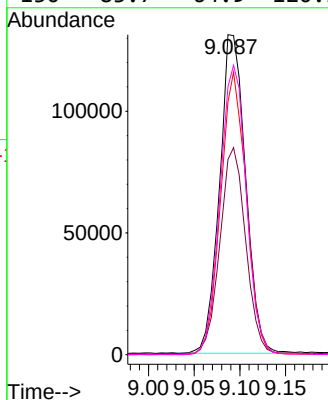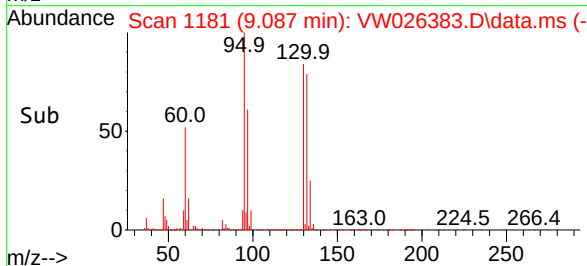

#35

Methylcyclohexane

Concen: 12.412 ug/L

RT: 9.337 min Scan# 1222

Delta R.T. 0.000 min

Lab File: VW026383.D

Acq: 28 Jun 2023 03:37




Tgt Ion: 83 Resp: 221746


Ion Ratio Lower Upper

83 100

55 86.0 68.8 103.2


98 47.8 37.8 56.6

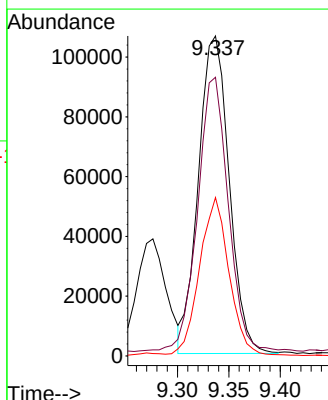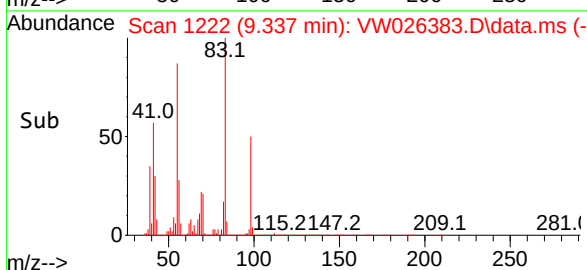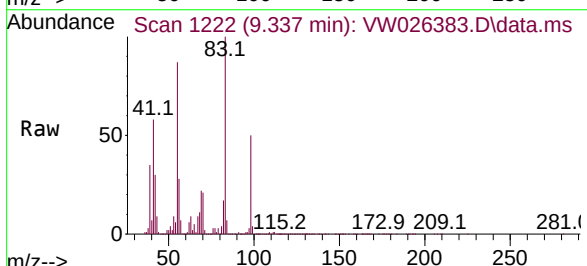

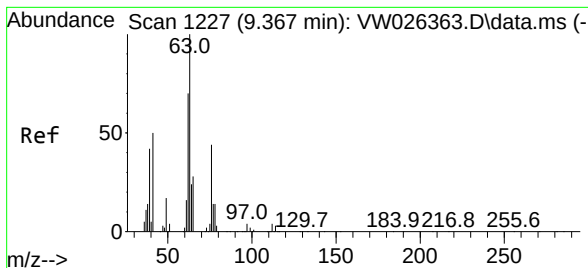

#37
1,2-Dichloropropane
Concen: 25.559 ug/L
RT: 9.367 min Scan# 112
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37



Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD

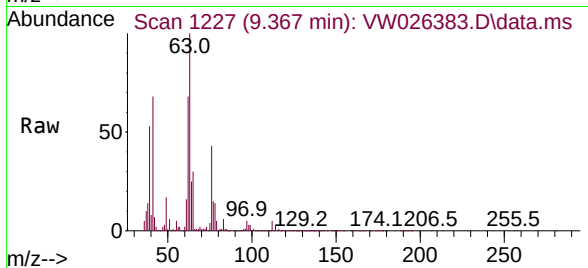

Tgt Ion: 63 Resp: 290562
Ion Ratio Lower Upper
63 100
112 4.1 3.0 4.6


Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt

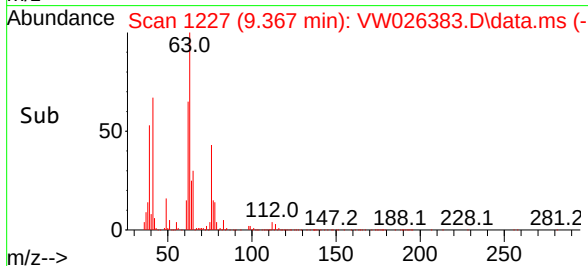


06/28/2023
Supervised By :Mahesh
Dadoda



06/29/2023

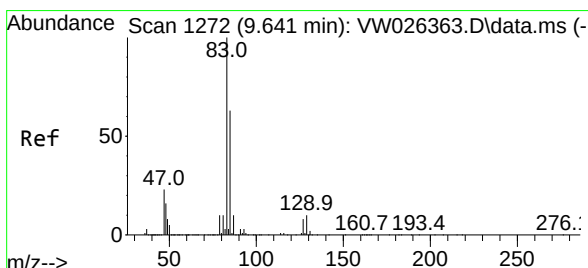


#38
Bromodichloromethane
Concen: 24.827 ug/L
RT: 9.642 min Scan# 1272
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

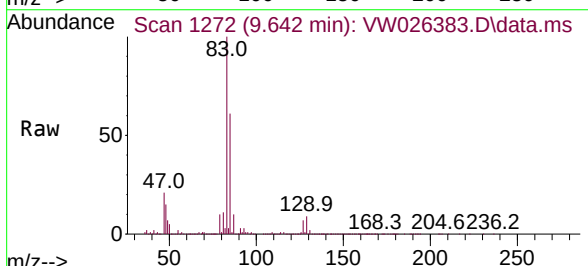


Tgt Ion: 83 Resp: 324127
Ion Ratio Lower Upper
83 100
85 61.2 44.9 83.5
127 7.4 6.2 9.2

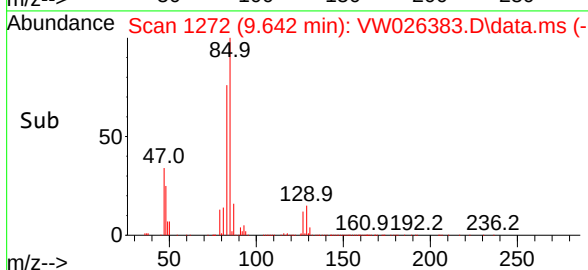



#39
cis-1,3-Dichloropropene
Concen: 22.035 ug/L
RT: 10.075 min Scan# 1343
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 75 Resp: 358904
Ion Ratio Lower Upper
75 100
77 31.0 22.8 42.4

Manual Integrations
APPROVED


Reviewed By :Semsettin
Yesilyurt

06/28/2023
Supervised By :Mahesh
Dadoda



06/29/2023

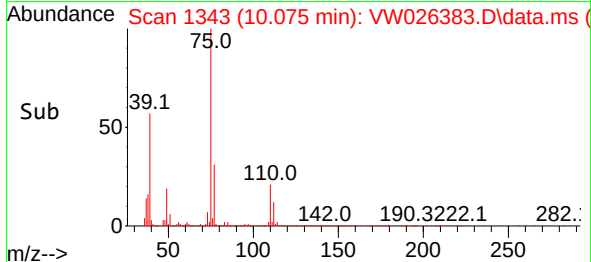


#40
4-Methyl-2-pentanone
Concen: 57.855 ug/L
RT: 10.209 min Scan# 1365
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37




Tgt Ion: 43 Resp: 424534
Ion Ratio Lower Upper
43 100
58 36.6 28.6 42.8
100 13.0 9.9 14.9

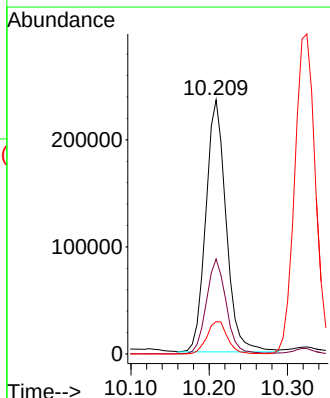



#42
Toluene
Concen: 24.571 ug/L
RT: 10.386 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 91 Resp: 1002948
Ion Ratio Lower Upper
91 100
92 59.9 40.3 74.8

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#44
trans-1,3-Dichloropropene
Concen: 20.571 ug/L
RT: 10.605 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 75 Resp: 282823
Ion Ratio Lower Upper
75 100
77 31.5 21.6 40.2

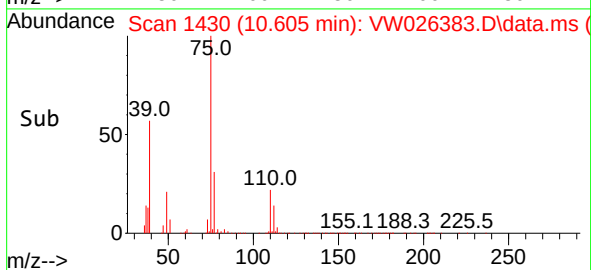



#45
1,1,2-Trichloroethane
Concen: 25.438 ug/L
RT: 10.788 min Scan# 1460
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 97 Resp: 193620
Ion Ratio Lower Upper
97 100
99 58.4 42.4 78.6
83 85.6 60.8 113.0
85 55.5 39.1 72.7

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

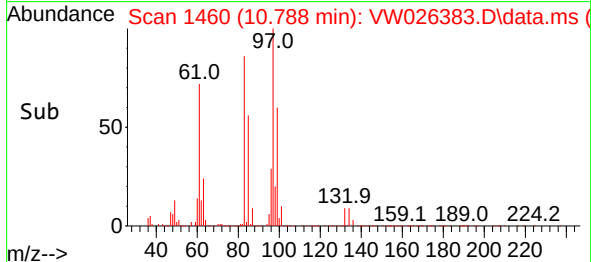

#46
Tetrachloroethene
Concen: 16.777 ug/L
RT: 10.861 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:164 Resp: 123140
Ion Ratio Lower Upper
164 100
129 104.3 73.8 137.0
131 102.2 69.0 128.2
166 115.6 91.1 169.3

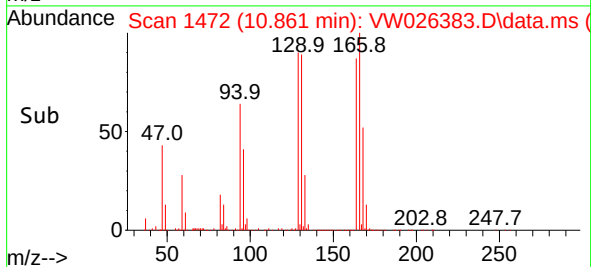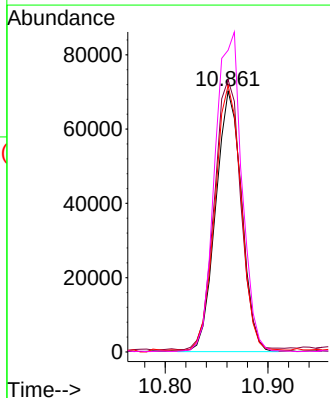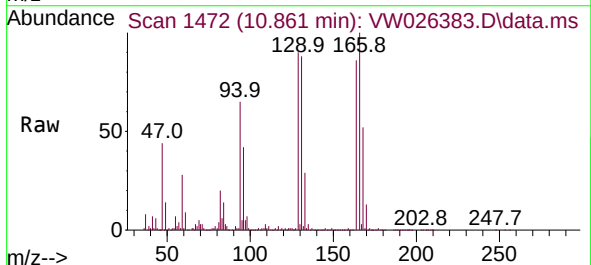



#48
2-Hexanone
Concen: 53.901 ug/L
RT: 10.965 min Scan# 1489
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 43 Resp: 279072
Ion Ratio Lower Upper
43 100
58 53.6 40.1 60.1
57 17.6 13.4 20.0
100 10.7 8.2 12.2

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#49
Dibromochloromethane
Concen: 23.021 ug/L
RT: 11.129 min Scan# 1516
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:129 Resp: 179424
Ion Ratio Lower Upper
129 100
127 80.3 54.4 101.0

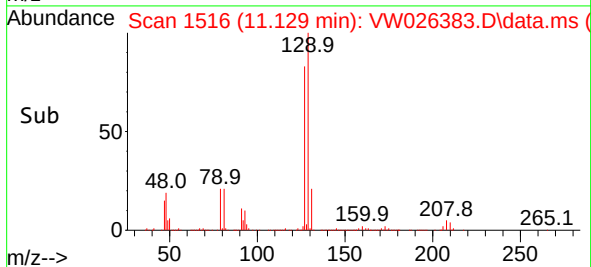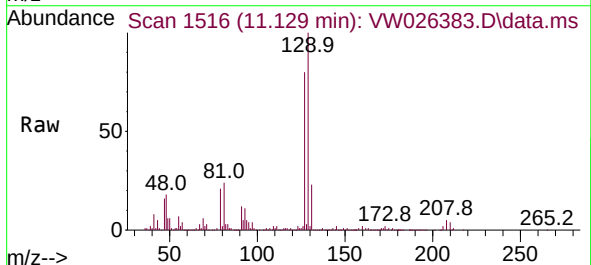



#50
1,2-Dibromoethane
Concen: 24.607 ug/L
RT: 11.233 min Scan# 1533
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD

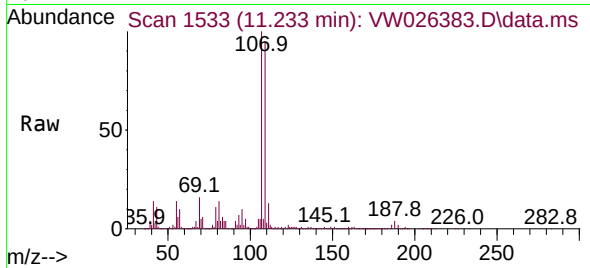



Tgt Ion:107 Resp: 171958
Ion Ratio Lower Upper
107 100
109 95.4 67.1 124.5
188 3.5 2.6 3.8

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

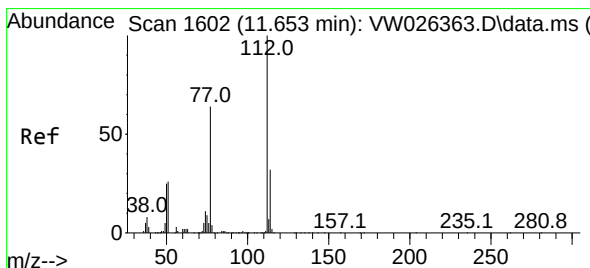

#51
Chlorobenzene
Concen: 20.028 ug/L
RT: 11.654 min Scan# 1602
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Tgt Ion:112 Resp: 521475
Ion Ratio Lower Upper
112 100
114 32.3 23.0 42.8
77 64.9 53.2 79.8

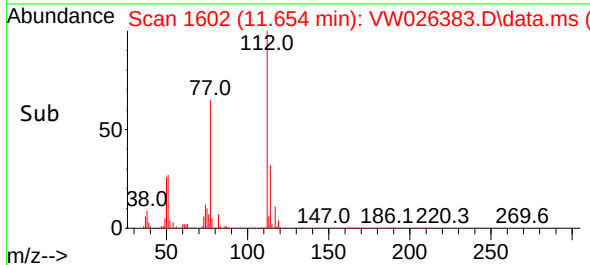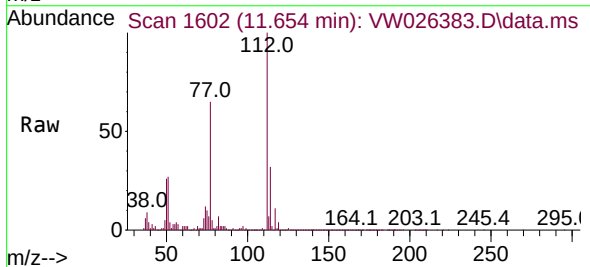



#52
Ethylbenzene
Concen: 19.351 ug/L
RT: 11.727 min Scan# 1614
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD





Tgt Ion: 91 Resp: 89004
Ion Ratio Lower Upper
91 100
106 29.7 19.9 36.9

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

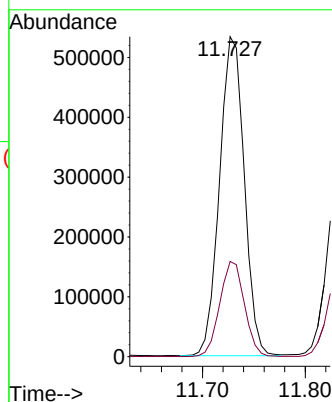

#53
m,p-Xylene
Concen: 18.586 ug/L
RT: 11.837 min Scan# 1632
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:106 Resp: 311770
Ion Ratio Lower Upper
106 100
91 220.7 152.1 282.5

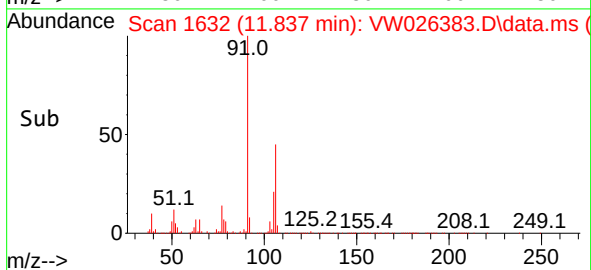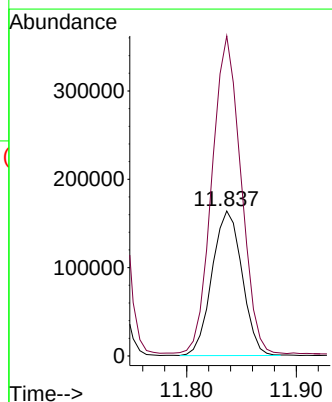



#54
o-Xylene
Concen: 18.971 ug/L
RT: 12.166 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion:106 Resp: 299624
Ion Ratio Lower Upper
106 100
91 223.1 161.5 299.9

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#55
Styrene
Concen: 16.677 ug/L
RT: 12.178 min Scan# 1688
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:104 Resp: 459410
Ion Ratio Lower Upper
104 100
78 48.6 33.3 61.9

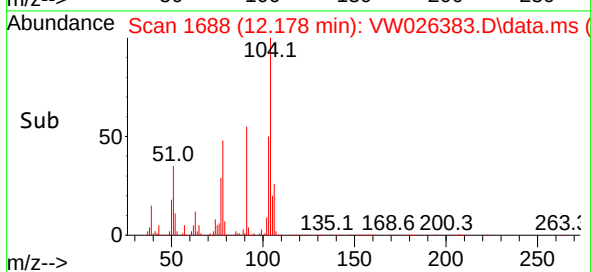



#57
1,1,2,2-Tetrachloroethane
Concen: 19.978 ug/L
RT: 12.714 min Scan# 1776
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion: 83 Resp: 190080
Ion Ratio Lower Upper
83 100
85 65.2 43.7 81.1
131 9.4 7.4 11.0

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#59
Bromoform
Concen: 33.722 ug/L
RT: 12.349 min Scan# 1716
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:173 Resp: 85542
Ion Ratio Lower Upper
173 100
175 51.7 39.7 59.5
254 9.1 7.1 10.7

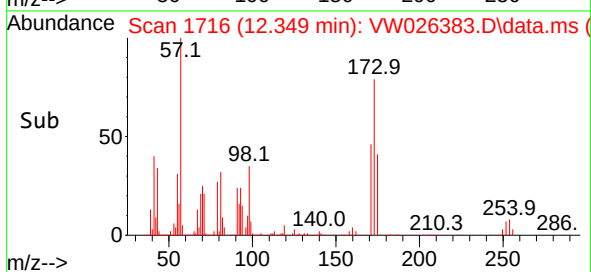



#60
Isopropylbenzene
Concen: 25.387 ug/L
RT: 12.458 min Scan# 1734
Delta R.T. -0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion:105 Resp: 639810
Ion Ratio Lower Upper
105 100
120 25.6 20.4 30.6
77 17.8 13.6 20.4

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023



#61
1,2,3-Trichloropropane
Concen: 39.171 ug/L
RT: 12.763 min Scan# 1784
Delta R.T. -0.006 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion: 75 Resp: 159665
Ion Ratio Lower Upper
75 100
77 34.2 25.9 38.9
110 40.0 29.4 44.0



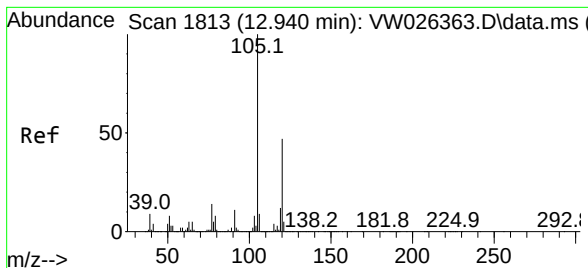

#62
1,3,5-Trimethylbenzene
Concen: 22.288 ug/L
RT: 12.940 min Scan# 1813
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD

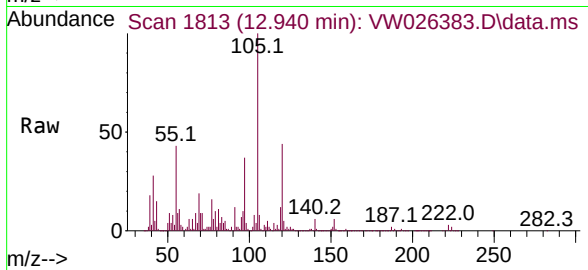




Tgt Ion:105 Resp: 43542
Ion Ratio Lower Upper
105 100
120 46.7 38.1 57.1

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

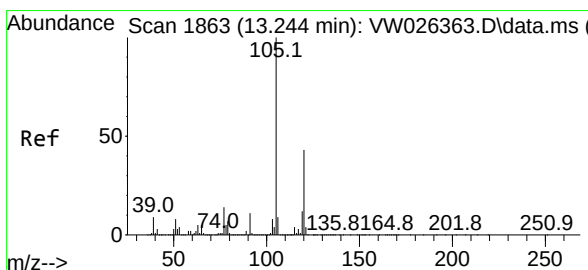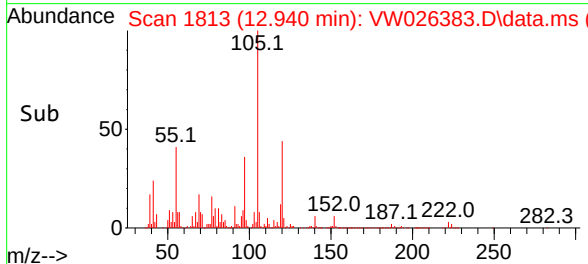

#63
1,2,4-Trimethylbenzene
Concen: 22.869 ug/L
RT: 13.245 min Scan# 1863
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:105 Resp: 430905
Ion Ratio Lower Upper
105 100
120 44.1 35.0 52.6

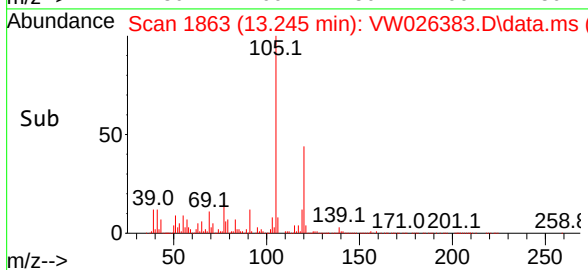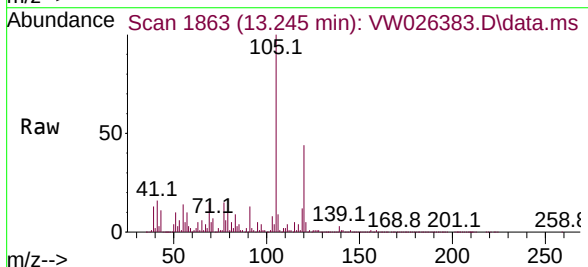



#64
1,3-Dichlorobenzene
Concen: 18.746 ug/L
RT: 13.495 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion:146 Resp: 202352
Ion Ratio Lower Upper
146 100
111 55.0 30.8 57.2
148 61.7 43.3 80.3

Manual Integrations
APPROVED


Reviewed By :Semsettin
Yesilyurt

06/28/2023
Supervised By :Mahesh
Dadoda



06/29/2023




#65
1,4-Dichlorobenzene
Concen: 19.735 ug/L
RT: 13.574 min Scan# 1917
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37



Tgt Ion:146 Resp: 213187
Ion Ratio Lower Upper
146 100
111 70.6 30.0 55.8#
148 63.3 43.7 81.1

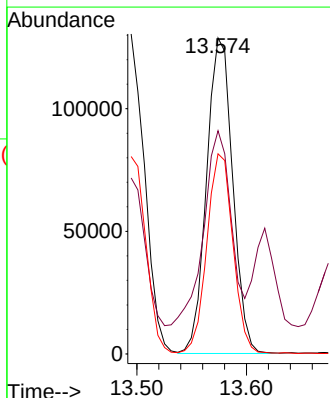



#67

1,2-Dichlorobenzene

Concen: 19.151 ug/L

RT: 13.867 min Scan# 1965

Delta R.T. 0.000 min

Lab File: VW026383.D


Acq: 28 Jun 2023 03:37

Instrument :

MSVOA_W

ClientSampleId :

A46K5MSD



Tgt Ion:	146	Resp:	18412
Ion Ratio	Lower	Upper	
146	100		
111	71.4	36.0	54.0
148	68.1	47.8	71.8




Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt

06/28/2023

Supervised By :Mahesh
Dadoda

06/29/2023



#68

1,2-Dibromo-3-chloropropane

Concen: 30.722 ug/L




RT: 14.482 min Scan# 2066


Delta R.T. 0.000 min

Lab File: VW026383.D

Acq: 28 Jun 2023 03:37


Tgt Ion:	75	Resp:	28862
Ion Ratio	Lower	Upper	
75	100		
155	67.9	57.5	86.3
157	93.8	73.4	110.0

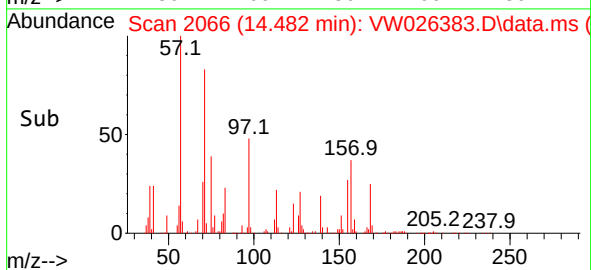



#69
1,3,5-Trichlorobenzene
Concen: 9.542 ug/L
RT: 14.629 min Scan# 2090
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion:180 Resp: 66189
Ion Ratio Lower Upper
180 100
182 93.3 74.2 111.4
184 28.9 23.8 35.6
145 32.5 25.4 38.0

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt




06/28/2023
Supervised By :Mahesh
Dadoda


06/29/2023

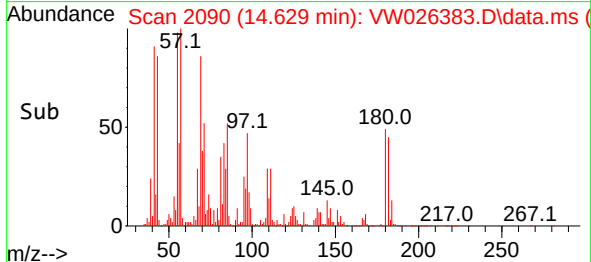

#70
1,2,4-trichlorobenzene
Concen: 10.021 ug/L
RT: 15.129 min Scan# 2172
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37


Tgt Ion:180 Resp: 56882
Ion Ratio Lower Upper
180 100
182 102.9 75.6 113.4
145 93.3 24.7 37.1#

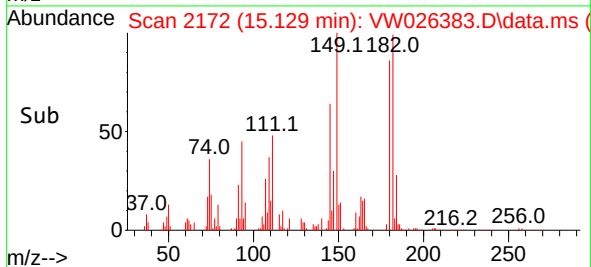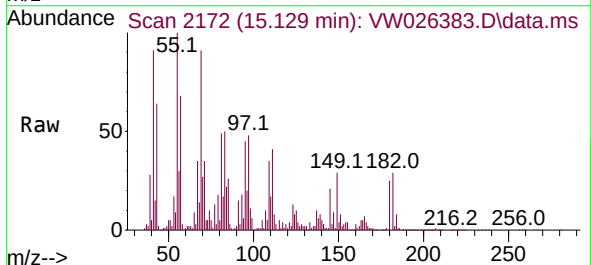



#71
Naphthalene
Concen: 17.763 ug/L
RT: 15.360 min Scan# 2210
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Instrument :
MSVOA_W
ClientSampleId :
A46K5MSD






Tgt Ion:128 Resp: 20269
Ion Ratio Lower Upper
128 100
127 23.7 10.9 16.3#
129 10.7 8.9 13.3#

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt

06/28/2023
Supervised By :Mahesh
Dadoda

06/29/2023



#72
1,2,3-Trichlorobenzene
Concen: 14.099 ug/L m
RT: 15.549 min Scan# 2241
Delta R.T. 0.000 min
Lab File: VW026383.D
Acq: 28 Jun 2023 03:37

Tgt Ion:180 Resp: 74721
Ion Ratio Lower Upper
180 100
182 6.1 75.0 112.6#
145 2.4 28.5 42.7#

