

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062724\
 Data File : VW029377.D
 Acq On : 27 Jun 2024 13:08
 Operator : SY/MD
 Sample : VIBLK483
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK483

Quant Time: Jun 28 00:54:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 27 05:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	271795	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	261074	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114428	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	79099	21.026	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.120%
7) Chloroethane-d5	2.905	69	62695	19.735	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.920%
11) 1,1-Dichloroethene-d2	4.027	65	38170	21.014	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.040%
21) 2-Butanone-d5	7.075	46	52399	46.556	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.120%
24) Chloroform-d	7.648	84	173953	21.455	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.840%
26) 1,2-Dichloroethane-d4	8.307	65	104340	22.414	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.640%
32) Benzene-d6	8.276	84	341506	21.536	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.160%
36) 1,2-Dichloropropane-d6	9.276	67	109567	21.736	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.960%
41) Toluene-d8	10.325	98	296086	21.104	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.400%
43) trans-1,3-Dichloroprop...	10.575	79	42406	20.876	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.520%
47) 2-Hexanone-d5	10.922	63	35104	44.424	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.840%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	87652	21.848	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	101319	25.509	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.040%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	22145	4.634	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062724\
Data File : VW029377.D
Acq On : 27 Jun 2024 13:08
Operator : SY/MD
Sample : VIBLK483
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK483

Quant Time: Jun 28 00:54:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 27 05:32:27 2024
Response via : Initial Calibration

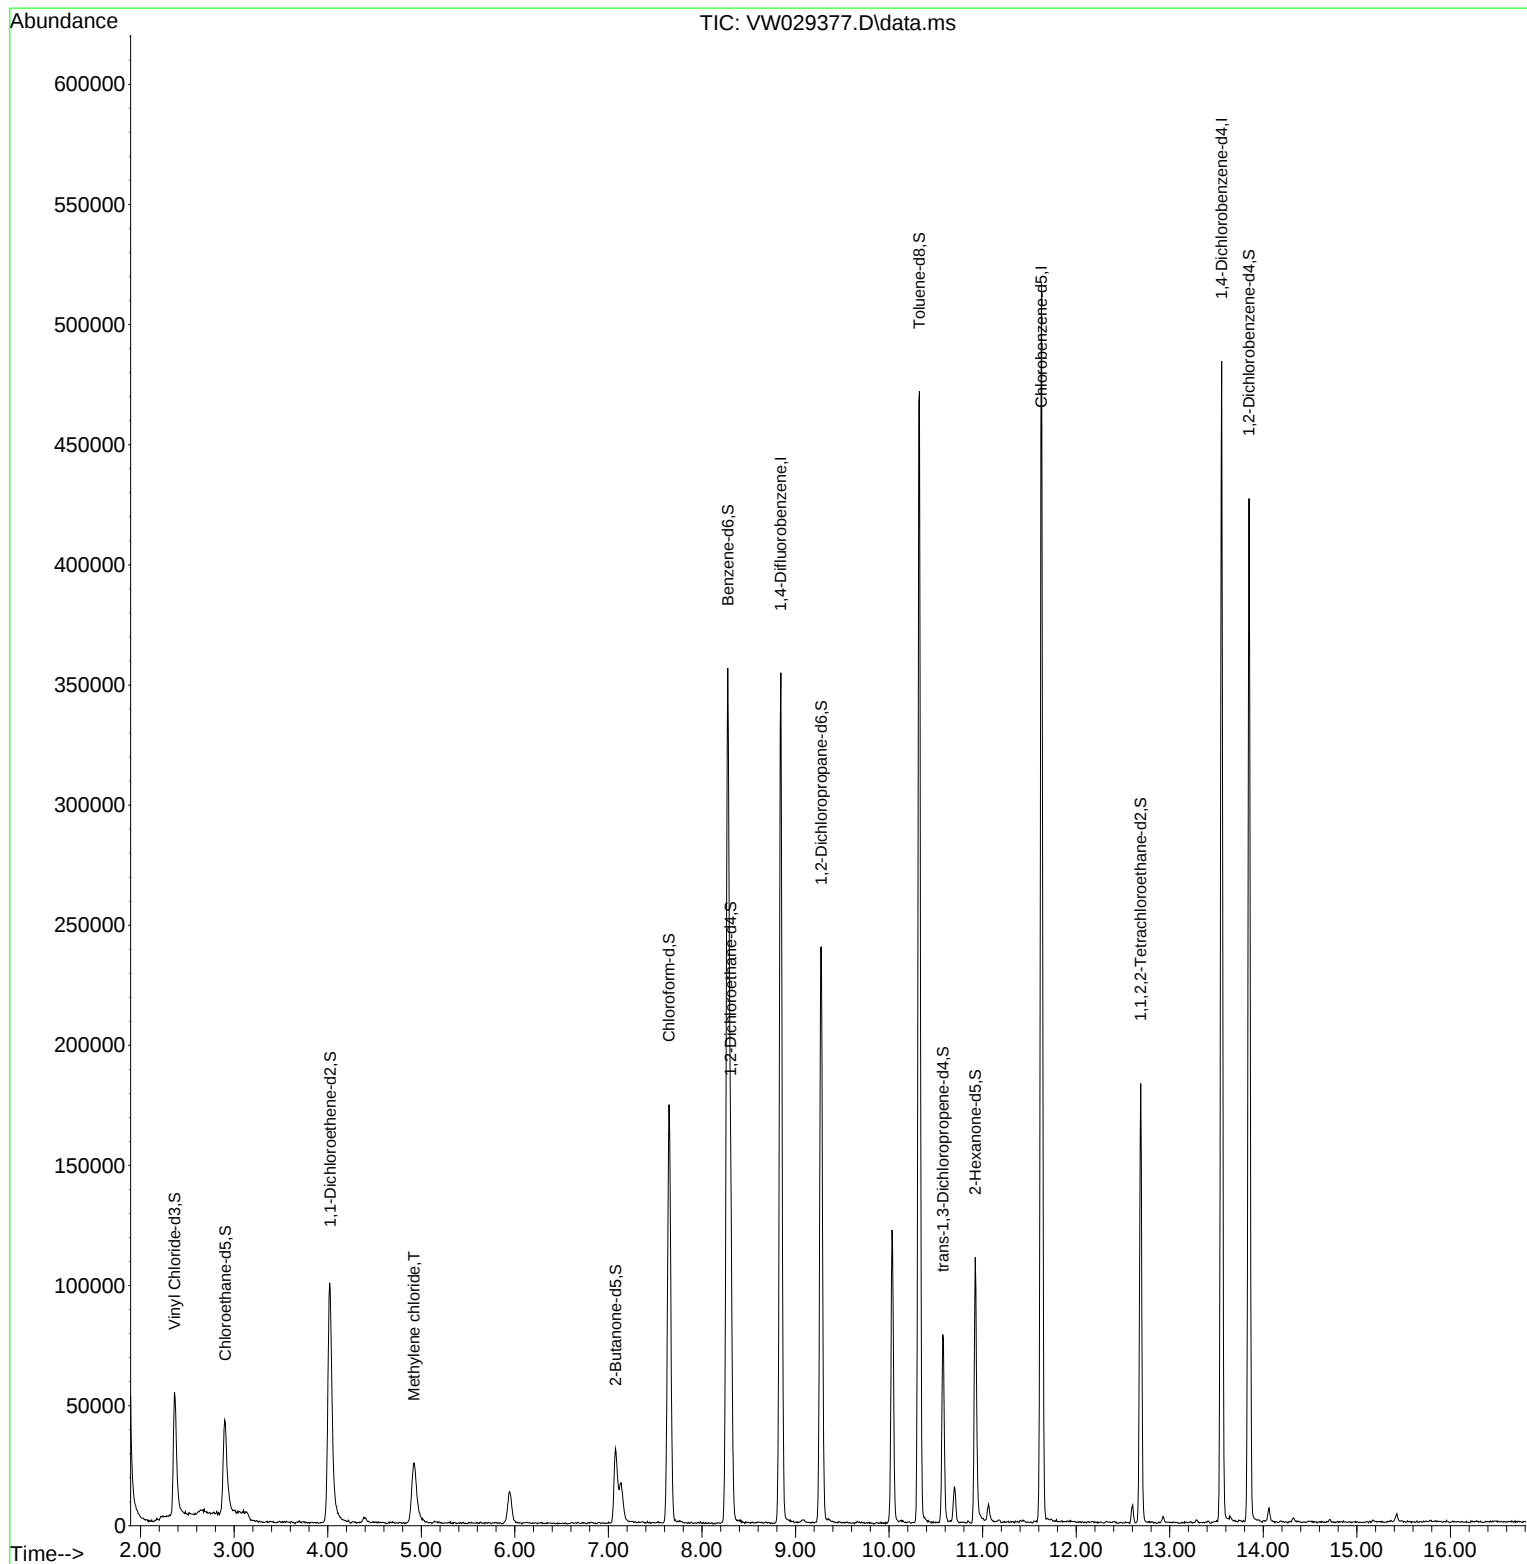

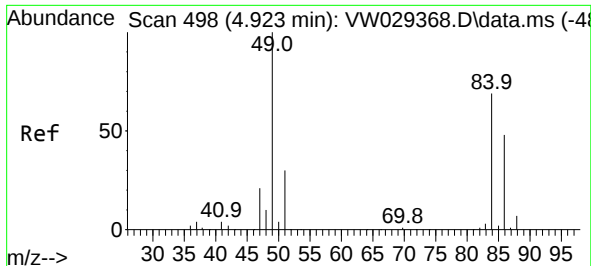

#16
Methylene chloride
Concen: 4.634 ug/L
RT: 4.923 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW029377.D
Acq: 27 Jun 2024 13:08

Instrument :
MSVOA_W
ClientSampleId :
VIBLK483

Tgt Ion: 84 Resp: 22145

Ion	Ratio	Lower	Upper
84	100		
86	64.3	41.4	77.0
49	132.4	95.7	177.7

