

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
 Data File : VW023531.D
 Acq On : 28 Jun 2022 14:15
 Operator : SY/VA
 Sample : N3506-01
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE9

Quant Time: Jun 29 02:16:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 29 02:13:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	433705	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	404522	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	194434	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	104092	18.644	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.560%
7) Chloroethane-d5	3.043	69	469	0.111	ug/L	0.16
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.440%#
11) 1,1-Dichloroethene-d2	4.013	63	112212	12.812	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.240%
21) 2-Butanone-d5	7.079	46	64861	48.812	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.620%
24) Chloroform-d	7.652	84	220817	19.829	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.320%
26) 1,2-Dichloroethane-d4	8.305	65	120545	20.563	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.240%
32) Benzene-d6	8.274	84	393557	19.679	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.720%
36) 1,2-Dichloropropane-d6	9.274	67	124616	20.899	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.600%
41) Toluene-d8	10.323	98	367921	18.821	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.280%
43) trans-1,3-Dichloroprop...	10.579	79	52131	19.314	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.240%
47) 2-Hexanone-d5	10.926	63	48410	50.143	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.280%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	121394	22.104	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	134317	19.885	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	4701	0.555	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
Data File : VW023531.D
Acq On : 28 Jun 2022 14:15
Operator : SY/VA
Sample : N3506-01
Misc : 4.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AE9

Quant Time: Jun 29 02:16:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 29 02:13:18 2022
Response via : Initial Calibration

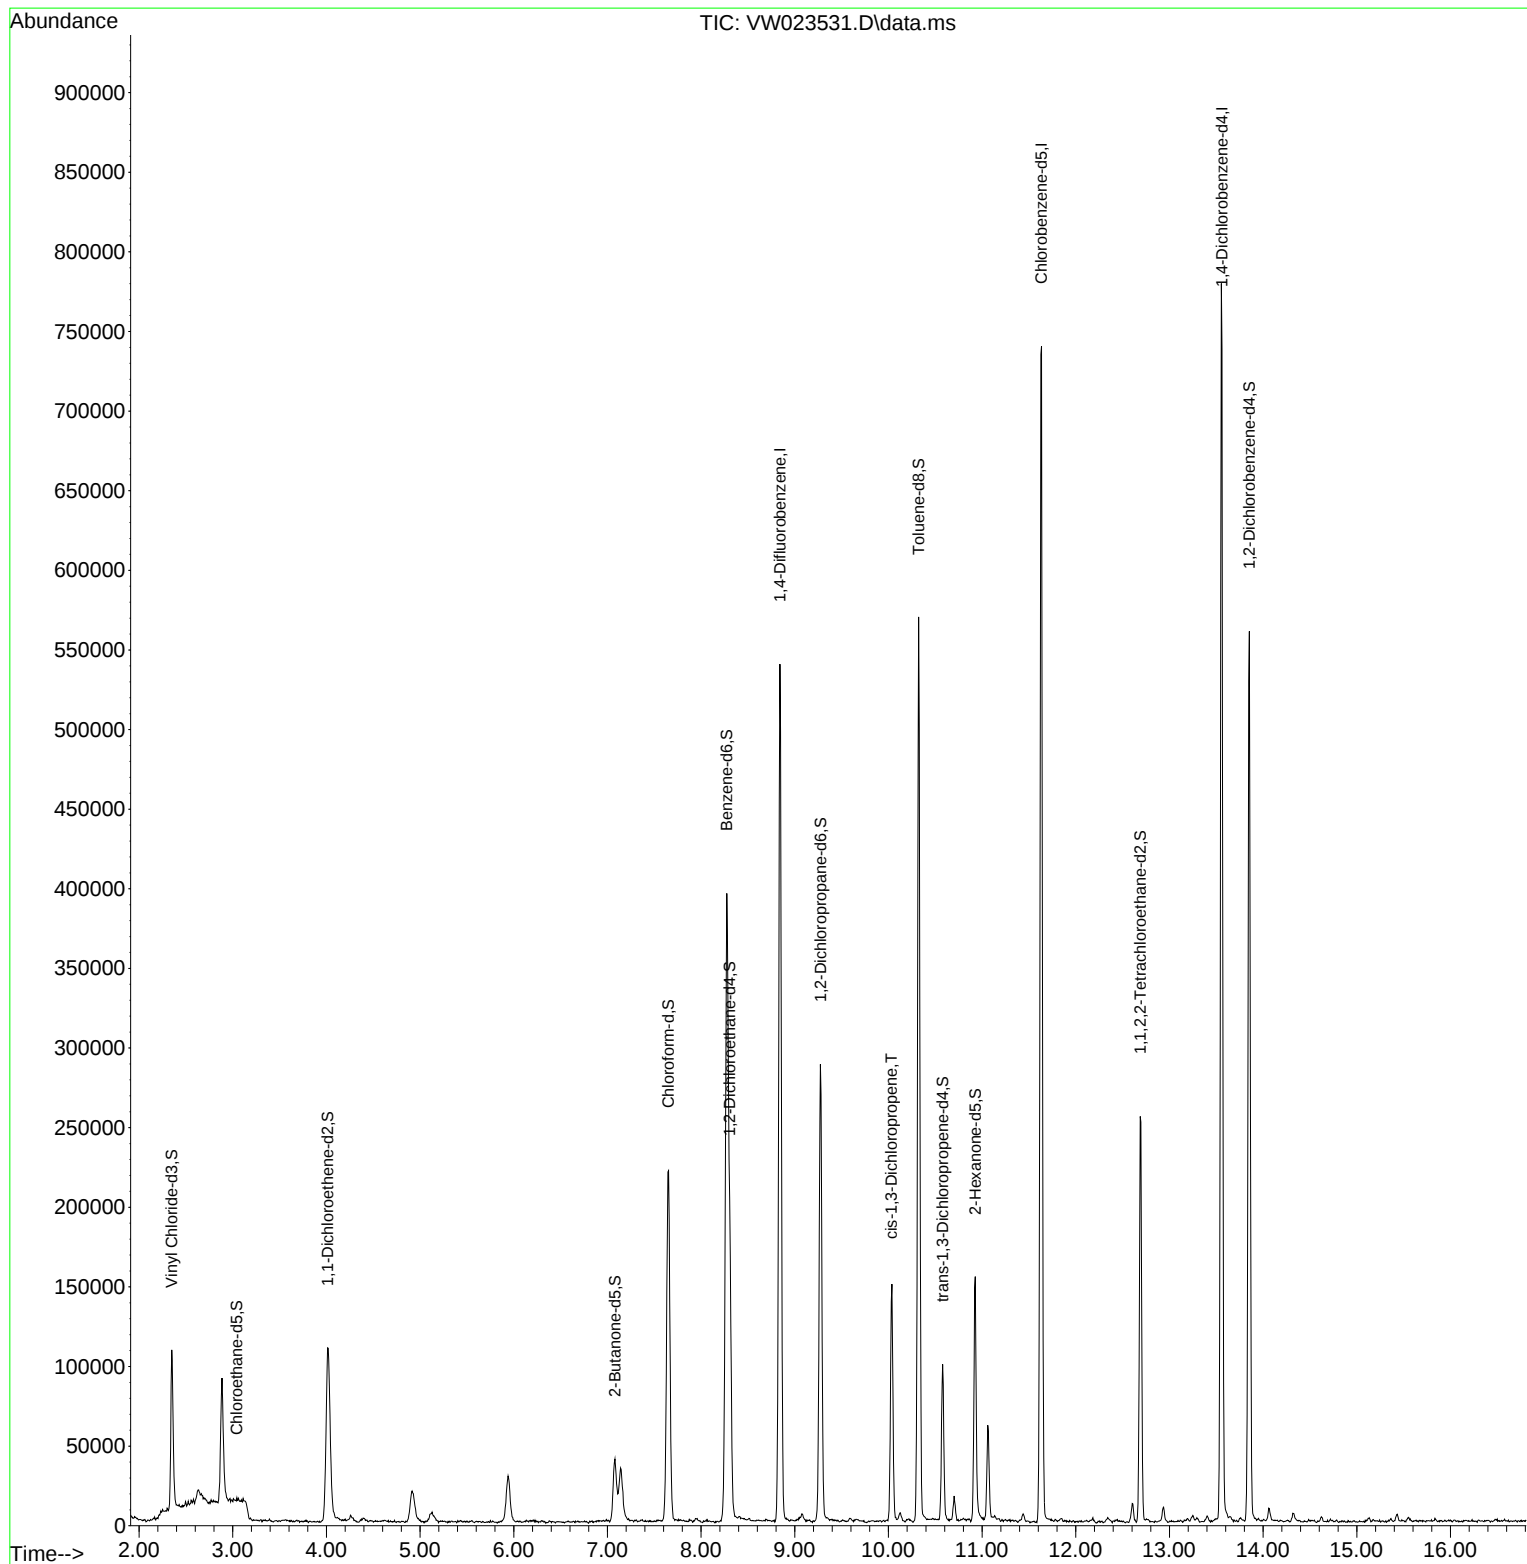

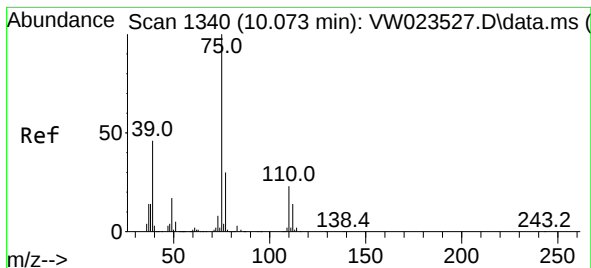

#39
 cis-1,3-Dichloropropene
 Concen: 0.555 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW023531.D
 Acq: 28 Jun 2022 14:15

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE9

Tgt Ion: 75 Resp: 4701
 Ion Ratio Lower Upper
 75 100
 77 38.0 23.0 42.8

