




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
 Data File : VW023531.D
 Acq On : 28 Jun 2022 14:15
 Operator : SY/VA
 Sample : N3506-01
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Quant Time: Jun 29 02:16:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 29 02:13:18 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

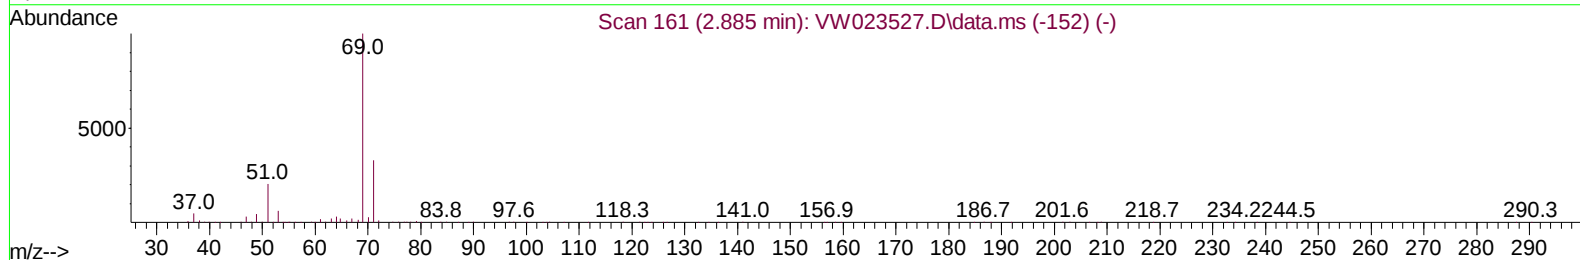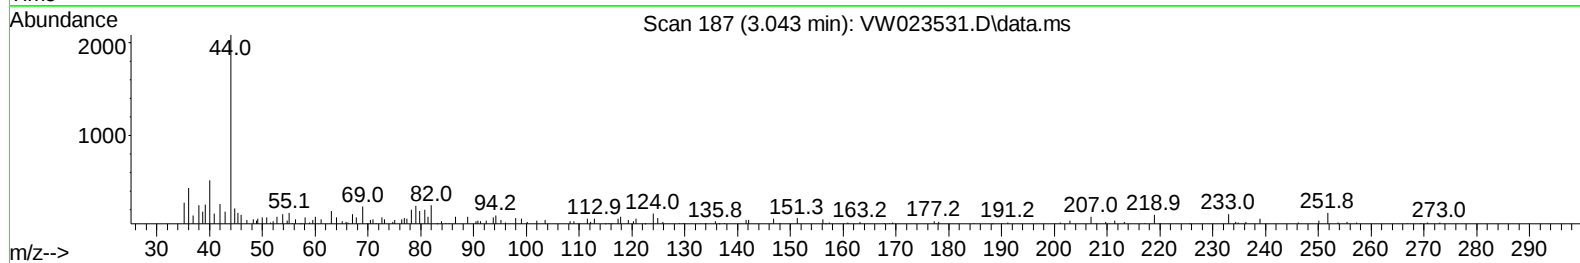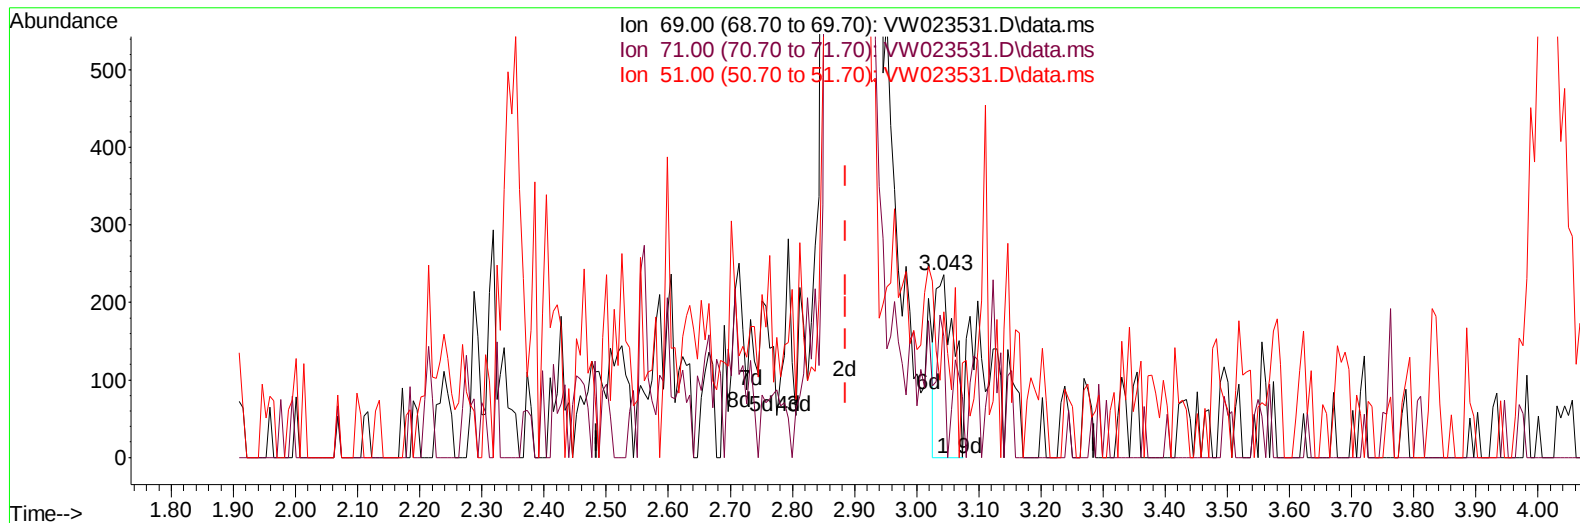

TIC: VW023531.D\data.ms

(7) Chloroethane-d5 (S)

3.043min (+ 0.158) 0.11 ug/L

response 469

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	34.33
51.00	28.80	27.51
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
 Data File : VW023531.D
 Acq On : 28 Jun 2022 14:15
 Operator : SY/VA
 Sample : N3506-01
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Quant Time: Jun 29 02:16:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 29 02:13:18 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

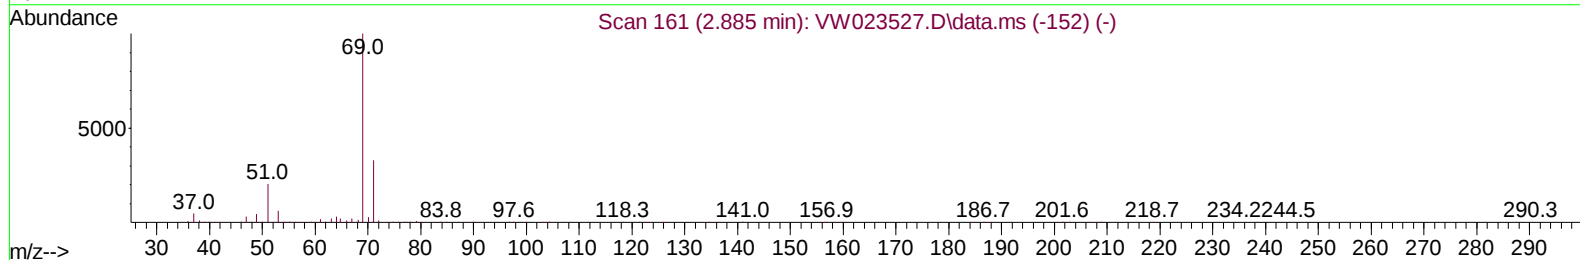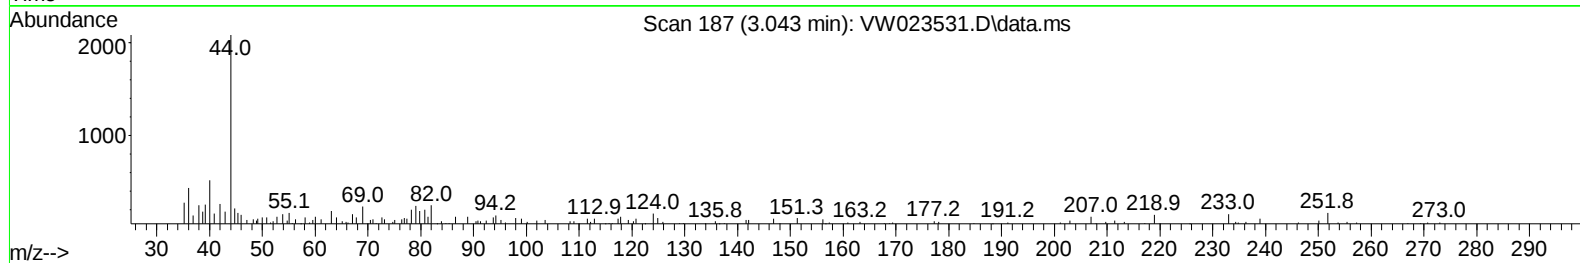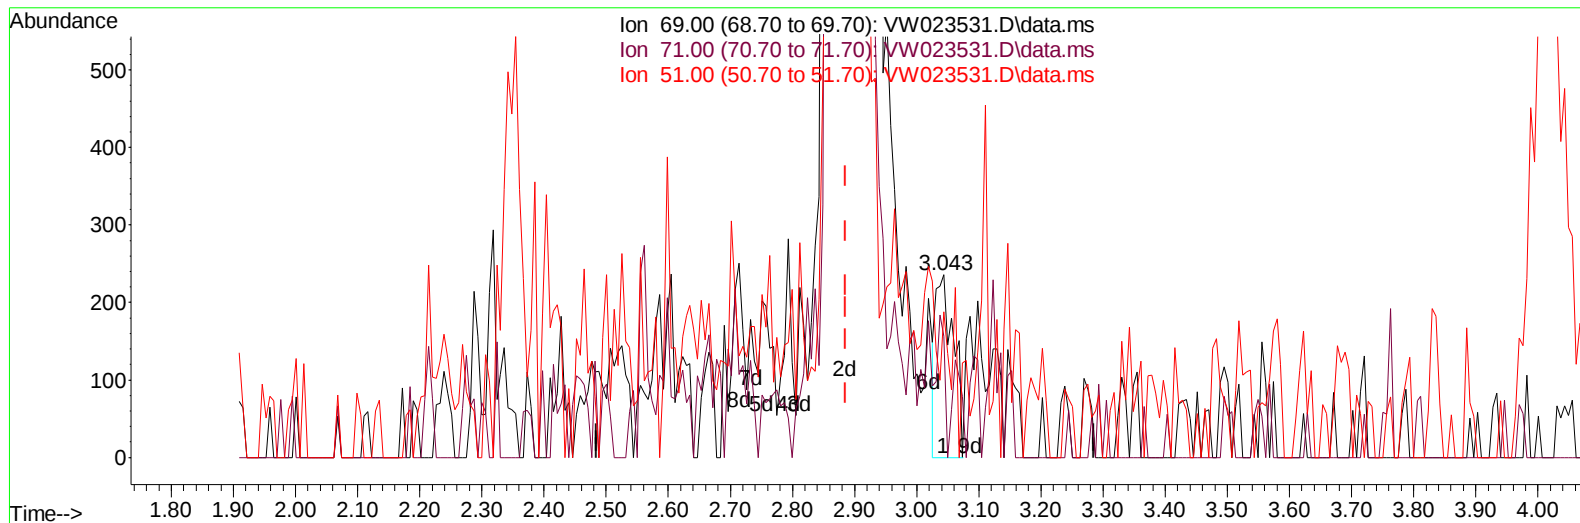

TIC: VW023531.D\data.ms

(7) Chloroethane-d5 (S)

3.043min (+ 0.158) 0.11 ug/L

response 469

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	34.33
51.00	28.80	27.51
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
 Data File : VW023531.D
 Acq On : 28 Jun 2022 14:15
 Operator : SY/VA
 Sample : N3506-01
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

Quant Time: Jun 29 02:16:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 29 02:13:18 2022
 Response via : Initial Calibration

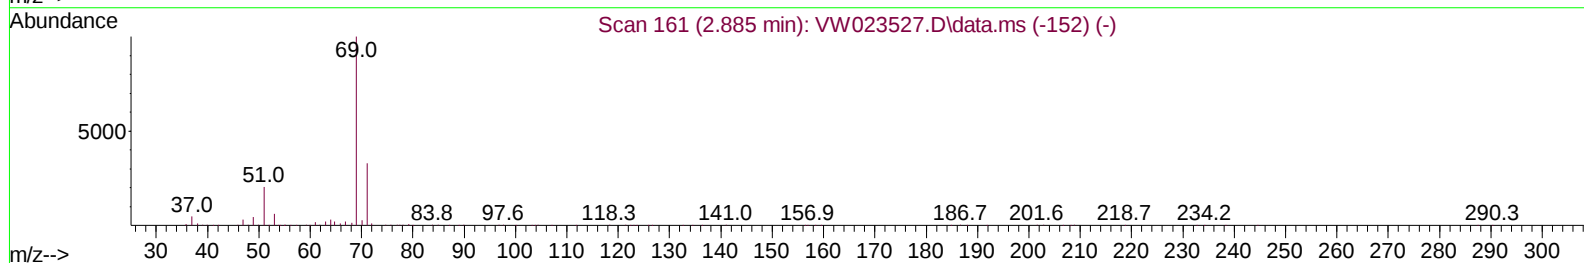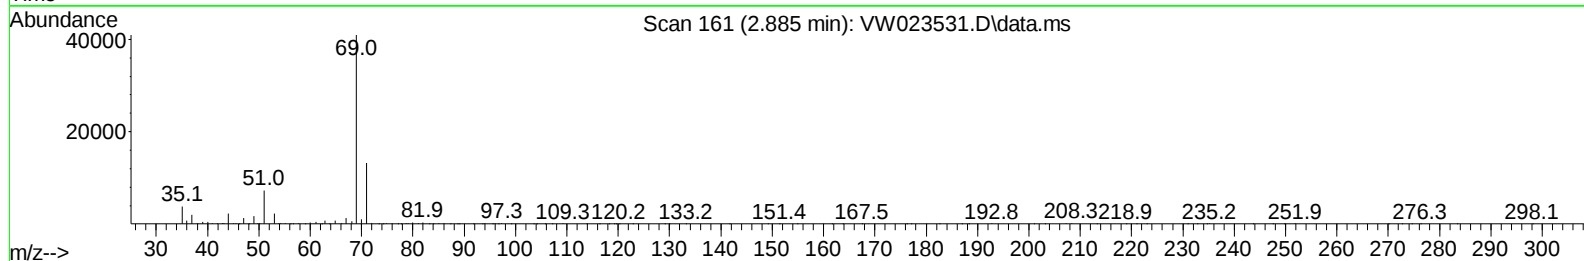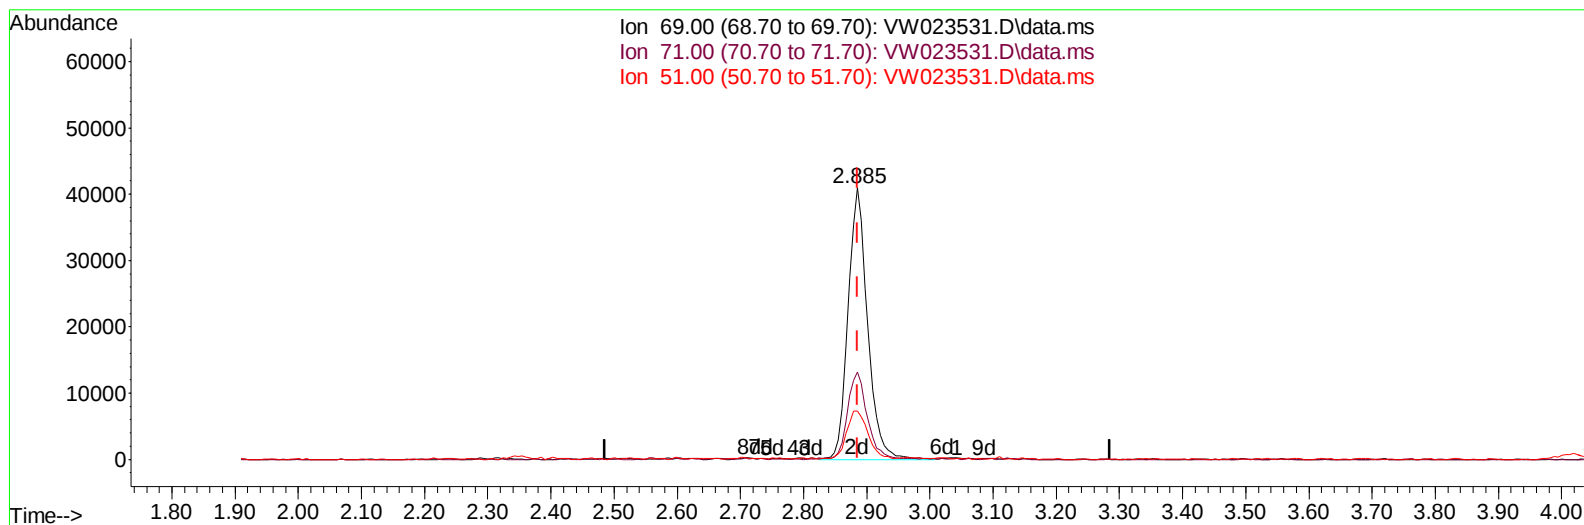

TIC: VW023531.D\data.ms

(7) Chloroethane-d5 (S)

2.885min (-0.000) 20.87 ug/L m

response 88048

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	0.18#
51.00	28.80	0.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
 Data File : VW023531.D
 Acq On : 28 Jun 2022 14:15
 Operator : SY/VA
 Sample : N3506-01
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

Quant Time: Jun 29 02:16:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 29 02:13:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	433705	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	404522	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	194434	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	104092	18.644	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.560%	
7) Chloroethane-d5	2.885	69	88048m	20.871	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.480%	
11) 1,1-Dichloroethene-d2	4.013	63	112212	12.812	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.240%	
21) 2-Butanone-d5	7.079	46	64861	48.812	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.620%	
24) Chloroform-d	7.652	84	220817	19.829	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	79.320%	
26) 1,2-Dichloroethane-d4	8.305	65	120545	20.563	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	82.240%	
32) Benzene-d6	8.274	84	393557	19.679	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	78.720%	
36) 1,2-Dichloropropane-d6	9.274	67	124616	20.899	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	83.600%	
41) Toluene-d8	10.323	98	367921	18.821	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.280%	
43) trans-1,3-Dichloroprop...	10.579	79	52131	19.314	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.240%	
47) 2-Hexanone-d5	10.926	63	48410	50.143	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.280%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	121394	22.104	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	88.400%	
66) 1,2-Dichlorobenzene-d4	13.853	152	134317	19.885	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	79.520%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062822\
Data File : VW023531.D
Acq On : 28 Jun 2022 14:15
Operator : SY/VA
Sample : N3506-01
Misc : 4.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AE9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

Quant Time: Jun 29 02:16:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062822SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 29 02:13:18 2022
Response via : Initial Calibration

