

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062824\
 Data File : VW029394.D
 Acq On : 28 Jun 2024 13:35
 Operator : SY/MD
 Sample : VW0628SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK515

Quant Time: Jun 29 02:10:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 29 02:05:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	246293	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	230573	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	102447	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	63894	18.743	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.960%
7) Chloroethane-d5	2.899	69	54988	19.101	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.400%
11) 1,1-Dichloroethene-d2	4.021	65	31692	19.254	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.000%
21) 2-Butanone-d5	7.075	46	46589	45.680	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.360%
24) Chloroform-d	7.648	84	162716	22.147	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	8.307	65	96365	22.845	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.360%
32) Benzene-d6	8.270	84	305679	21.826	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.320%
36) 1,2-Dichloropropane-d6	9.276	67	102269	22.972	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.880%
41) Toluene-d8	10.325	98	269249	21.730	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.920%
43) trans-1,3-Dichloroprop...	10.575	79	38062	21.216	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.880%
47) 2-Hexanone-d5	10.922	63	30684	43.967	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.940%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	78587	22.180	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	92204	25.929	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.720%
Target Compounds						
16) Methylene chloride	4.917	84	12765	2.948	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062824\
Data File : VW029394.D
Acq On : 28 Jun 2024 13:35
Operator : SY/MD
Sample : VW0628SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK515


Quant Time: Jun 29 02:10:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 29 02:05:50 2024
Response via : Initial Calibration

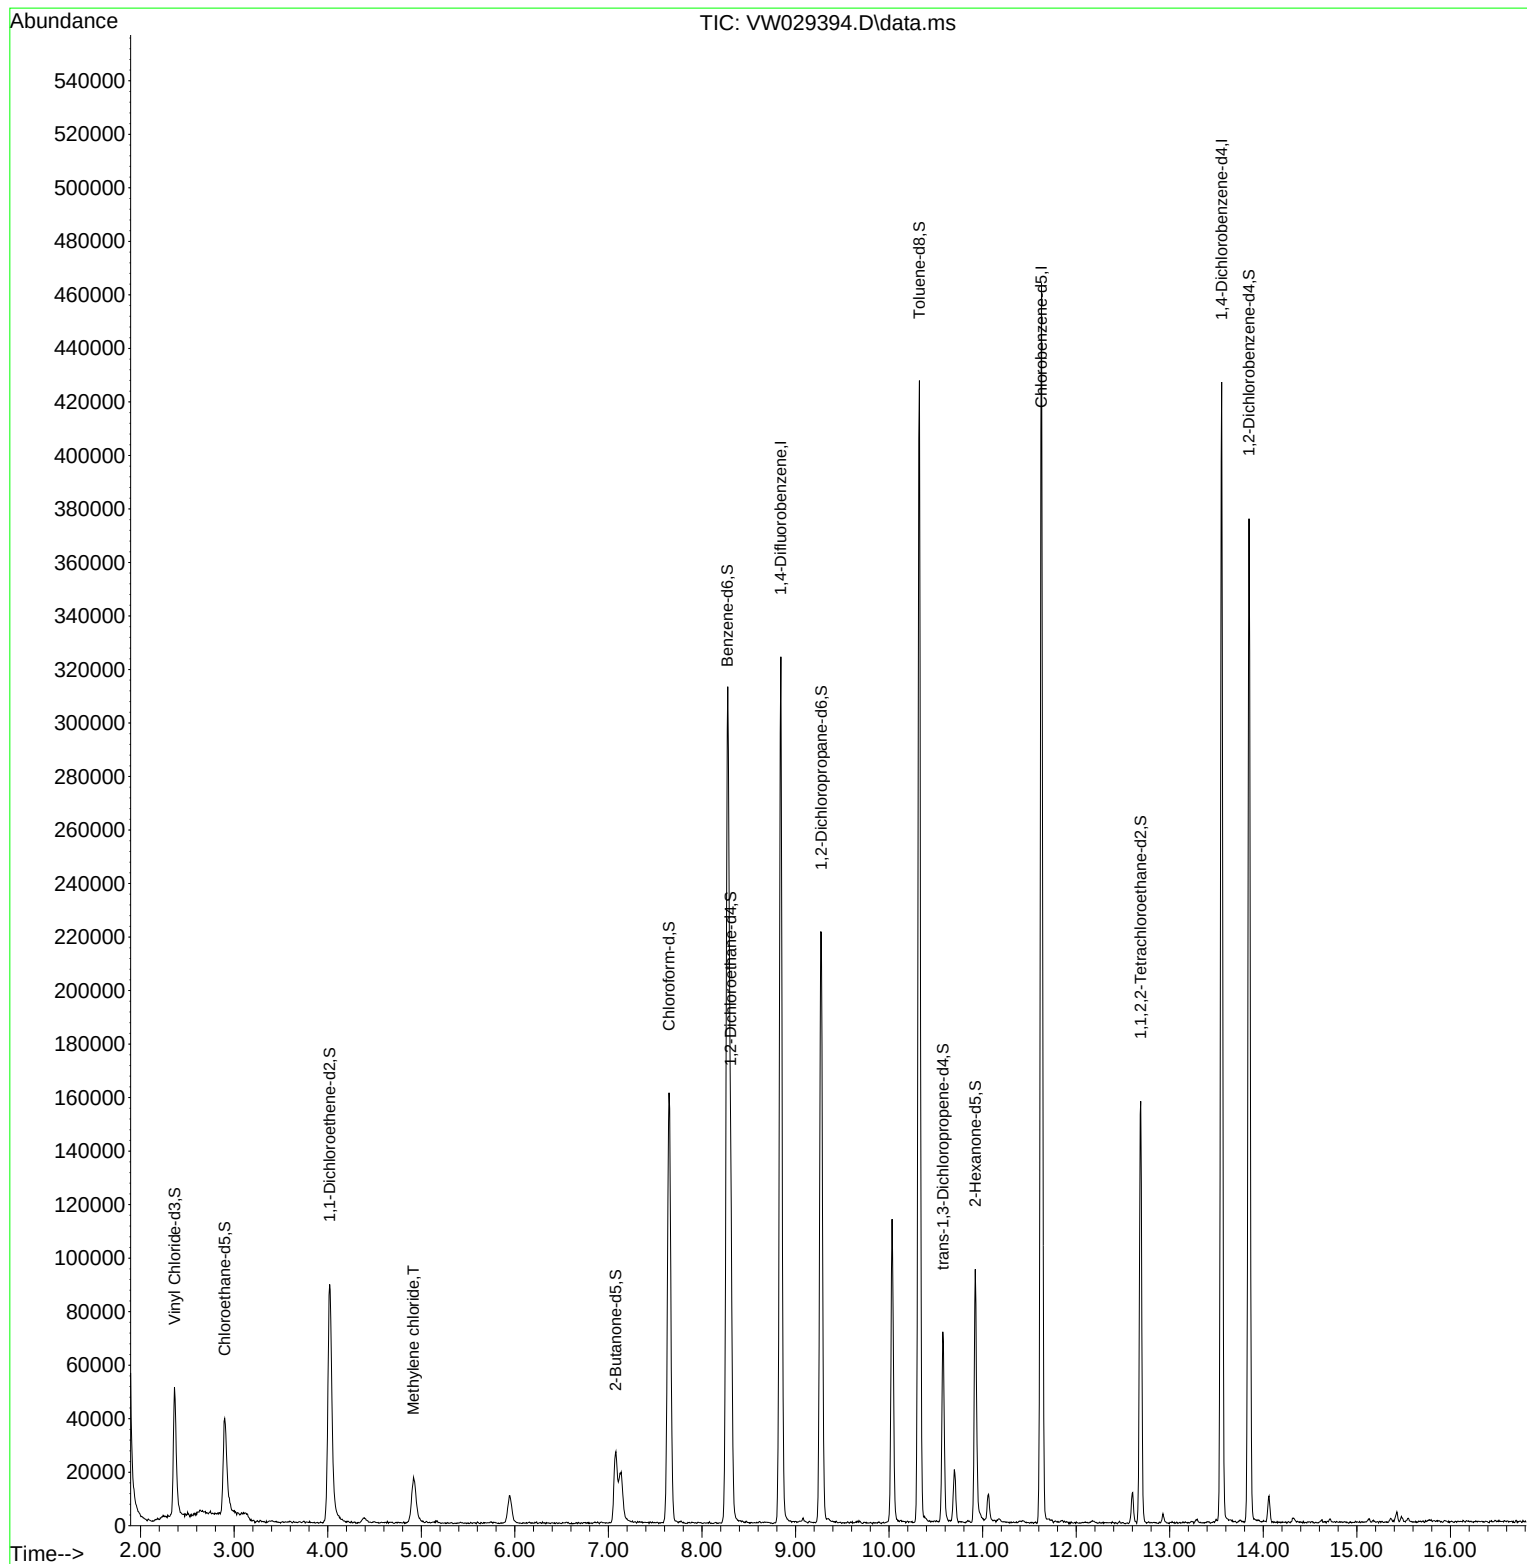

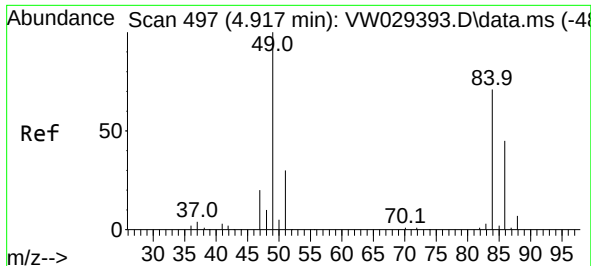

#16
Methylene chloride
Concen: 2.948 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW029394.D
Acq: 28 Jun 2024 13:35

Instrument :
MSVOA_W
ClientSampleId :
VBLK515

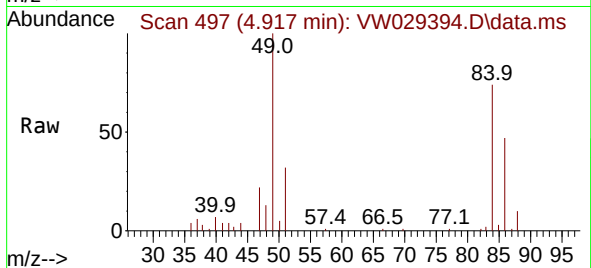

Tgt Ion:	84	Resp:	12765
Ion	Ratio	Lower	Upper
84	100		
86	64.4	41.4	77.0
49	135.7	95.7	177.7

