

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019351.D
 Acq On : 29 Jun 2021 10:57
 Operator : SY/VA
 Sample : M2808-22
 Misc : 4.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDx9

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:14 PM

Quant Time: Jun 30 02:50:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

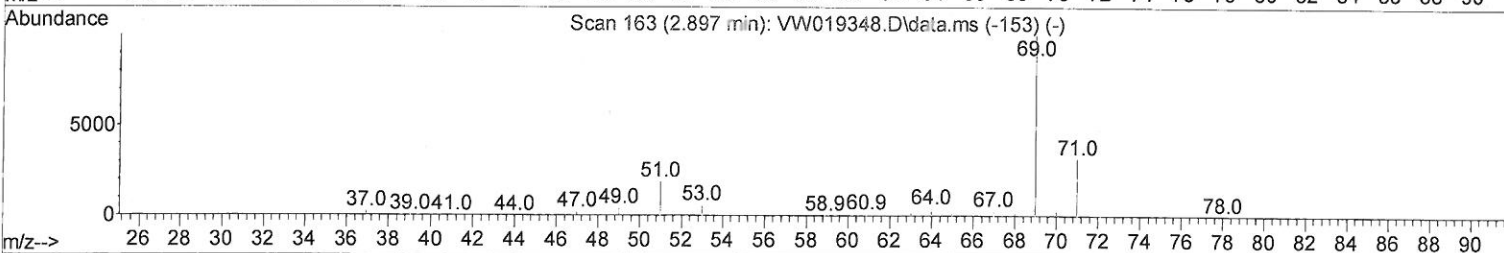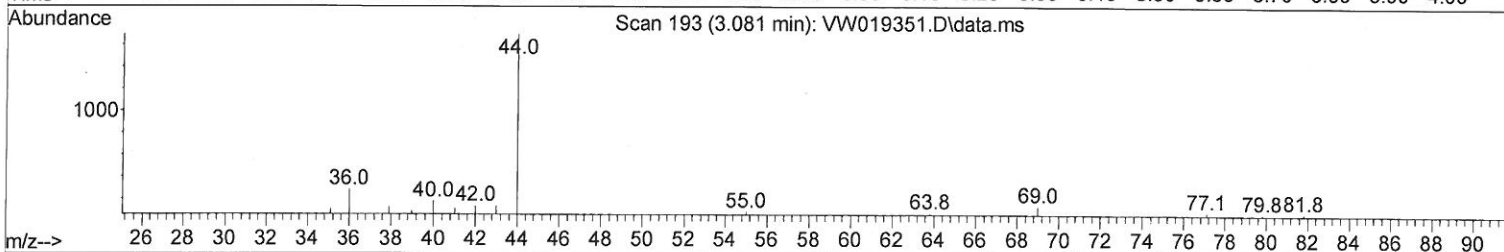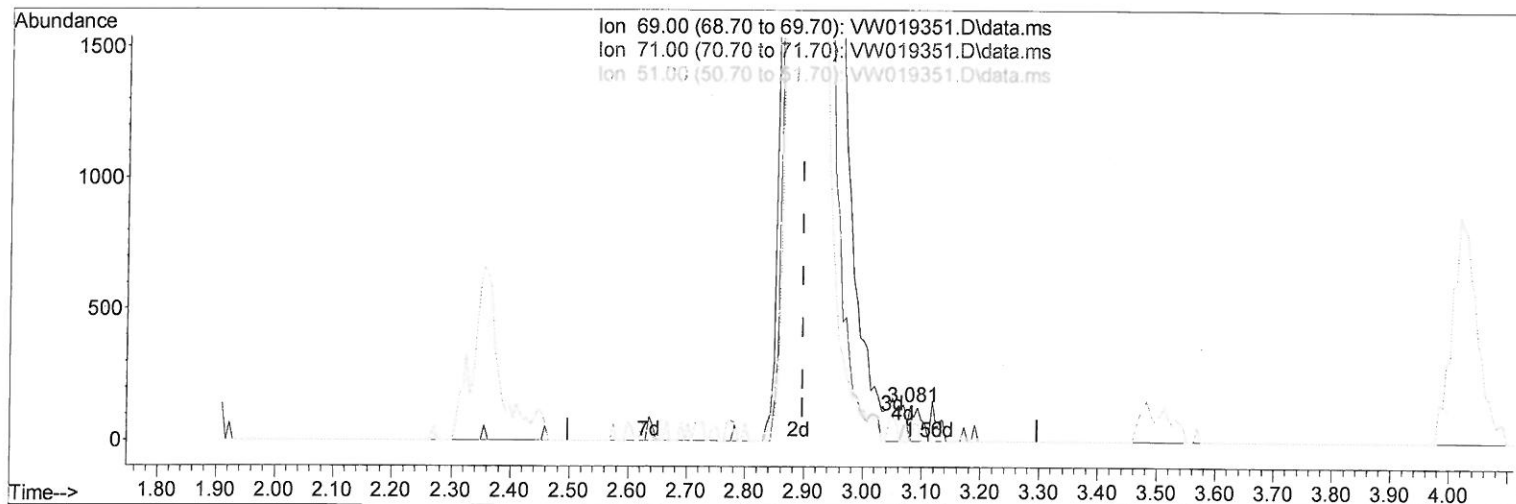

TIC: VW019351.D\data.ms

(7) Chloroethane-d5 (S)

3.081min (+ 0.183) 0.03 ug/L

response 184

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	24.46
51.00	28.40	26.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019351.D
Acq On : 29 Jun 2021 10:57
Operator : SY/VA
Sample : M2808-22
Misc : 4.39G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDX9

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:14 PM

Quant Time: Jun 30 01:20:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

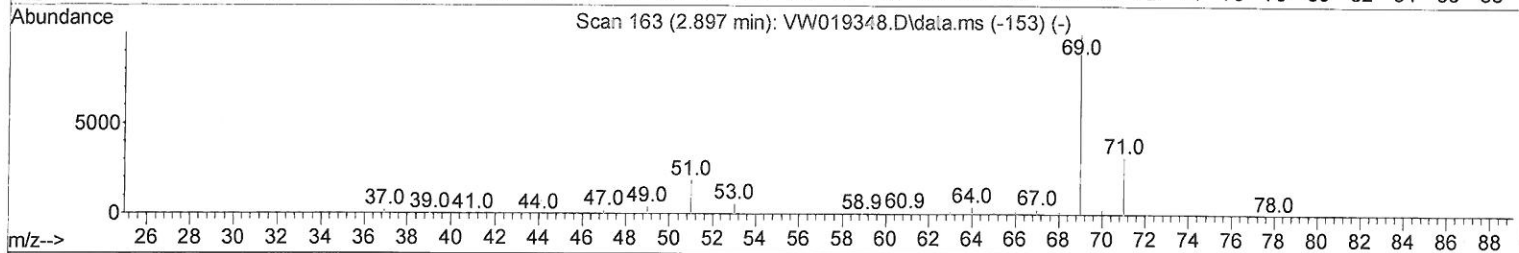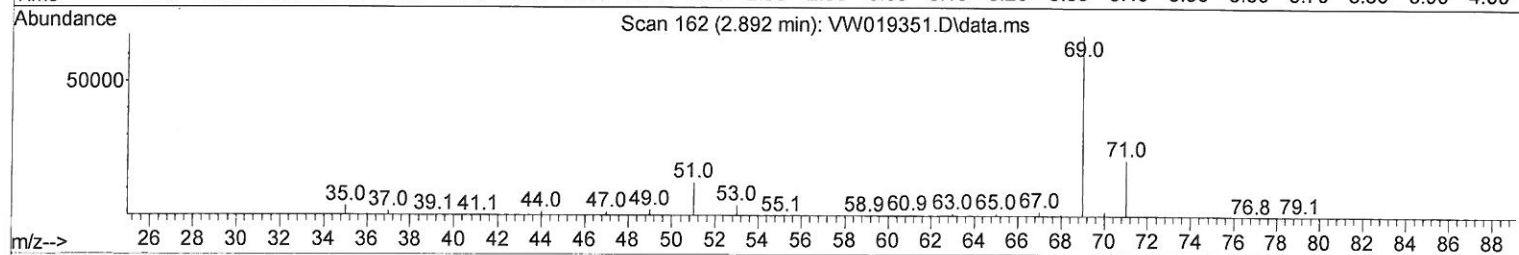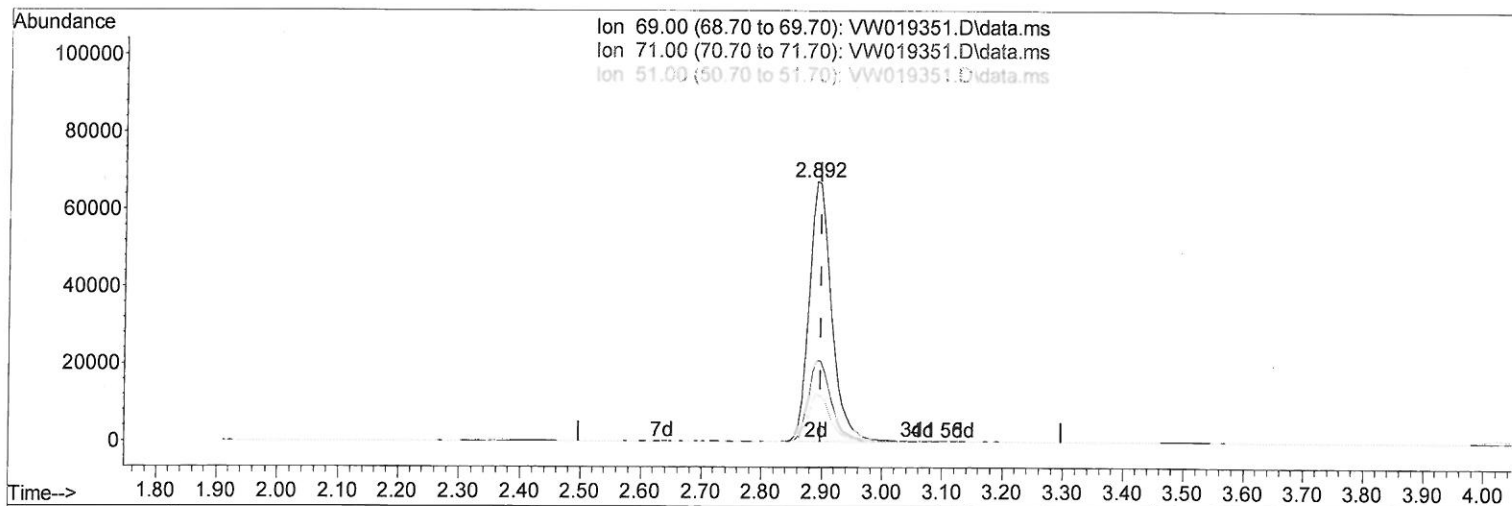

TIC: VW019351.D\data.ms

(7) Chloroethane-d5 (S)

2.892min (-0.006) 26.34 ug/L m

response 171836

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.03#
51.00	28.40	0.03#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019351.D
 Acq On : 29 Jun 2021 10:57
 Operator : SY/VA
 Sample : M2808-22
 Misc : 4.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BGDx9

Manual Integrations
APPROVED

MMDadoda
 6/30/2021 3:12:14 PM

Quant Time: Jun 30 02:50:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

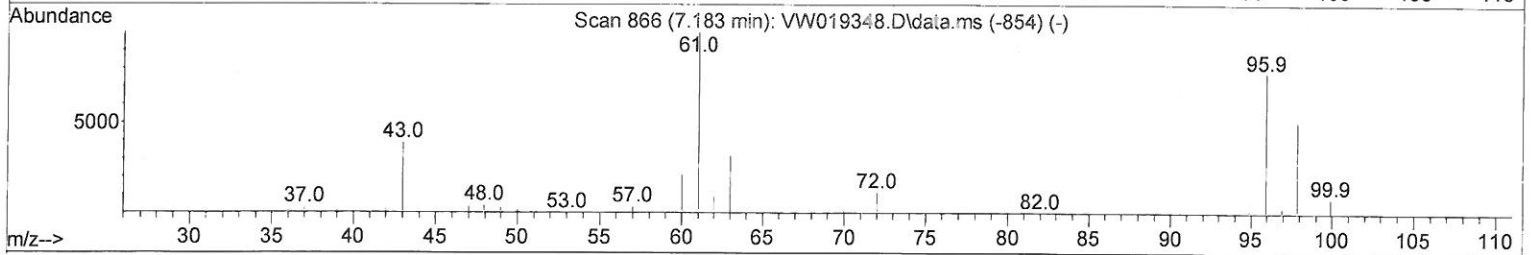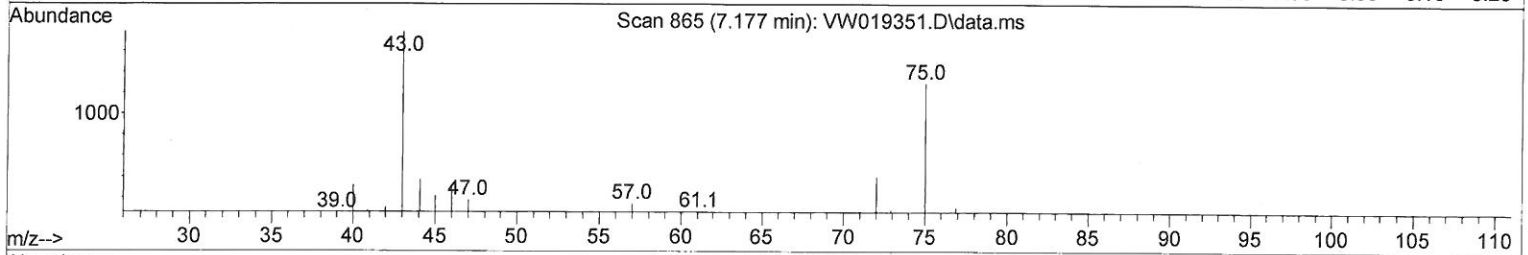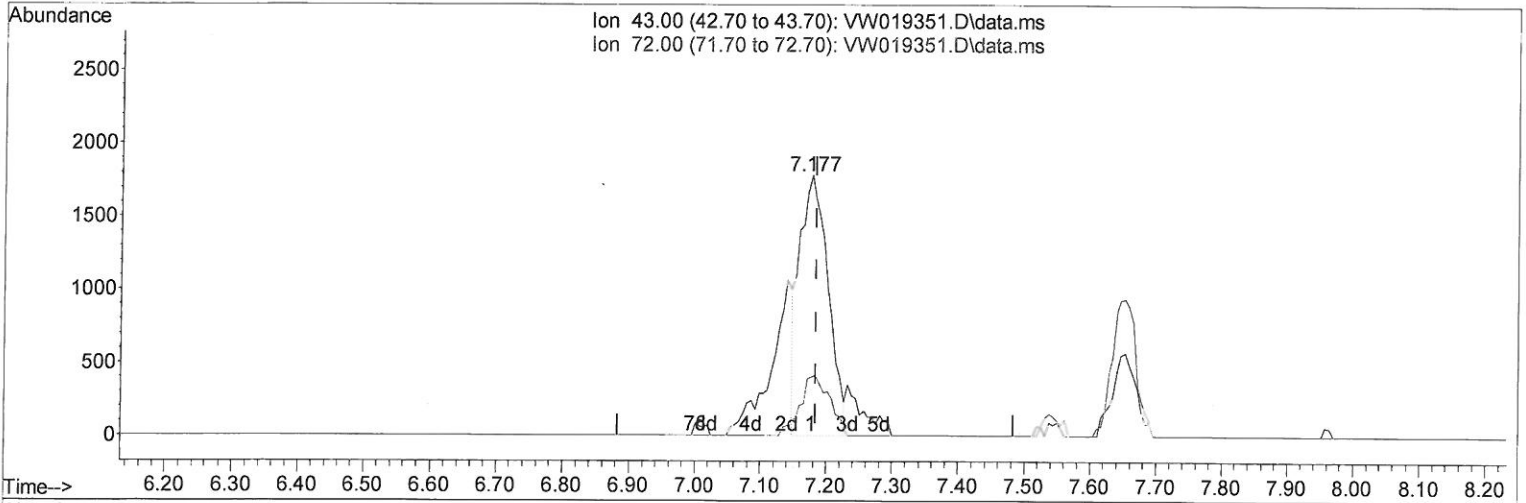

TIC: VW019351.D\data.ms

(22) 2-Butanone (T)

7.177min (-0.006) 2.44 ug/L

response 5413

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	23.68
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019351.D
Acq On : 29 Jun 2021 10:57
Operator : SY/VA
Sample : M2808-22
Misc : 4.39G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDX9

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:14 PM

Quant Time: Jun 30 01:20:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

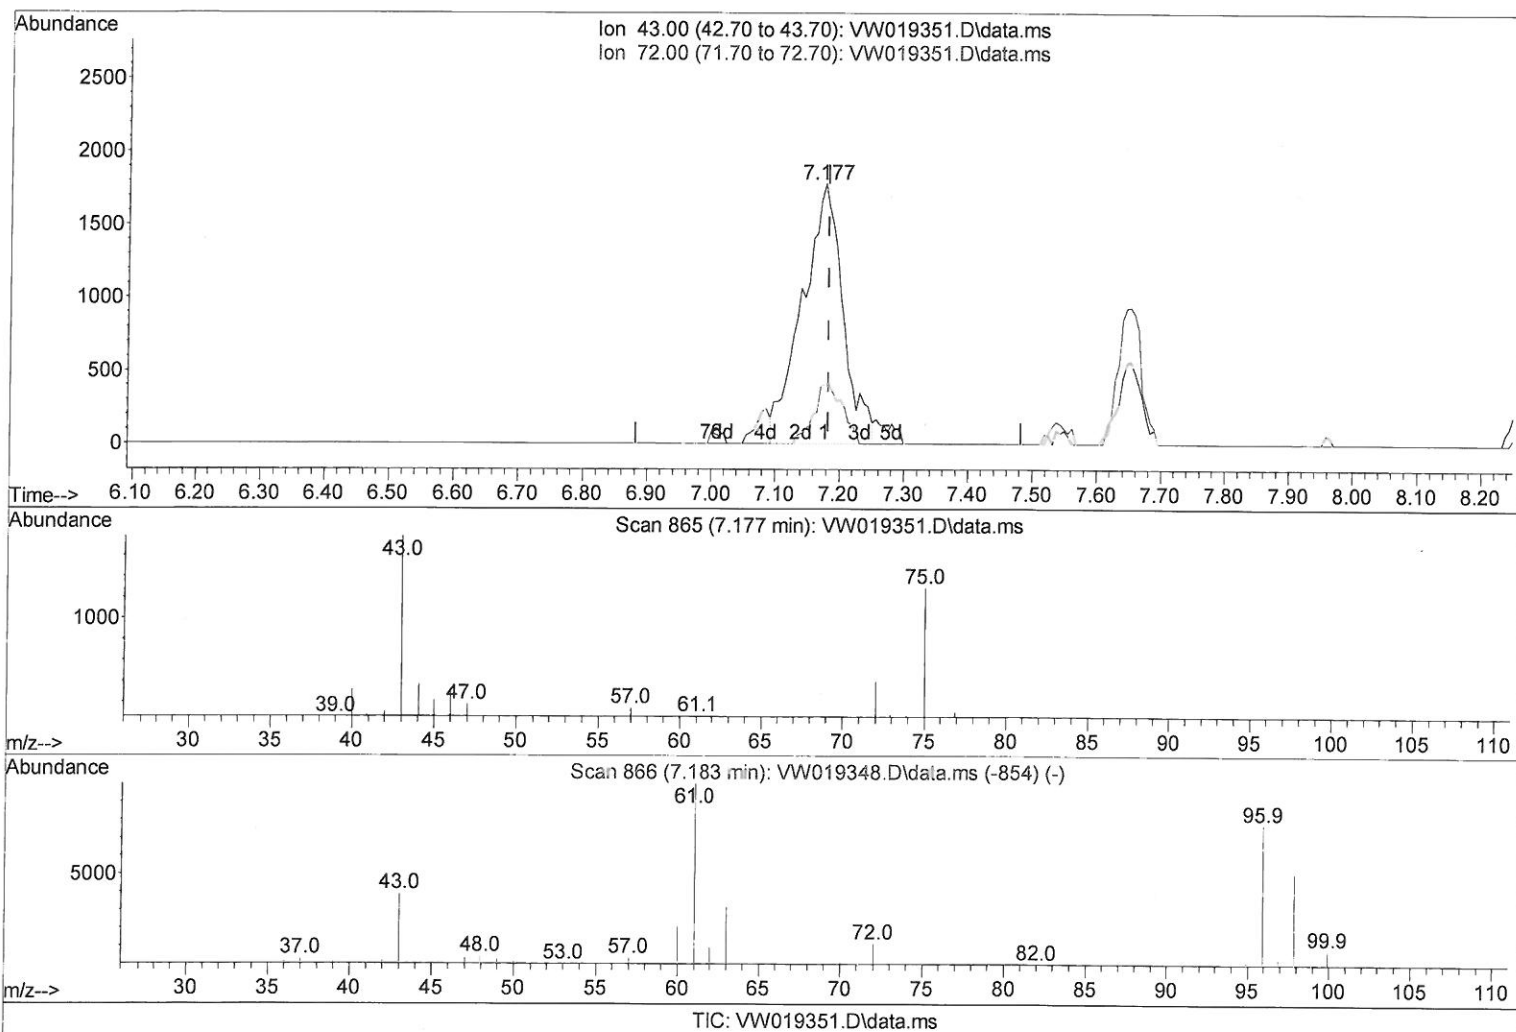

(22) 2-Butanone (T)

7.177min (-0.006) 3.52 ug/L m

response 7815

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	16.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019351.D
 Acq On : 29 Jun 2021 10:57
 Operator : SY/VA
 Sample : M2808-22
 Misc : 4.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDx9

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:14 PM

Quant Time: Jun 30 01:20:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	639163	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	487032	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	151352	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	190655	22.720	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 90.880%			
7) Chloroethane-d5	2.892	69	171836m	26.341	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 105.360%			
11) 1,1-Dichloroethene-d2	4.026	63	327304	19.087	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 76.360%			
21) 2-Butanone-d5	7.080	46	72645	34.856	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 69.720%			
24) Chloroform-d	7.653	84	433889	24.574	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 98.280%			
26) 1,2-Dichloroethane-d4	8.311	65	211381	23.313	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 93.240%			
32) Benzene-d6	8.281	84	924231	30.964	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 123.840%			
36) 1,2-Dichloropropane-d6	9.275	67	275064	30.234	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 120.920%#			
41) Toluene-d8	10.323	98	791424	29.274	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 117.080%			
43) trans-1,3-Dichloroprop...	10.579	79	75125	20.971	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 83.880%			
47) 2-Hexanone-d5	10.927	63	57058	40.129	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 80.260%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	140124	20.878	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 83.520%			
66) 1,2-Dichlorobenzene-d4	13.853	152	136652	24.682	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 98.720%			
Target Compounds						
13) Acetone	4.129	43	10205	7.850	ug/L	89
16) Methylene chloride	4.922	84	28017	2.508	ug/L	94
22) 2-Butanone	7.177	43	7815m	3.525	ug/L	
42) Toluene	10.390	91	10485	0.318	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019351.D
Acq On : 29 Jun 2021 10:57
Operator : SY/VA
Sample : M2808-22
Misc : 4.39G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDX9

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:14 PM

Quant Time: Jun 30 01:20:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

