

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019364.D
 Acq On : 29 Jun 2021 16:09
 Operator : SY/VA
 Sample : M2878-15
 Misc : 5.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGE07

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:26 PM

Quant Time: Jun 30 01:23:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

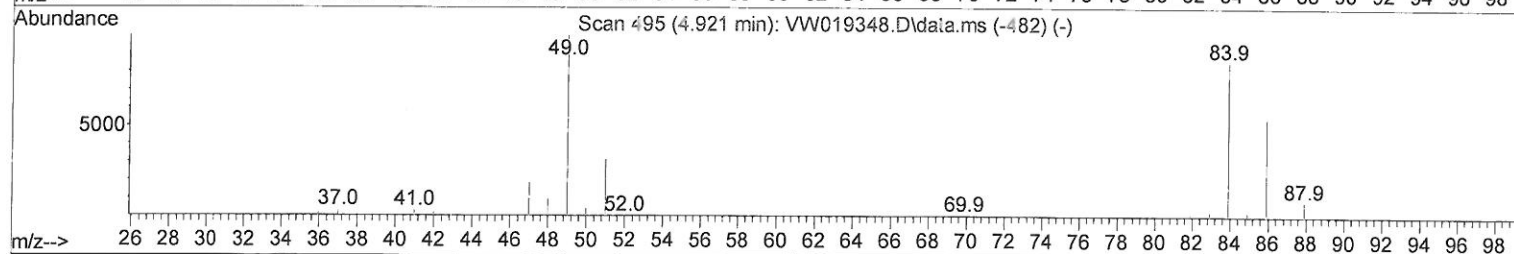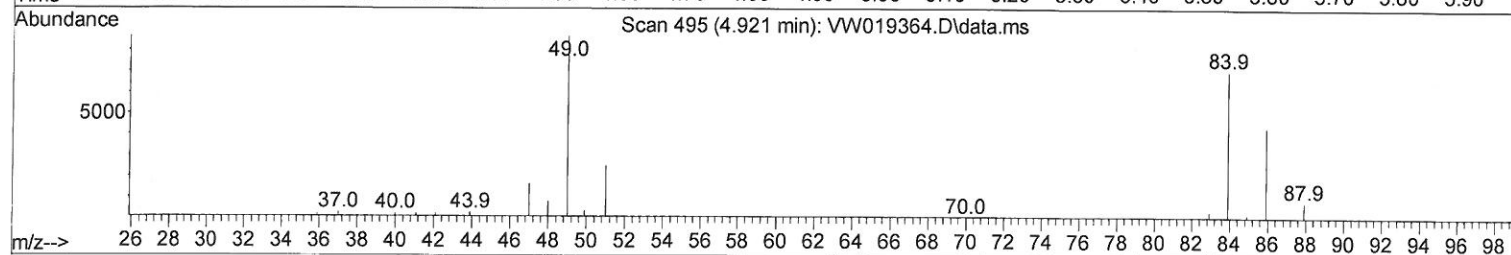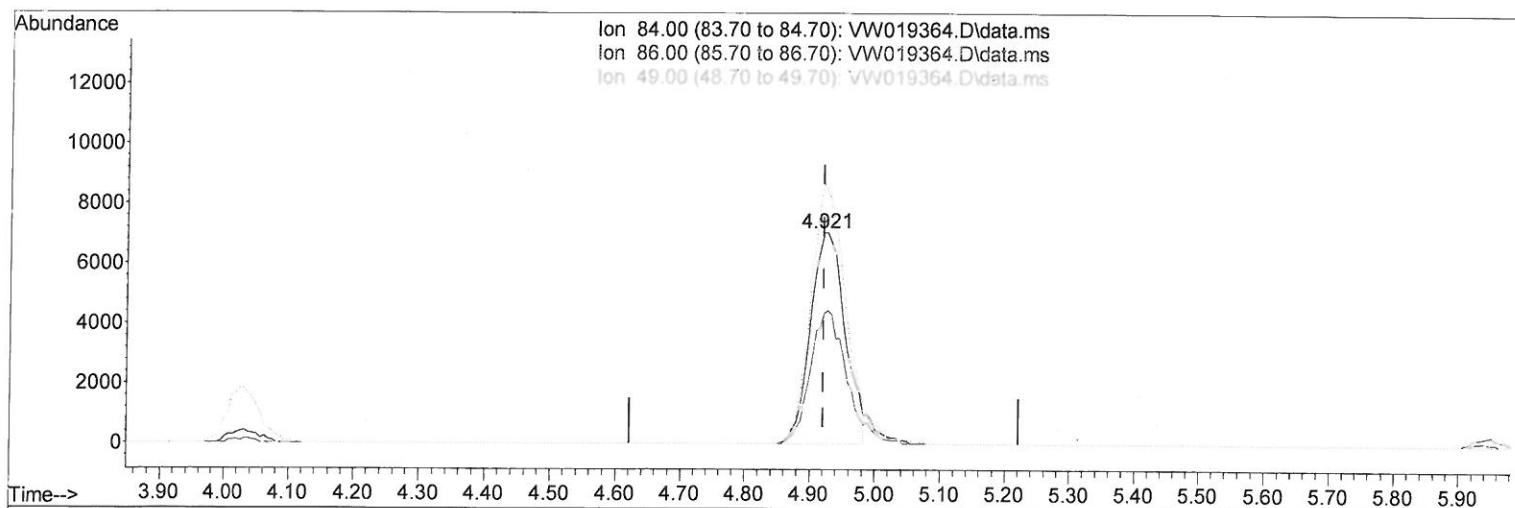

TIC: VW019364.D\data.ms

(16) Methylene chloride (T)

4.921min (+ 0.000) 4.07 ug/L

response 26213

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	61.79
49.00	123.70	123.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019364.D
 Acq On : 29 Jun 2021 16:09
 Operator : SY/VA
 Sample : M2878-15
 Misc : 5.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGE07

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:26 PM

Quant Time: Jun 30 01:23:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

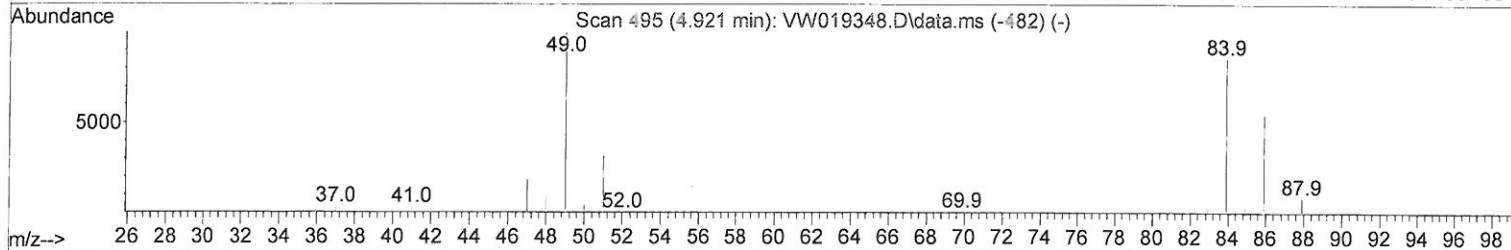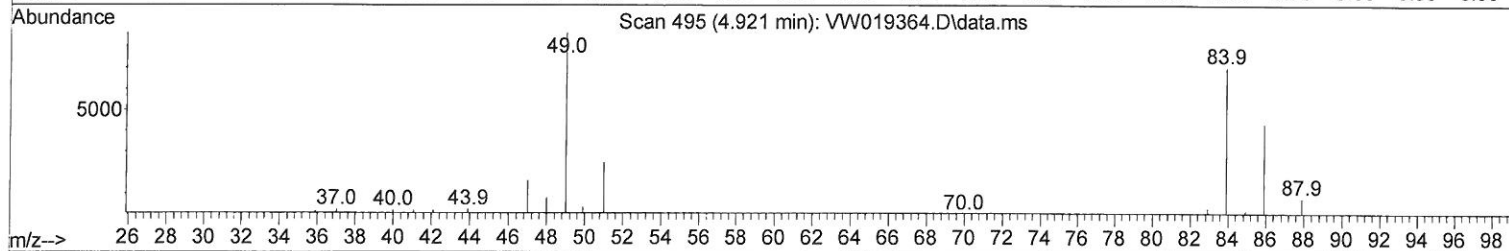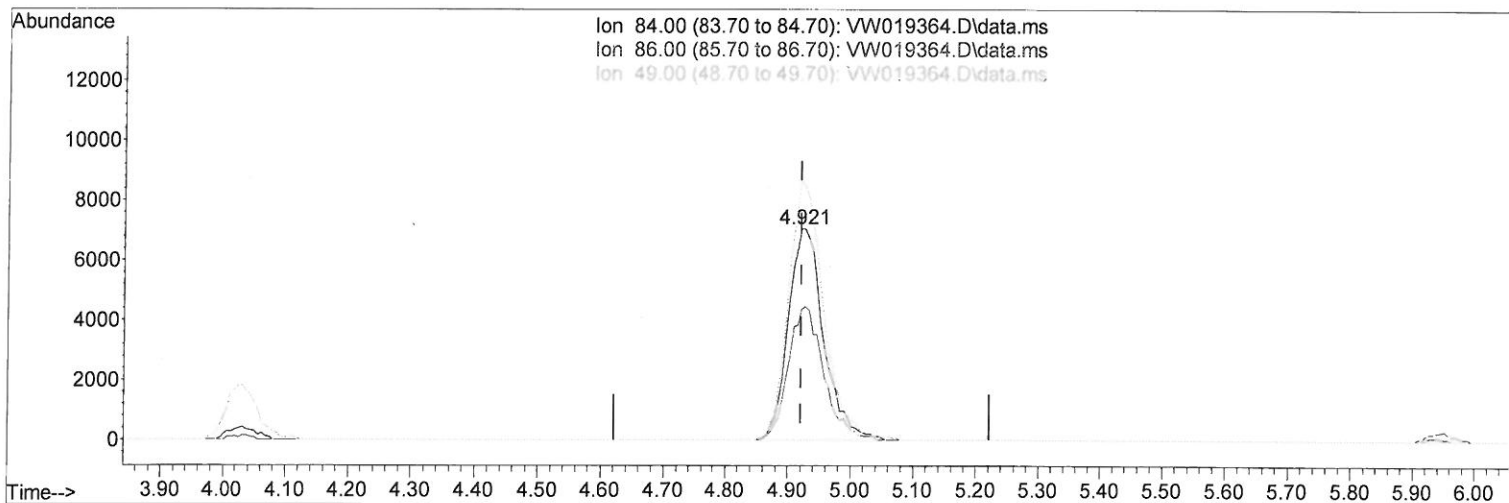

TIC: VW019364.D\data.ms

(16) Methylene chloride (T)

4.921min (+ 0.000) 4.29 ug/L m

response 27624

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	61.79
49.00	123.70	123.04
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019364.D
 Acq On : 29 Jun 2021 16:09
 Operator : SY/VA
 Sample : M2878-15
 Misc : 5.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGE07

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:26 PM

Quant Time: Jun 30 01:23:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

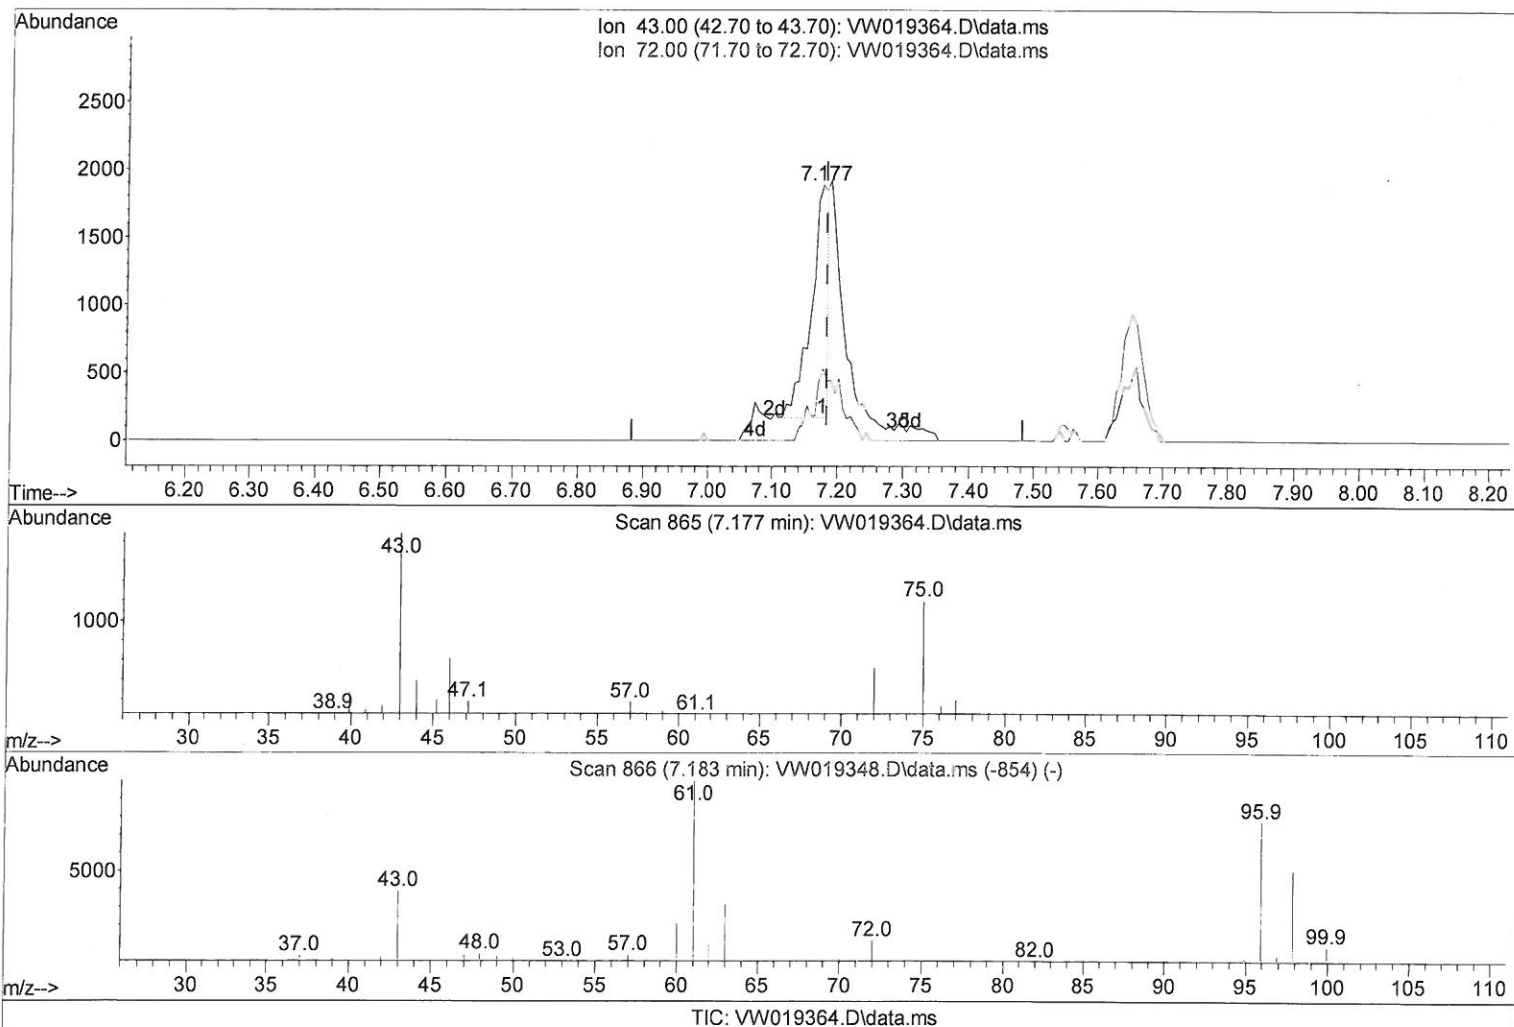

(22) 2-Butanone (T)

7.177min (-0.006) 2.45 ug/L

response 3128

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	16.53
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019364.D
Acq On : 29 Jun 2021 16:09
Operator : SY/VA
Sample : M2878-15
Misc : 5.05G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGE07

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:26 PM

Quant Time: Jun 30 01:23:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

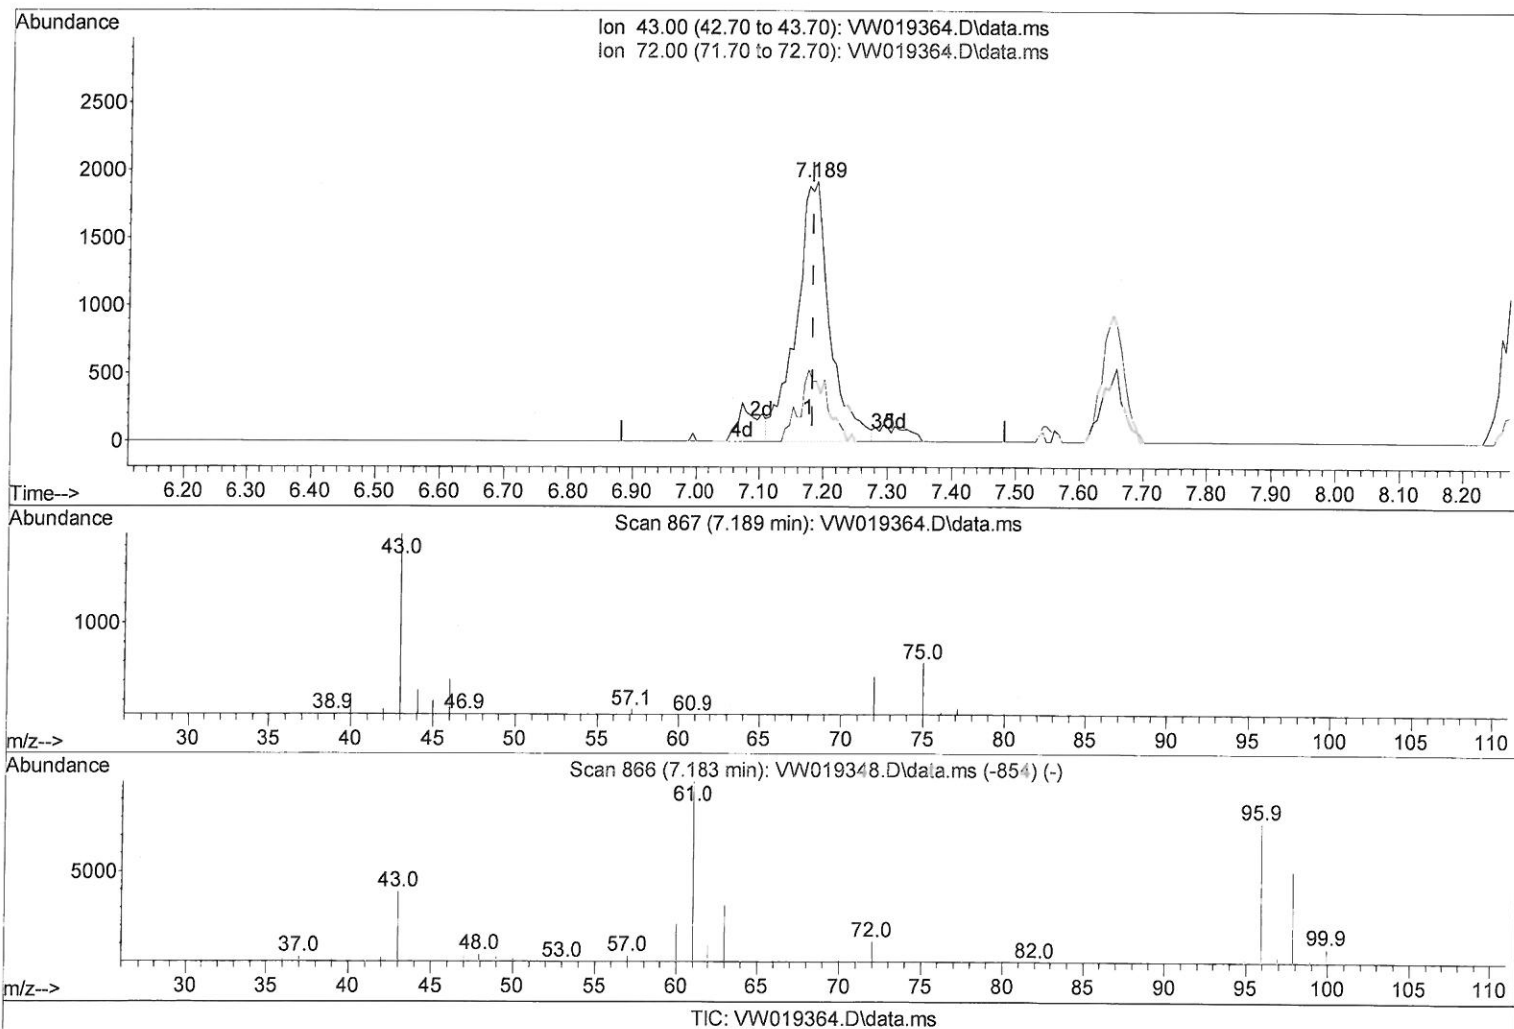

(22) 2-Butanone (T)

7.189min (+ 0.006) 5.42 ug/L m

response 6927

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	7.46#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019364.D
 Acq On : 29 Jun 2021 16:09
 Operator : SY/VA
 Sample : M2878-15
 Misc : 5.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGE07

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:26 PM

Quant Time: Jun 30 01:23:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	368210	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	299166	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	112559	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	161594	33.427	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	133.720%	
7) Chloroethane-d5	2.897	69	146137	38.886	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	155.560%#	
11) 1,1-Dichloroethene-d2	4.025	63	272021	27.537	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	110.160%#	
21) 2-Butanone-d5	7.080	46	73344	61.087	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	122.180%	
24) Chloroform-d	7.653	84	391904	38.530	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	154.120%#	
26) 1,2-Dichloroethane-d4	8.311	65	198853	38.070	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	152.280%#	
32) Benzene-d6	8.281	84	785663	42.851	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	171.400%#	
36) 1,2-Dichloropropane-d6	9.274	67	247790	44.339	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	177.360%#	
41) Toluene-d8	10.323	98	630012	37.937	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	151.760%#	
43) trans-1,3-Dichloroprop...	10.579	79	76923	34.957	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	139.840%#	
47) 2-Hexanone-d5	10.926	63	56649	64.860	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	129.720%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	153649	37.269	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	149.080%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	163176	39.630	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	158.520%#	
Target Compounds						
13) Acetone	4.129	43	22423	29.940	ug/L	92
16) Methylene chloride	4.921	84	27624m	4.292	ug/L	
22) 2-Butanone	7.189	43	6927m	5.423	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019364.D
Acq On : 29 Jun 2021 16:09
Operator : SY/VA
Sample : M2878-15
Misc : 5.05G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGE07

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:26 PM

Quant Time: Jun 30 01:23:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

