

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019367.D
Acq On : 29 Jun 2021 17:21
Operator : SY/VA
Sample : M2878-15
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGE07

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:34 PM

Quant Time: Jun 30 03:02:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

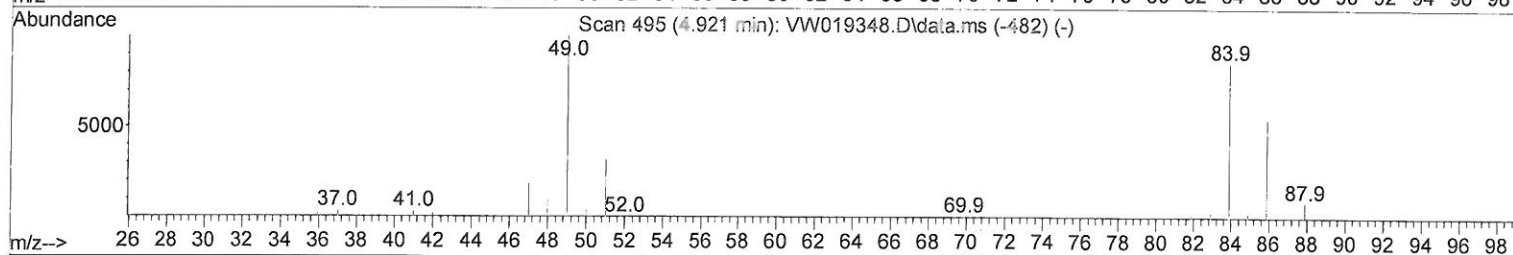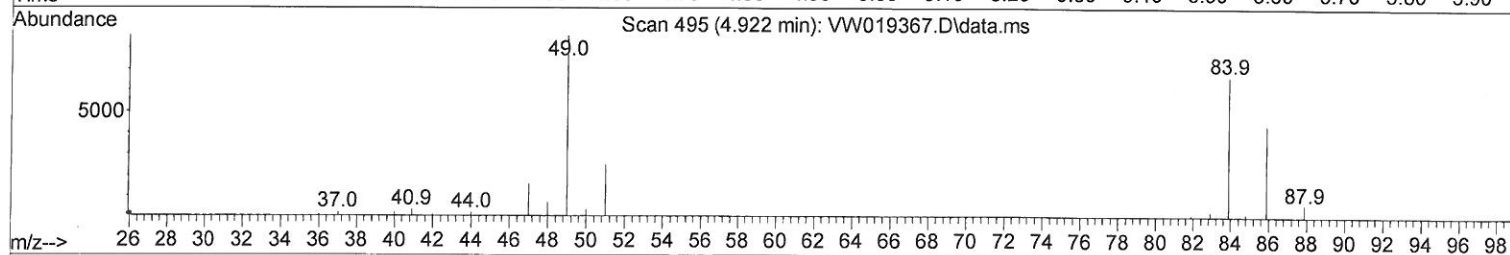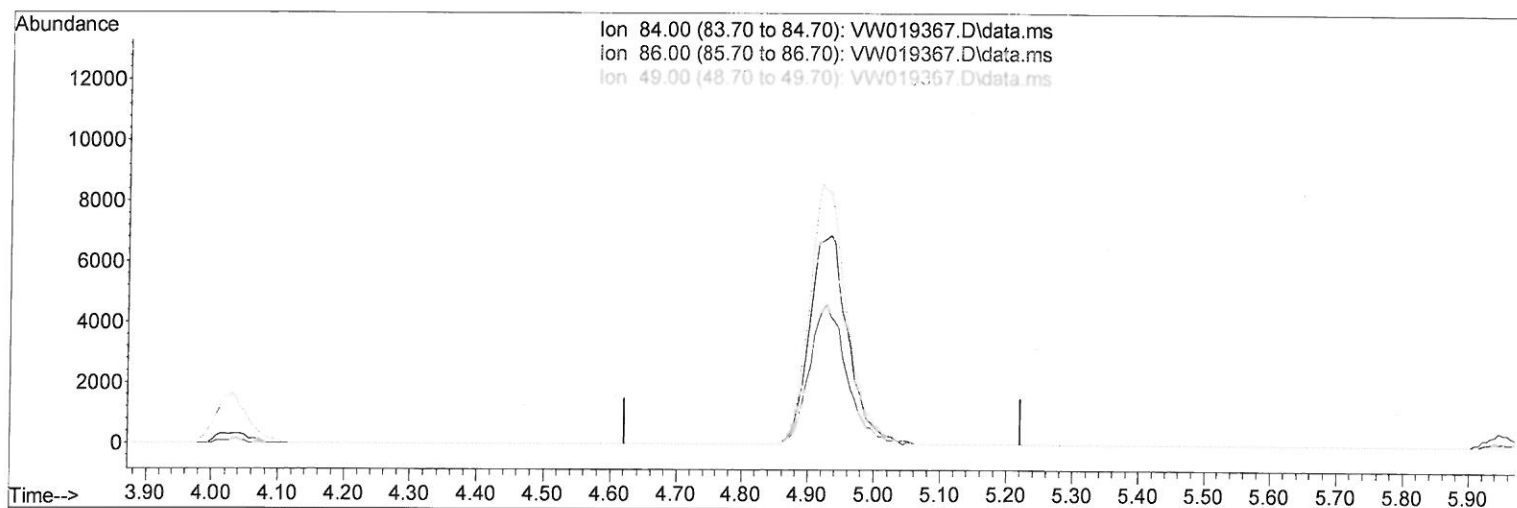

TIC: VW019367.D\data.ms

(16) Methylene chloride (T)

4.921min (-4.921) 0.00 ug/L

response 0

Ion	Exp%	Act%
84.00	100.00	0.00
86.00	64.70	0.00#
49.00	123.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019367.D
 Acq On : 29 Jun 2021 17:21
 Operator : SY/VA
 Sample : M2878-15
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGE07

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:34 PM

Quant Time: Jun 30 01:23:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

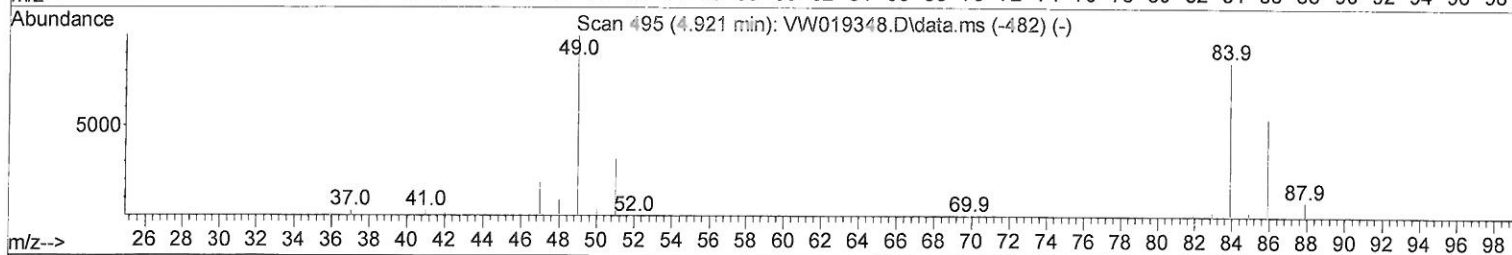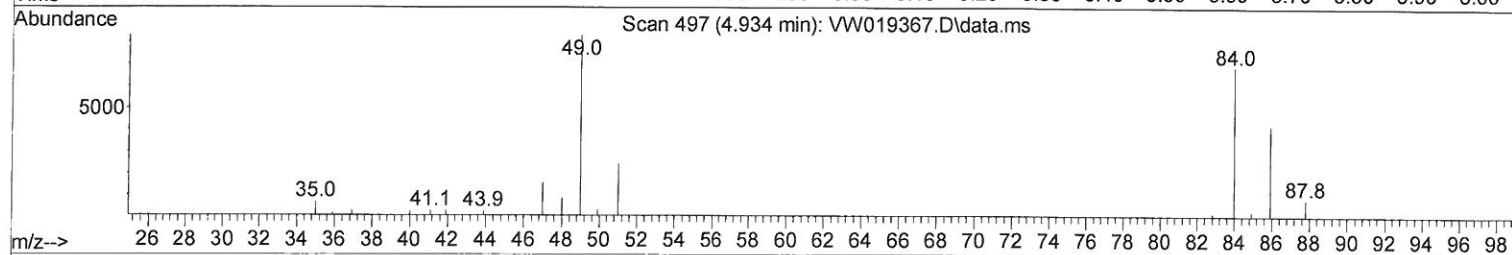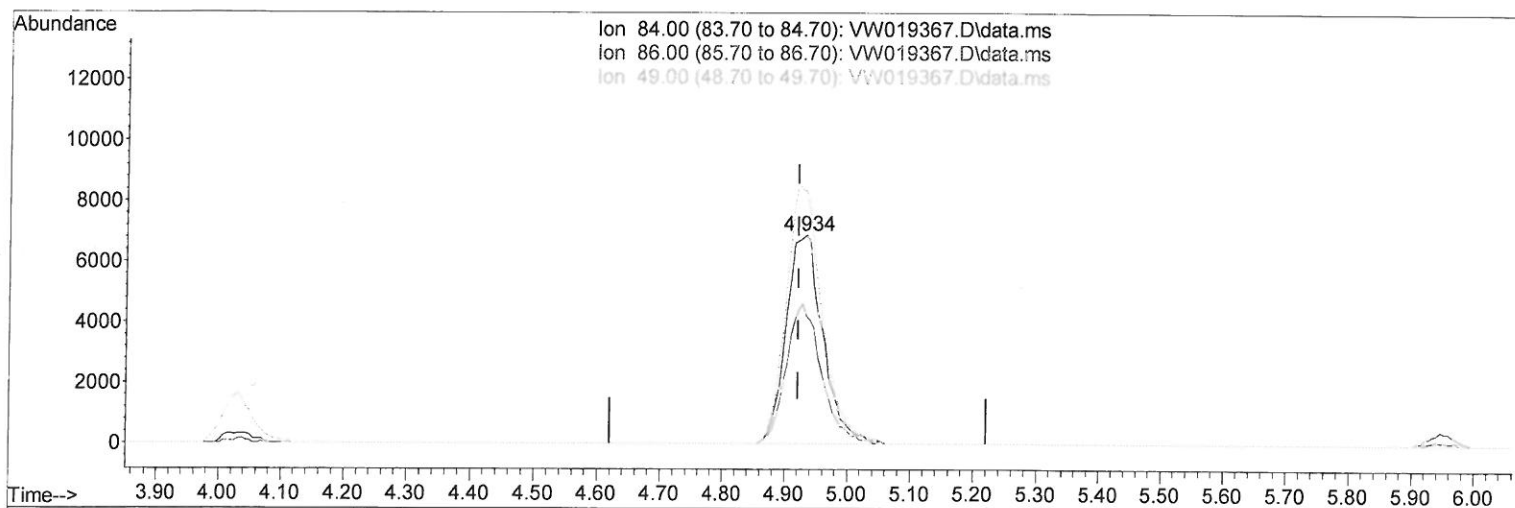

TIC: VW019367.D\data.ms

(16) Methylene chloride (T)

4.934min (+ 0.012) 2.78 ug/L m

response 28120

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	60.92
49.00	123.70	120.80
0.00	0.00	0.00

706/30/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019367.D
 Acq On : 29 Jun 2021 17:21
 Operator : SY/VA
 Sample : M2878-15
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGE07

Manual Integrations
 APPROVED

MMDadoda
 6/30/2021 3:12:34 PM

Quant Time: Jun 30 01:23:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	578016	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	506542	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	217926	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	146587	19.316	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.280%		
7) Chloroethane-d5	2.898	69	118459	20.080	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.320%		
11) 1,1-Dichloroethene-d2	4.025	63	230150	14.841	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.360%		
21) 2-Butanone-d5	7.080	46	58479	31.027	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	62.060%		
24) Chloroform-d	7.653	84	310240	19.430	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.720%		
26) 1,2-Dichloroethane-d4	8.311	65	151892	18.524	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	74.080%		
32) Benzene-d6	8.281	84	649564	20.924	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.680%		
36) 1,2-Dichloropropane-d6	9.274	67	196895	20.808	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.240%		
41) Toluene-d8	10.323	98	576006	20.485	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.960%		
43) trans-1,3-Dichloroprop...	10.579	79	65164	17.490	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	69.960%		
47) 2-Hexanone-d5	10.927	63	48546	32.827	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	65.660%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	119406	17.106	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	68.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	162649	20.403	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.600%		
Target Compounds						
13) Acetone	4.135	43	12007	10.213	ug/L	89
16) Methylene chloride	4.934	84	28120m	2.783	ug/L	83
22) 2-Butanone	7.183	43	5119	2.553	ug/L	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019367.D
Acq On : 29 Jun 2021 17:21
Operator : SY/VA
Sample : M2878-15
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BGE07

Manual Integrations
APPROVED

MMDadoda
6/30/2021 3:12:34 PM

Quant Time: Jun 30 01:23:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

