

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
 Data File : VW019350.D
 Acq On : 29 Jun 2021 10:33
 Operator : SY/VA
 Sample : M2854-16
 Misc : 5.02G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jun 30 01:20:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 30 01:19:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	493986	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	448210	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	210111	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	164942	25.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.720%
7) Chloroethane-d5	2.897	69	127735	25.335	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.360%
11) 1,1-Dichloroethene-d2	4.025	63	246987	18.636	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.560%
21) 2-Butanone-d5	7.080	46	72453	44.980	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.960%
24) Chloroform-d	7.653	84	327309	23.986	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.960%
26) 1,2-Dichloroethane-d4	8.311	65	169543	24.194	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.760%
32) Benzene-d6	8.275	84	696956	25.372	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.480%
36) 1,2-Dichloropropane-d6	9.274	67	206974	24.720	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.880%
41) Toluene-d8	10.323	98	619293	24.891	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.560%
43) trans-1,3-Dichloroprop...	10.579	79	77211	23.420	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.680%
47) 2-Hexanone-d5	10.927	63	57826	44.192	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.380%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	141015	22.830	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	196951	25.624	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.480%
Target Compounds						Qvalue
16) Methylene chloride	4.928	84	22119	2.561	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062921\
Data File : VW019350.D
Acq On : 29 Jun 2021 10:33
Operator : SY/VA
Sample : M2854-16
Misc : 5.02G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Jun 30 01:20:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 30 01:19:19 2021
Response via : Initial Calibration

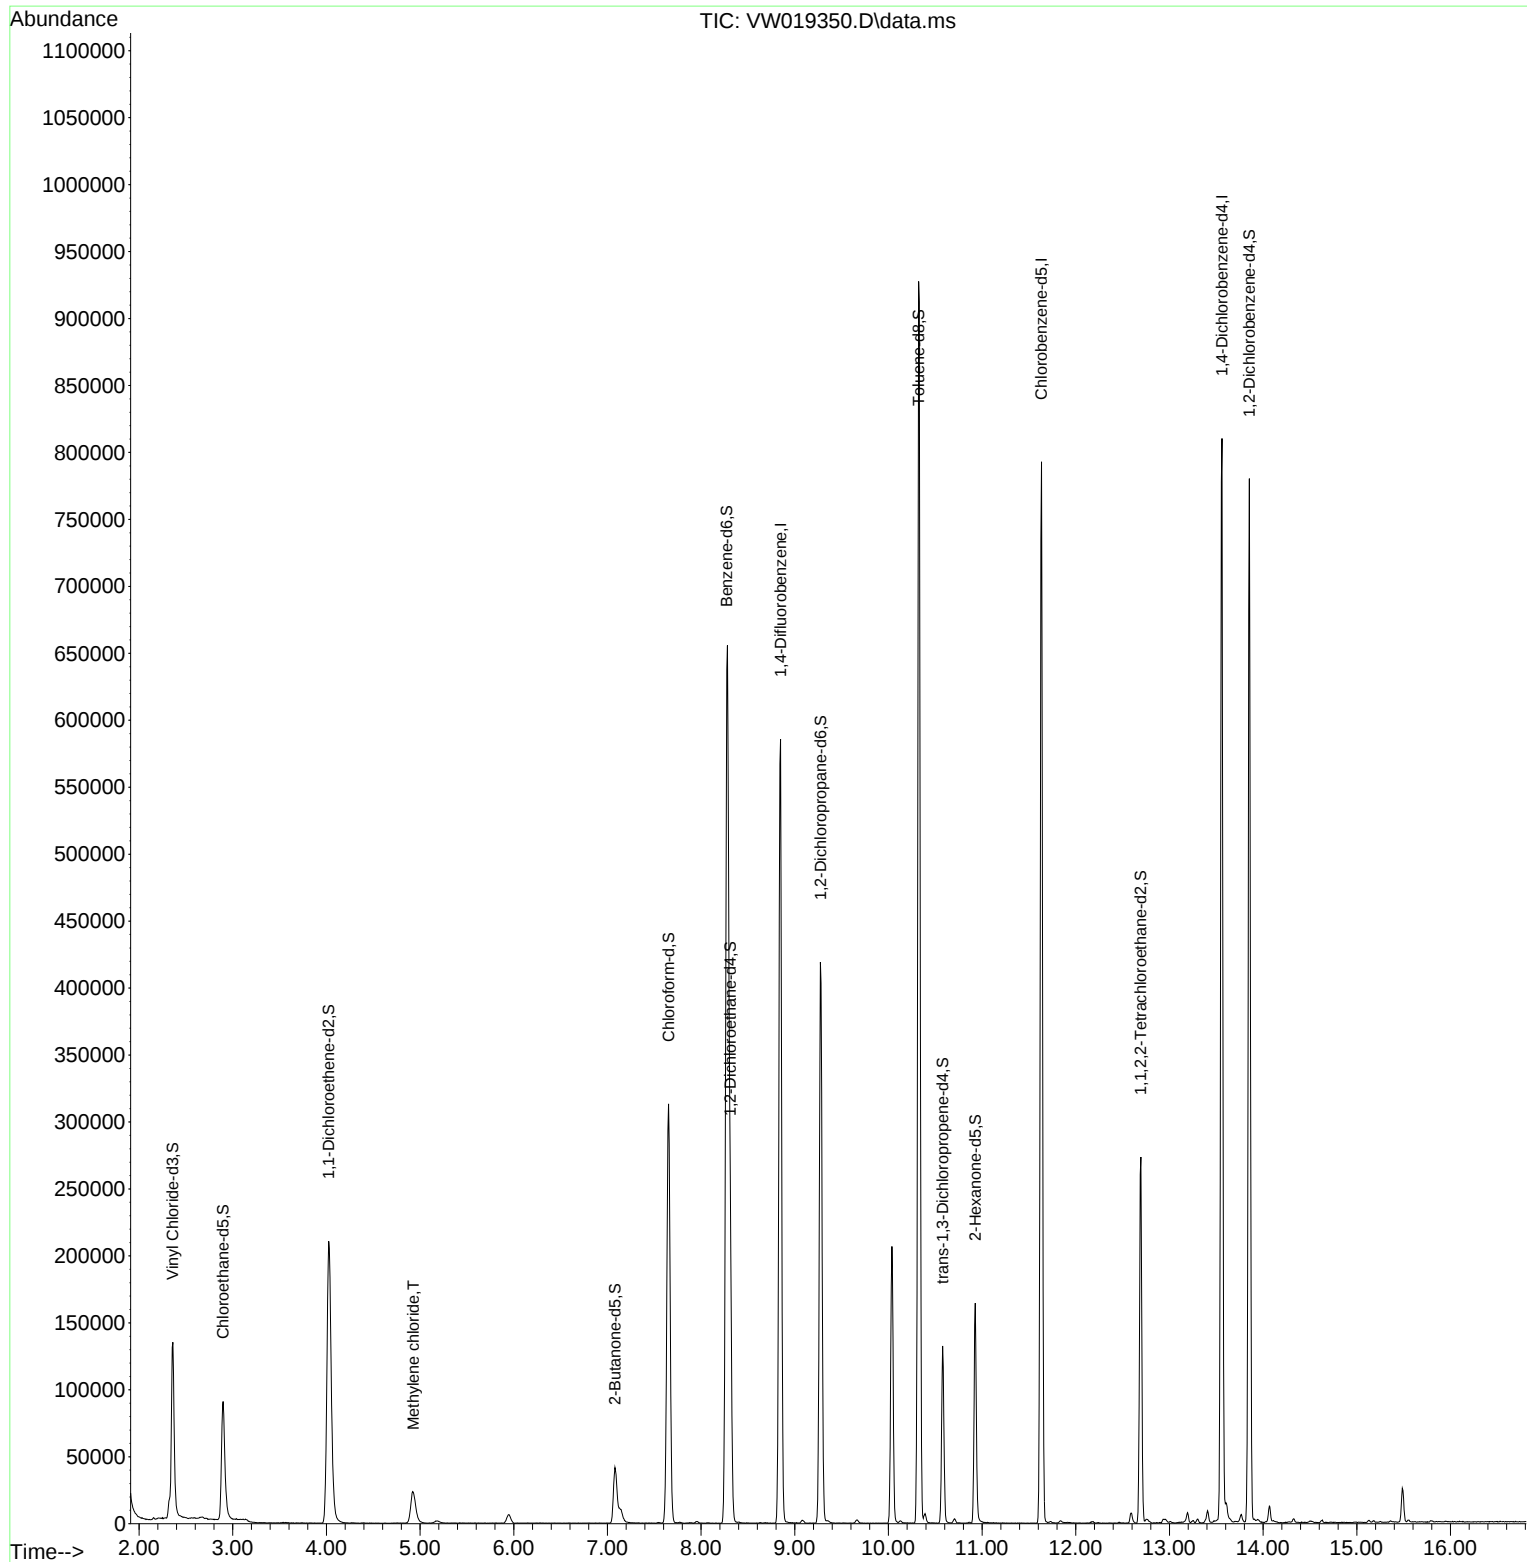

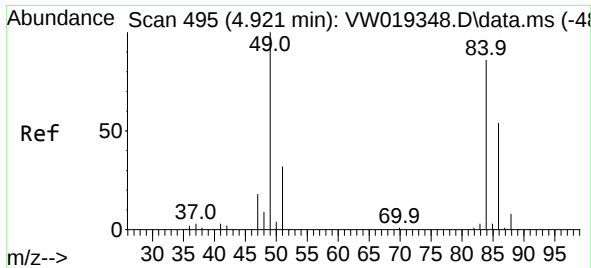

#16
Methylene chloride
Concen: 2.561 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019350.D
Acq: 29 Jun 2021 10:33

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	22119
Ion	Ratio	Lower	Upper
84	100		
86	58.2	45.3	84.1
49	115.7	86.6	160.8

