

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062923\
 Data File : VW026439.D
 Acq On : 29 Jun 2023 18:01
 Operator : SY/MD
 Sample : VW0629SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK530

Quant Time: Jun 30 01:20:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 01:16:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	832349	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	746573	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	356166	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	242170	25.553	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.200%			
7) Chloroethane-d5	2.893	69	196325	25.440	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.760%			
11) 1,1-Dichloroethene-d2	4.027	65	92205	19.445	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 77.760%			
21) 2-Butanone-d5	7.075	46	170057	47.481	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 94.960%			
24) Chloroform-d	7.648	84	481531	23.735	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 94.920%			
26) 1,2-Dichloroethane-d4	8.307	65	281152	25.353	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 101.400%			
32) Benzene-d6	8.276	84	1013160	23.334	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 93.320%			
36) 1,2-Dichloropropane-d6	9.276	67	334897	24.200	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 96.800%			
41) Toluene-d8	10.319	98	905821	23.617	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 94.480%			
43) trans-1,3-Dichloroprop...	10.581	79	124445	22.310	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 89.240%			
47) 2-Hexanone-d5	10.922	63	109968	47.517	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 95.040%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	245527	22.978	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 91.920%			
66) 1,2-Dichlorobenzene-d4	13.849	152	285703	23.037	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 92.160%			
Target Compounds						Qvalue
16) Methylene chloride	4.929	84	29366	2.088	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062923\
Data File : VW026439.D
Acq On : 29 Jun 2023 18:01
Operator : SY/MD
Sample : VW0629SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK530


Quant Time: Jun 30 01:20:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 30 01:16:39 2023
Response via : Initial Calibration

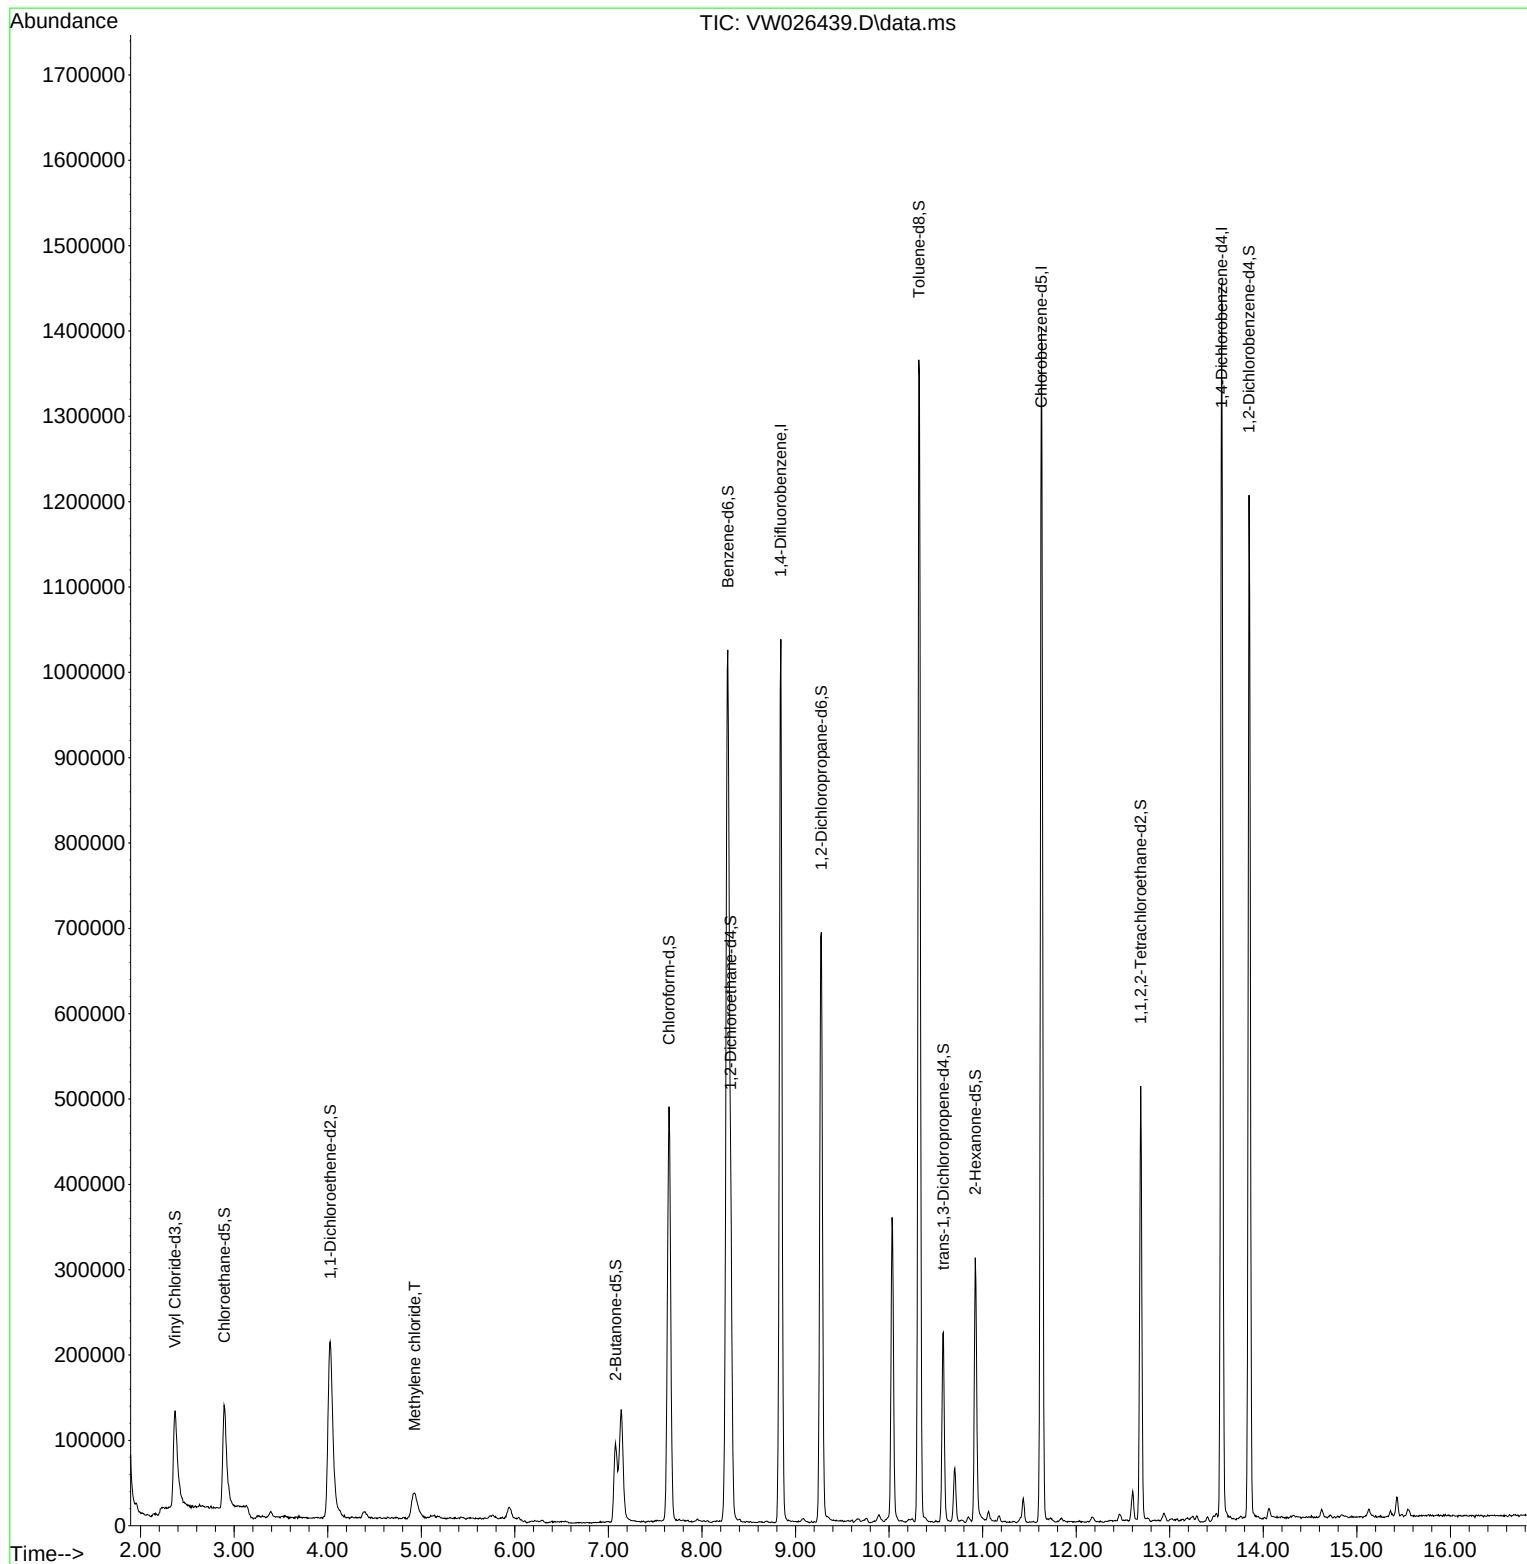

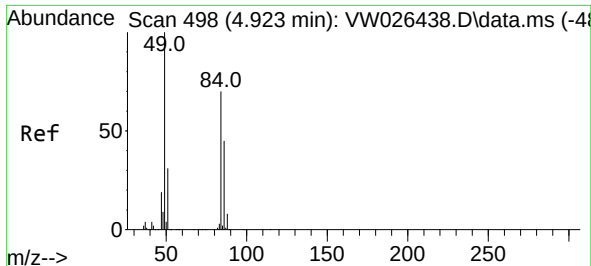

#16
Methylene chloride
Concen: 2.088 ug/L
RT: 4.929 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW026439.D
Acq: 29 Jun 2023 18:01

Instrument :
MSVOA_W
ClientSampleId :
VBLK530

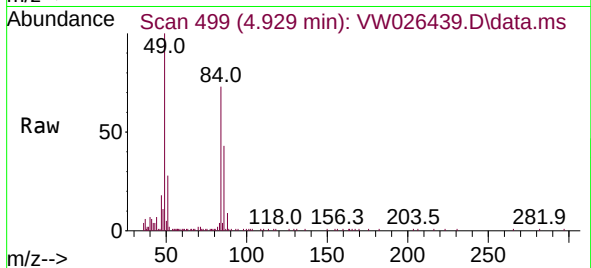

Tgt Ion:	84	Resp:	29366
Ion	Ratio	Lower	Upper
84	100		
86	59.7	44.1	81.9
49	137.9	94.1	174.8

