




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026483.D
 Acq On : 30 Jun 2023 19:30
 Operator : SY/MD
 Sample : 03504-02
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46S2

Manual IntegrationsAPPROVED

Quant Time: Jun 30 23:44:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

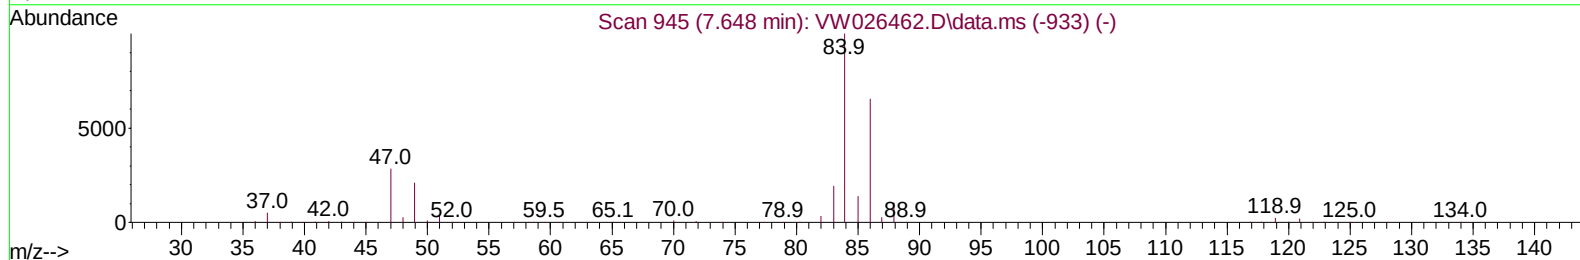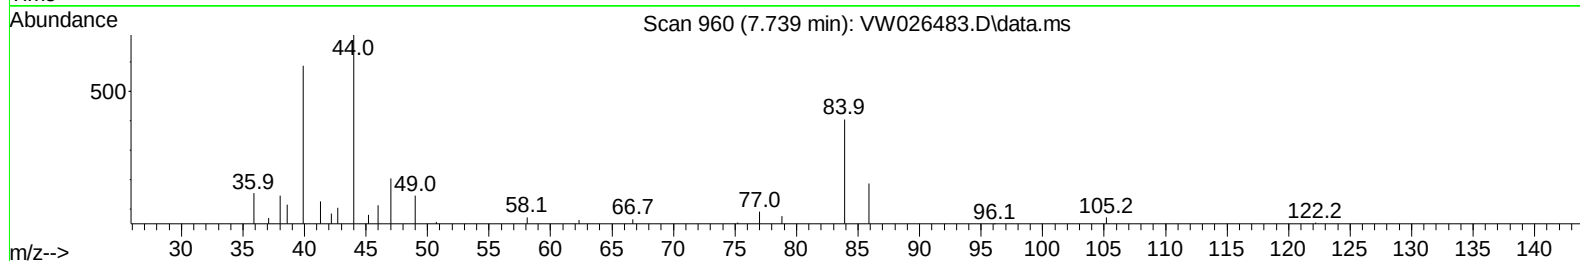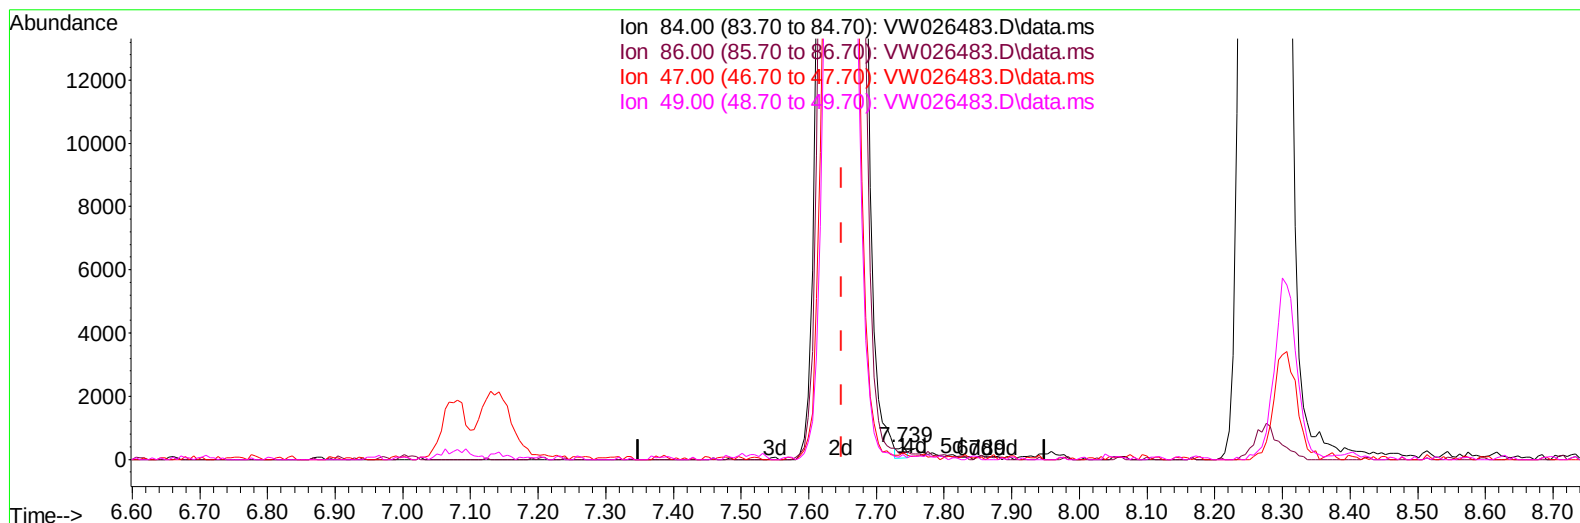

TIC: VW026483.D\data.ms

(24) Chloroform-d (S)

7.739min (+ 0.091) 0.01 ug/L

response 317

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	66.25
47.00	45.20	48.58
49.00	26.30	23.66




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026483.D
 Acq On : 30 Jun 2023 19:30
 Operator : SY/MD
 Sample : 03504-02
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46S2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:26:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

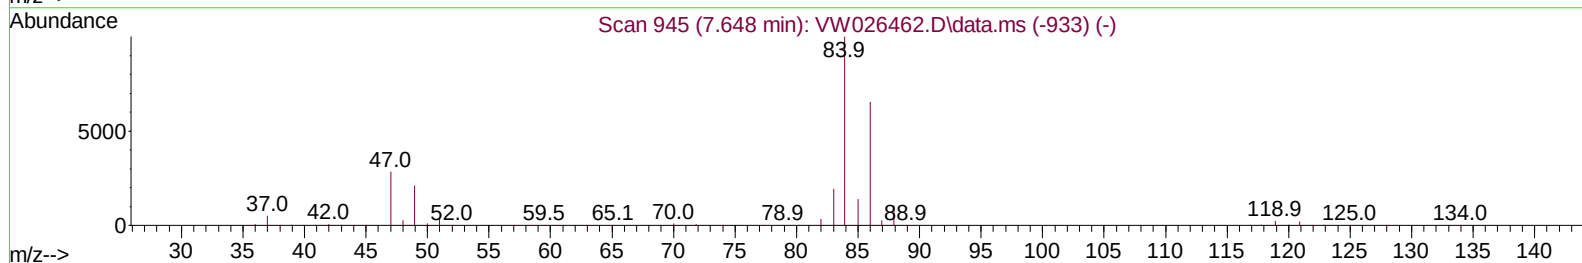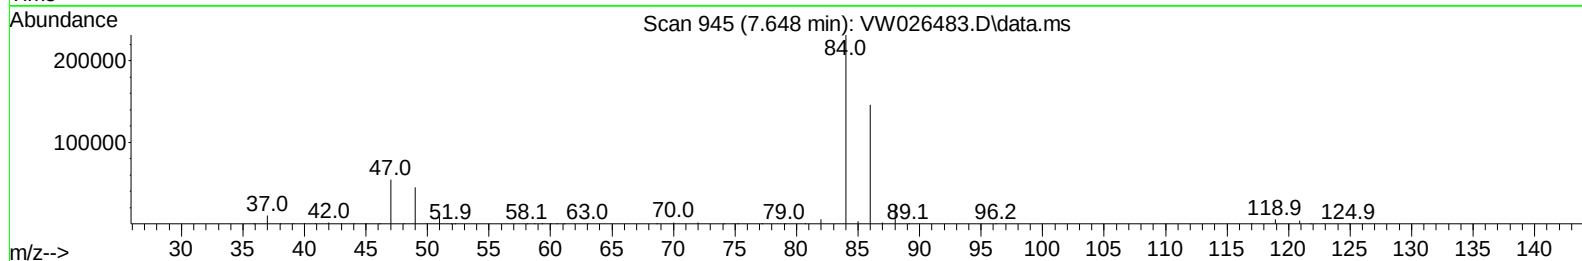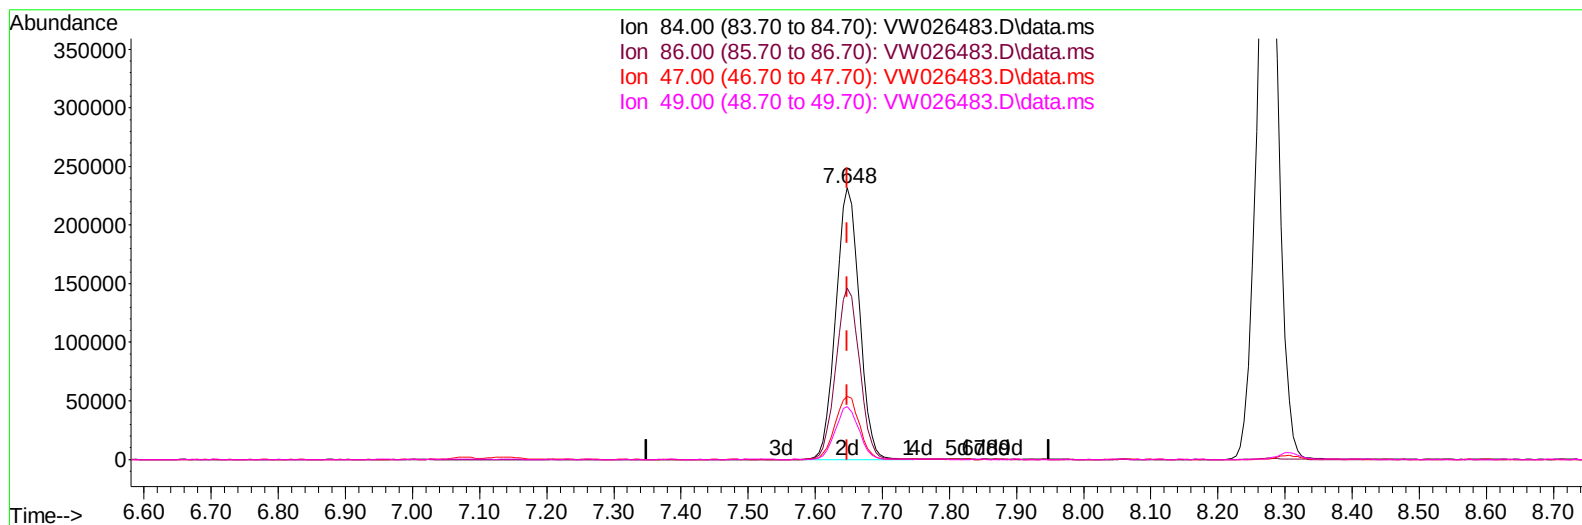

TIC: VW026483.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 21.50 ug/L m

response 564041

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	0.04#
47.00	45.20	0.03#
49.00	26.30	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026483.D
 Acq On : 30 Jun 2023 19:30
 Operator : SY/MD
 Sample : 03504-02
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46S2

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:26:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		1076103	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		883955	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152		349115	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		229456	18.727	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	74.920%	
7) Chloroethane-d5	2.899	69		196325	19.678	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.720%	
11) 1,1-Dichloroethene-d2	4.027	65		121163	19.764	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	79.040%	
21) 2-Butanone-d5	7.075	46		207440	44.799	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	89.600%	
24) Chloroform-d	7.648	84		564041m	21.504	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	86.000%	
26) 1,2-Dichloroethane-d4	8.306	65		323370	22.555	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	90.240%	
32) Benzene-d6	8.276	84		1175348	22.862	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	91.440%	
36) 1,2-Dichloropropane-d6	9.270	67		387770	23.666	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	94.680%	
41) Toluene-d8	10.324	98		979579	21.571	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	86.280%	
43) trans-1,3-Dichloroprop...	10.580	79		146072	22.117	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	88.480%	
47) 2-Hexanone-d5	10.922	63		141769	51.737	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	103.480%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		288367	22.793	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	91.160%	
66) 1,2-Dichlorobenzene-d4	13.848	152		253584	20.860	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	83.440%	
Target Compounds							
						Qvalue	
13) Acetone	4.124	43		33088	10.115	ug/L	99
14) Carbon disulfide	4.386	76		40194	1.031	ug/L #	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
Data File : VW026483.D
Acq On : 30 Jun 2023 19:30
Operator : SY/MD
Sample : 03504-02
Misc : 4.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46S2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 01 01:26:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 30 23:38:58 2023
Response via : Initial Calibration

