




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026485.D
 Acq On : 30 Jun 2023 20:18
 Operator : SY/MD
 Sample : 03444-14
 Misc : 4.49g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46T8

Manual IntegrationsAPPROVED

Quant Time: Jun 30 23:45:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

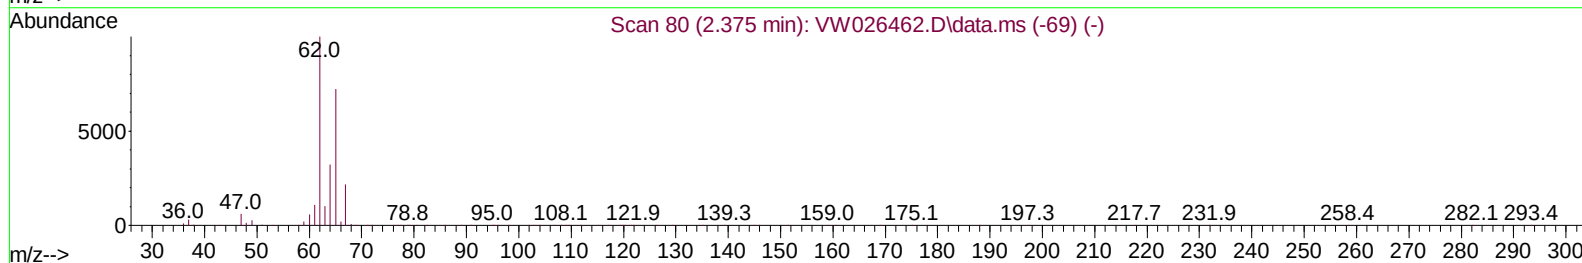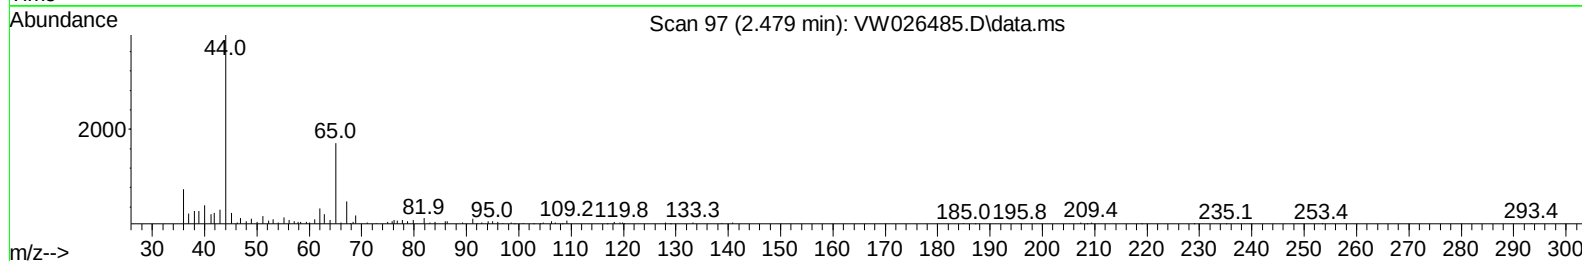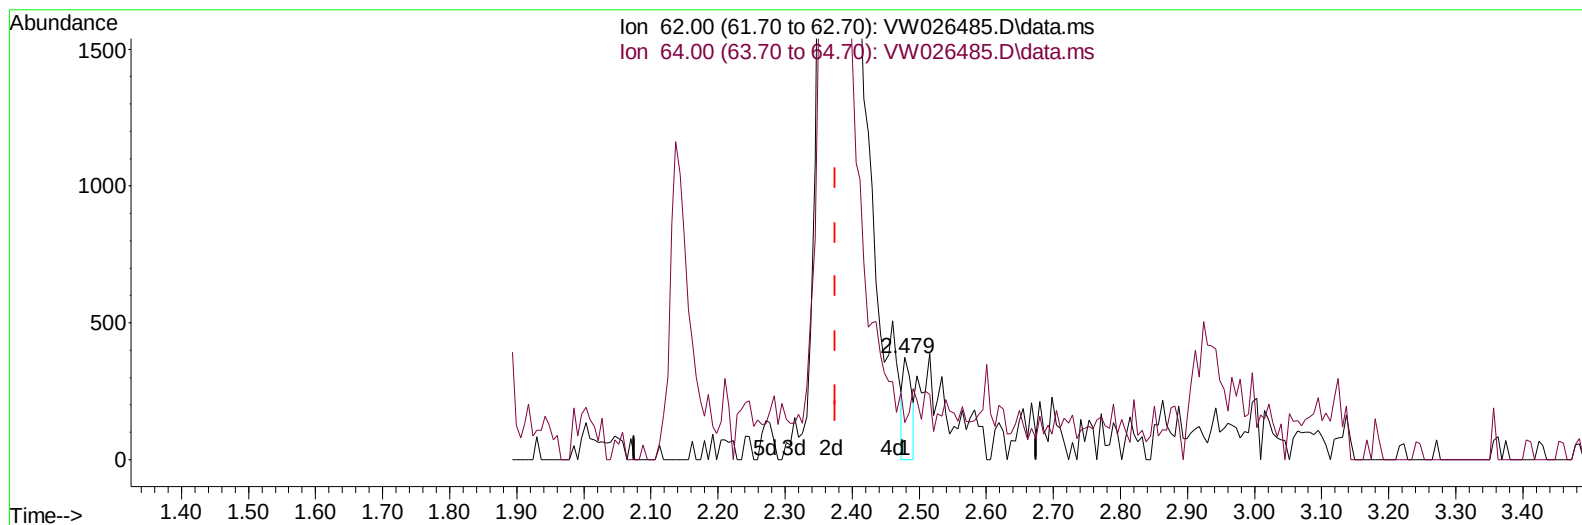

TIC: VW026485.D\data.ms

(5) Vinyl chloride (T)

2.479min (+ 0.104) 0.02 ug/L

response 325

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	32.90	36.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026485.D
 Acq On : 30 Jun 2023 20:18
 Operator : SY/MD
 Sample : 03444-14
 Misc : 4.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46T8

Manual IntegrationsAPPROVED

Quant Time: Jun 30 23:45:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

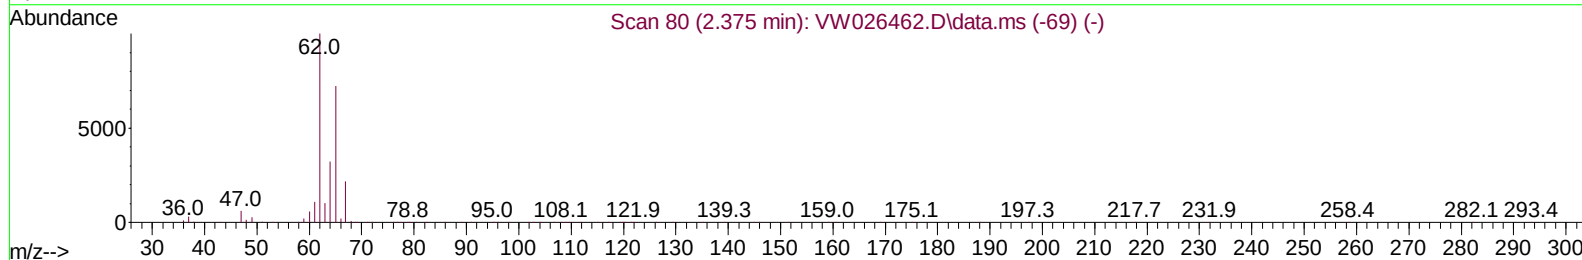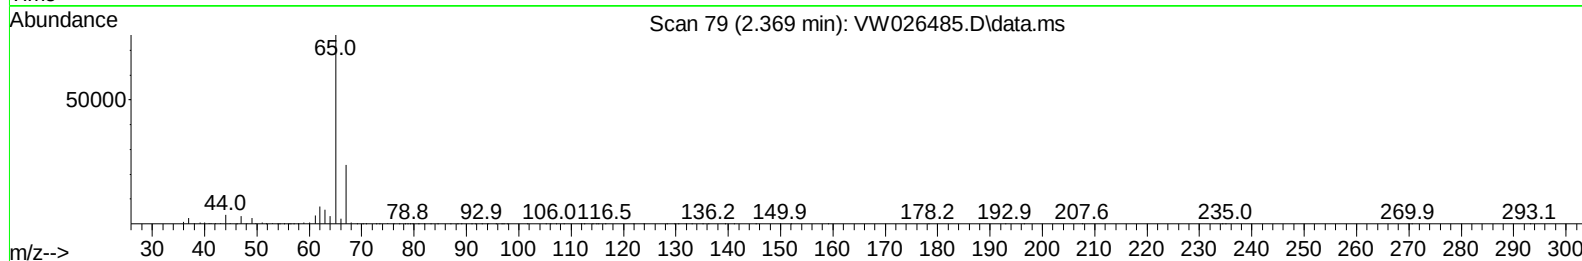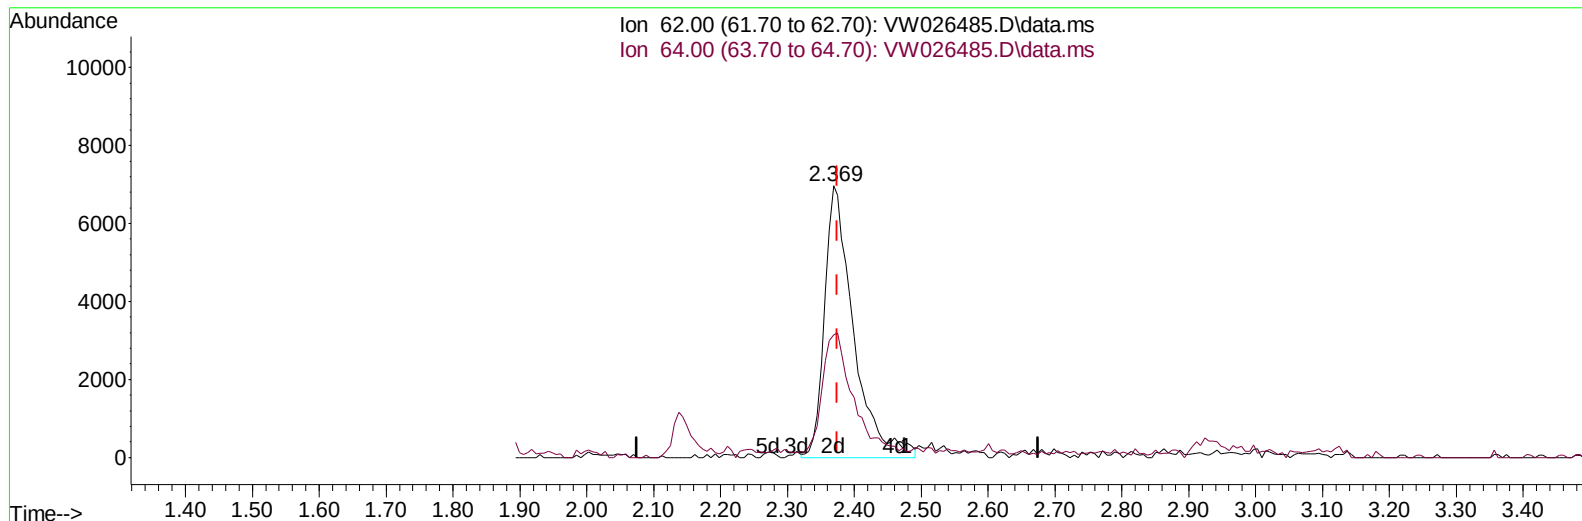

TIC: VW026485.D\data.ms

(5) Vinyl chloride (T)

2.369min (-0.006) 1.17 ug/L m

response 20915

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	32.90	45.18#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
 Data File : VW026485.D
 Acq On : 30 Jun 2023 20:18
 Operator : SY/MD
 Sample : 03444-14
 Misc : 4.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46T8

Manual IntegrationsAPPROVED

Quant Time: Jun 30 23:45:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 30 23:38:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		1261803	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		1075005	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		489741	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		242948	16.910	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	67.640%	
7) Chloroethane-d5	2.893	69		201777	17.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	69.000%	
11) 1,1-Dichloroethene-d2	4.021	65		132018	18.365	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	73.480%	
21) 2-Butanone-d5	7.075	46		218343	40.214	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	80.420%	
24) Chloroform-d	7.648	84		605058	19.673	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	78.680%	
26) 1,2-Dichloroethane-d4	8.307	65		345049	20.525	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	82.120%	
32) Benzene-d6	8.270	84		1277488	20.433	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	81.720%	
36) 1,2-Dichloropropane-d6	9.270	67		417233	20.939	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	83.760%	
41) Toluene-d8	10.319	98		1115563	20.200	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	80.800%	
43) trans-1,3-Dichloroprop...	10.575	79		157987	19.670	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	78.680%	
47) 2-Hexanone-d5	10.922	63		146701	44.023	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	88.040%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		332710	21.625	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	86.480%	
66) 1,2-Dichlorobenzene-d4	13.849	152		342217	20.068	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	80.280%	
Target Compounds							
5) vinyl chloride	2.369	62		20915m	1.169	ug/L	
13) Acetone	4.125	43		14545	3.792	ug/L	97
20) cis-1,2-Dichloroethene	7.167	96		105464	6.126	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063023\
Data File : VW026485.D
Acq On : 30 Jun 2023 20:18
Operator : SY/MD
Sample : 03444-14
Misc : 4.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46T8

Manual IntegrationsAPPROVED

Quant Time: Jun 30 23:45:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062923SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 30 23:38:58 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

